
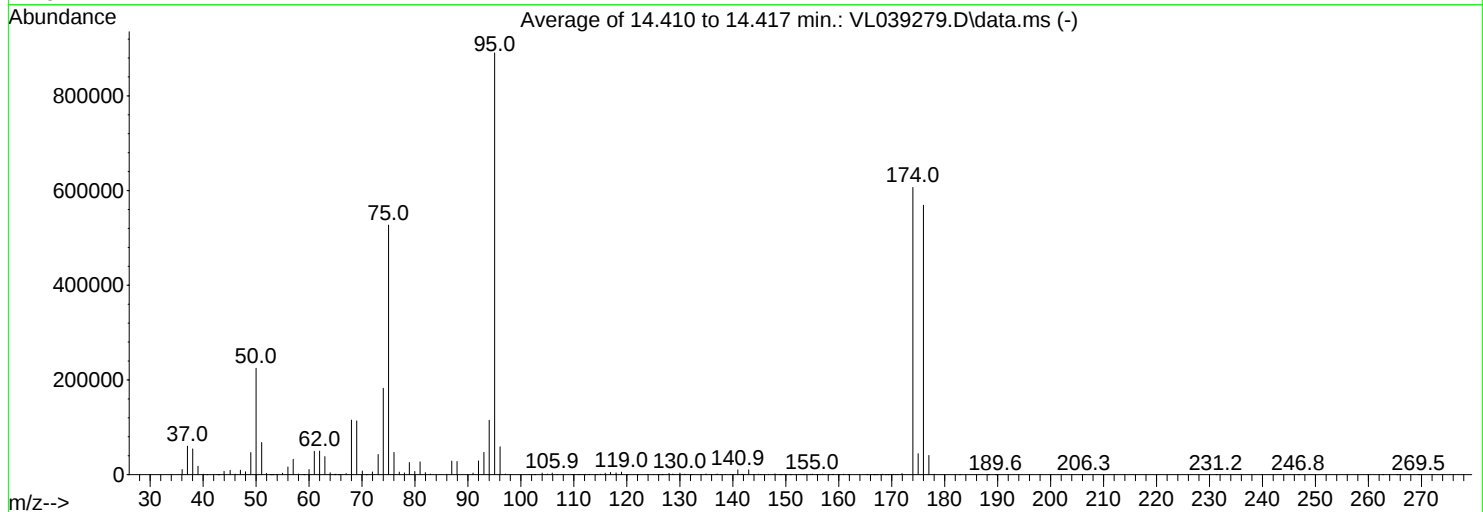


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061422\
 Data File : VL039279.D
 Acq On : 14 Jun 2022 12:39
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun 01 01:22:18 2022
 Last Update : Wed Jun 01 01:22:18 2022

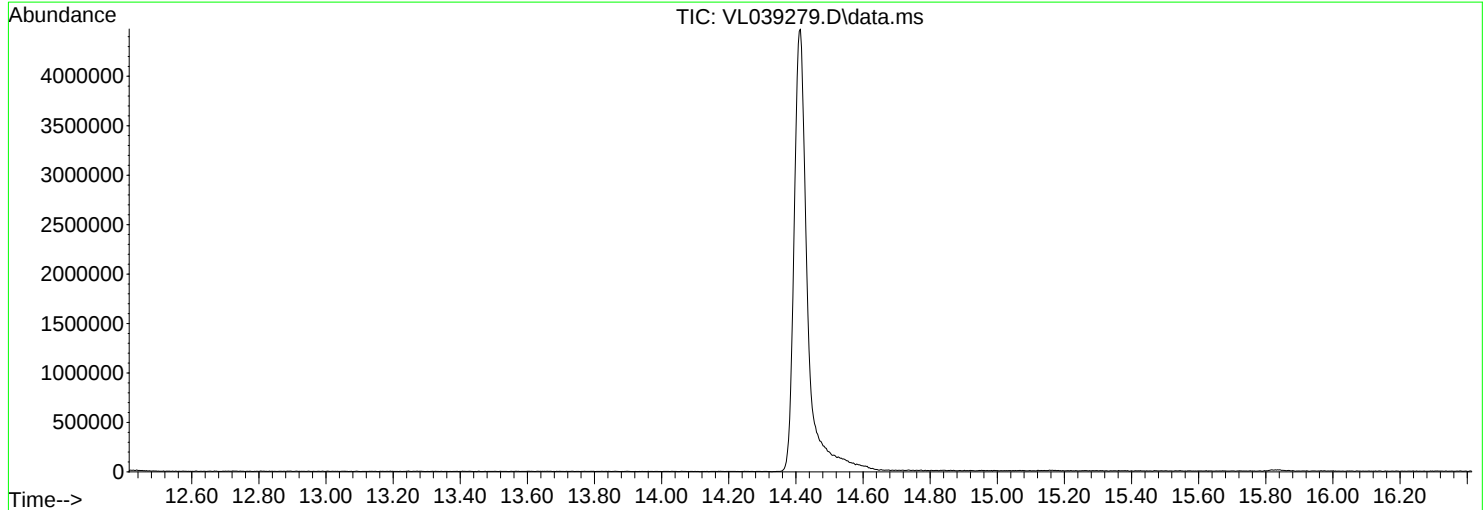

AutoFind: Scans 3615, 3616, 3617; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.2	224858	PASS
75	95	30	66	59.2	527253	PASS
95	95	100	100	100.0	890859	PASS
96	95	5	9	6.6	58821	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.1	606656	PASS
175	174	4	9	7.3	44461	PASS
176	174	93	101	93.8	569088	PASS
177	176	5	9	7.1	40520	PASS

Average of 14.410 to 14.417 min.: VL039279.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	10749	46.10	892	55.00	3173	65.05	981
37.05	60173	47.05	9347	56.00	16079	65.60	71
38.05	54331	48.00	6124	57.00	32424	67.00	243
39.05	18091	49.00	46667	58.00	1455	68.00	11521
40.05	1137	50.00	224858	59.00	154	69.00	113453
40.70	78	51.05	68093	60.00	10959	70.05	7807
42.60	240	51.95	2646	61.00	49379	70.80	142
42.80	82	52.70	157	62.00	49843	71.95	5632
43.00	102	52.90	61	63.00	38096	73.05	42499
43.95	7037	53.20	128	64.00	3968	74.00	182421
45.10	9133	53.85	320	64.80	119	75.00	527253

Average of 14.410 to 14.417 min.: VL039279.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.05	46872	90.95	3541	105.05	1350	114.50	238
77.05	5487	92.00	28949	105.90	3568	115.05	1145
78.00	3599	93.00	46901	106.85	812	115.90	3088
78.95	25760	94.00	115056	109.70	279	116.90	4921
79.95	6853	95.05	890859	110.05	424	117.95	3740
80.95	27109	96.05	58821	110.80	685	119.00	5415
81.95	4305	97.05	1490	111.10	202	120.00	128
82.95	1518	102.60	89	111.70	389	122.00	97
86.00	909	102.75	544	112.20	568	123.85	571
86.95	28896	104.00	3503	112.90	796	125.00	387
87.95	27616	104.70	449	114.00	57	125.80	304

Average of 14.410 to 14.417 min.: VL039279.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.20	213	135.90	229	143.95	744	150.90	173
126.60	121	136.80	548	144.80	1201	151.95	344
126.90	222	137.05	1231	145.20	208	152.70	280
127.95	2704	137.65	273	145.70	433	152.95	305
128.70	1288	138.65	382	146.00	519	153.40	75
128.90	417	139.60	740	146.75	821	153.95	594
130.00	3260	140.10	399	147.95	1719	154.70	567
130.95	1186	140.95	10287	148.75	411	155.00	1389
132.10	155	141.75	1047	149.00	142	155.85	287
134.05	436	142.10	308	149.80	590	156.05	337
134.95	1613	143.00	10069	150.10	289	156.60	512

Average of 14.410 to 14.417 min.: VL039279.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.95	1022	167.20	52	171.95	2304	231.20	81
158.10	74	167.90	90	174.00	606656	246.75	172
158.80	804	168.30	696	175.00	44461	259.90	55
159.00	751	168.80	131	176.00	569088	262.70	72
160.00	63	169.10	382	177.00	40520	265.40	73
160.95	1066	169.30	76	177.80	436	269.50	74
161.80	64	169.70	445	178.05	908		
165.30	60	170.30	698	182.80	53		
166.25	240	170.70	192	188.20	75		
166.60	62	171.00	294	189.60	186		
166.80	52	171.20	364	206.30	299		