


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL061521\
 Data File : VL037153.D
 Acq On : 15 Jun 2021 8:47
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL061421AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Mon Jun 14 16:49:11 2021
 Last Update : Mon Jun 14 16:49:11 2021

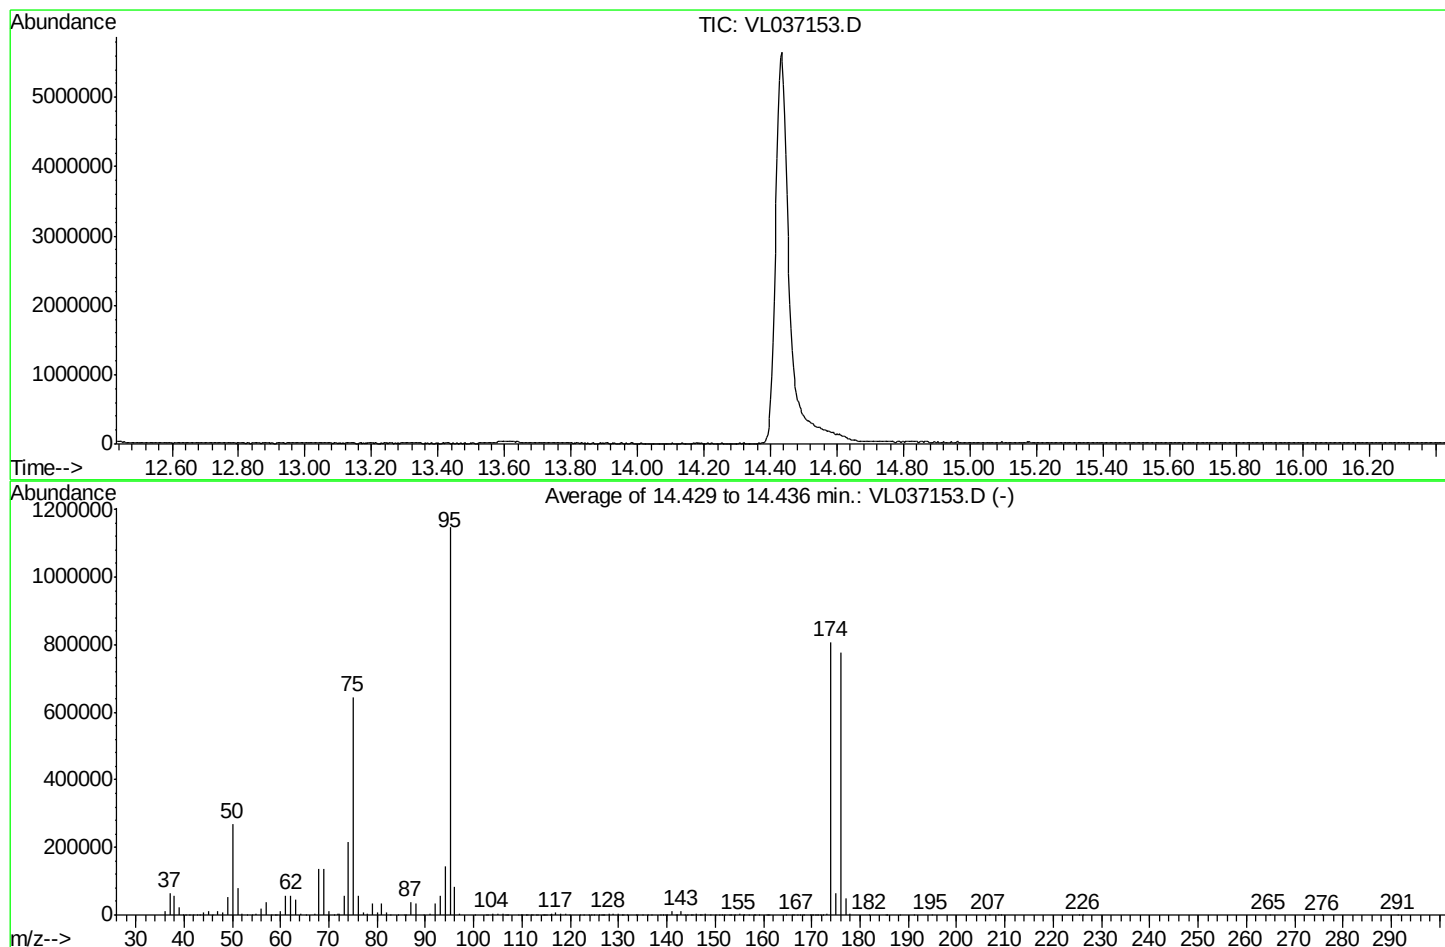

AutoFind: Scans 3621, 3622, 3623; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.6	270784	PASS
75	95	30	66	56.3	645888	PASS
95	95	100	100	100.0	1147221	PASS
96	95	5	9	7.3	83189	PASS
173	174	0.00	2	0.4	2856	PASS
174	95	50	120	70.5	808554	PASS
175	174	4	9	7.8	63008	PASS
176	174	93	101	96.2	777813	PASS
177	176	5	9	6.5	50381	PASS