

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061523\
 Data File : VL040467.D
 Acq On : 15 Jun 2023 14:37
 Operator : SY/MD
 Sample : QC053023 CAN 10294
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC053023 CAN 10294

Quant Time: Jun 16 05:36:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue Jun 06 06:22:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.198	49	1032129	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.664	114	2629829	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.484	117	2209947	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.796	95	1821192	9.985	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.800%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061523\
Data File : VL040467.D
Acq On : 15 Jun 2023 14:37
Operator : SY/MD
Sample : QC053023 CAN 10294
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC053023 CAN 10294

Quant Time: Jun 16 05:36:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Tue Jun 06 06:22:12 2023
Response via : Initial Calibration




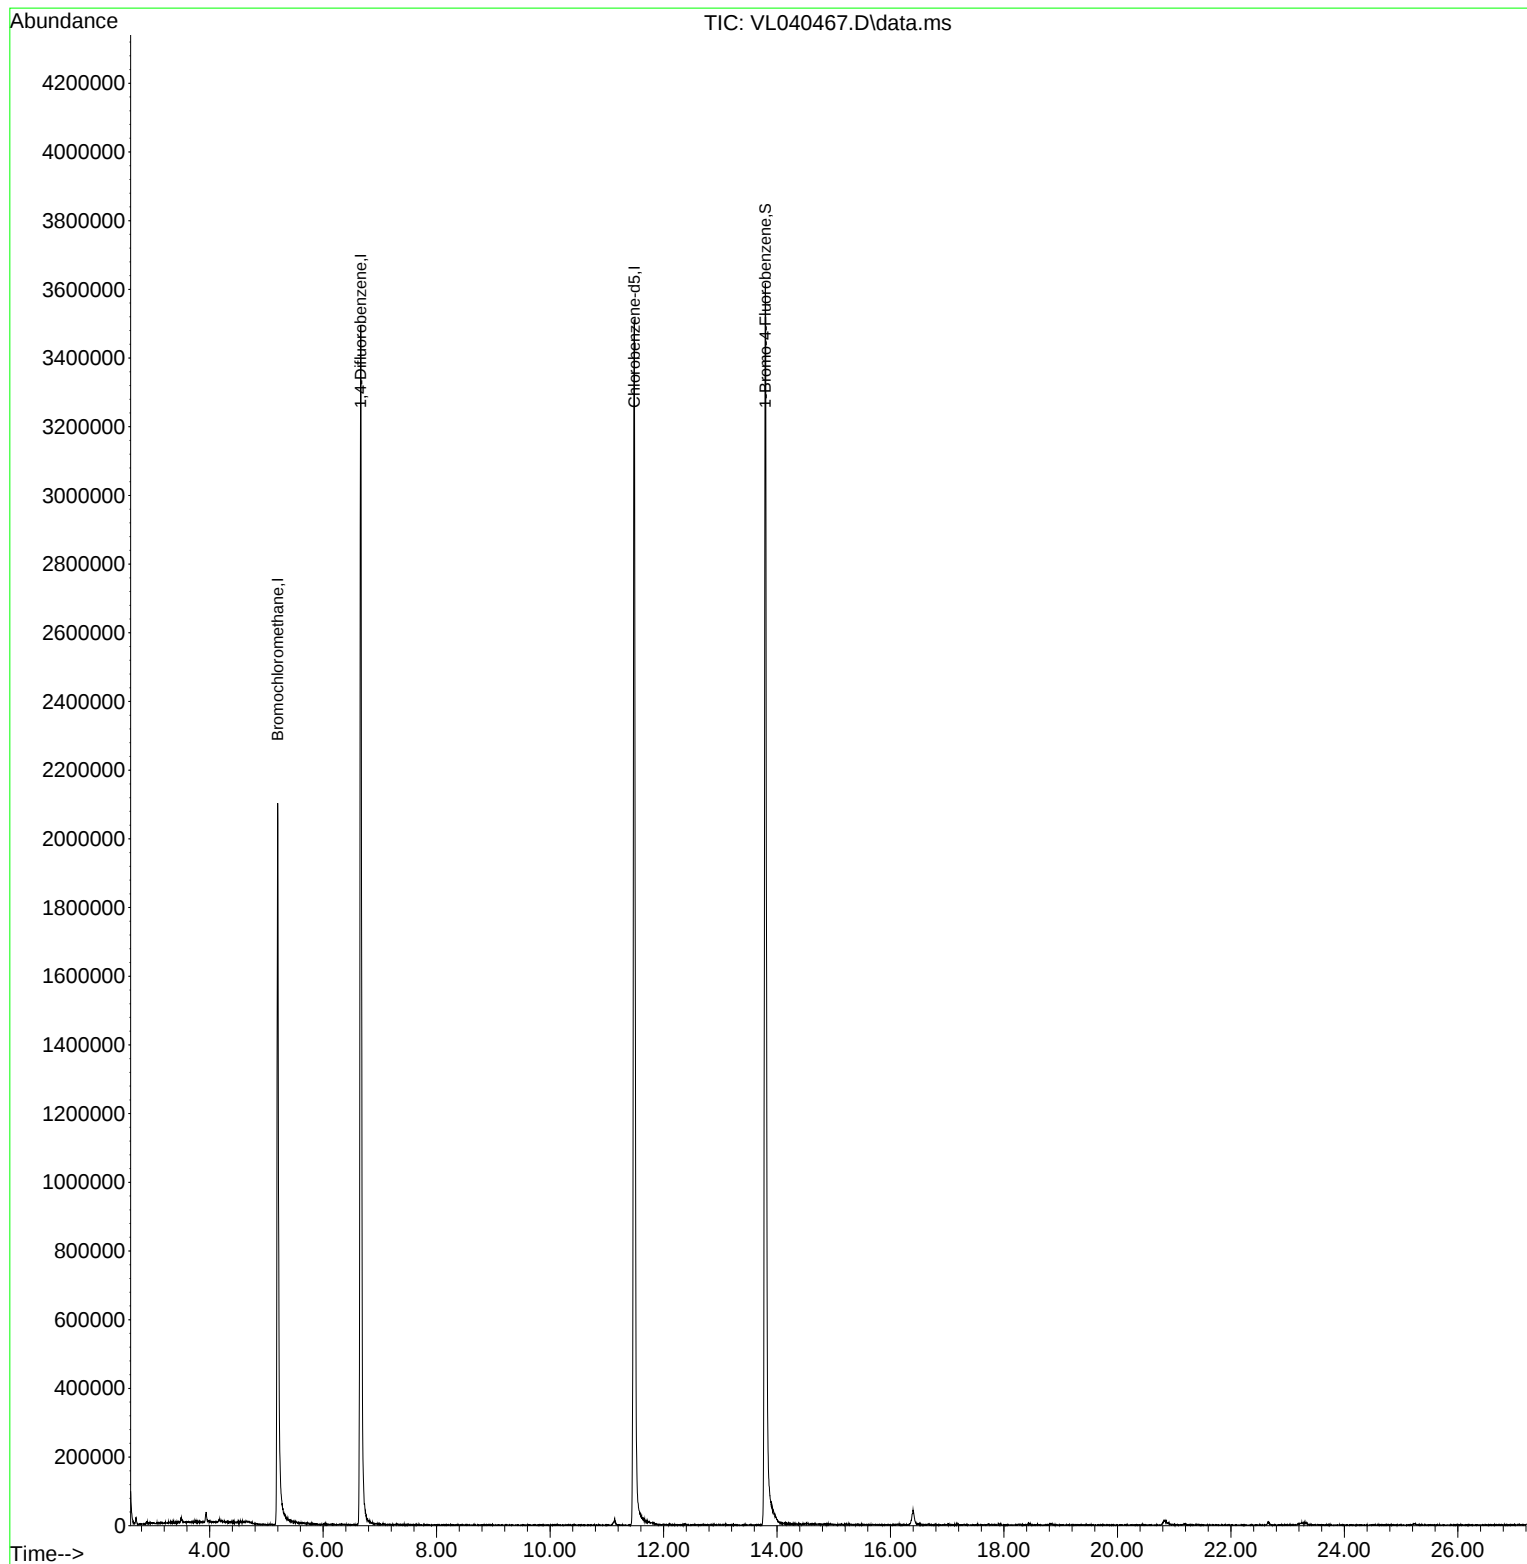


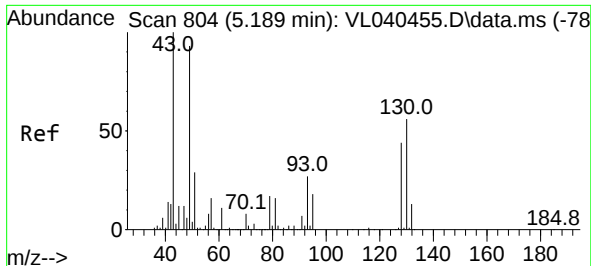

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.198 min Scan# 804
Delta R.T. 0.009 min
Lab File: VL040467.D
Acq: 15 Jun 2023 14:37




Instrument :
MSVOA_1
ClientSampleId :
QC053023 CAN 10294


Tgt Ion: 49 Resp: 1032129
Ion Ratio Lower Upper
49 100
128 50.1 24.7 74.1
130 63.5 31.4 94.2

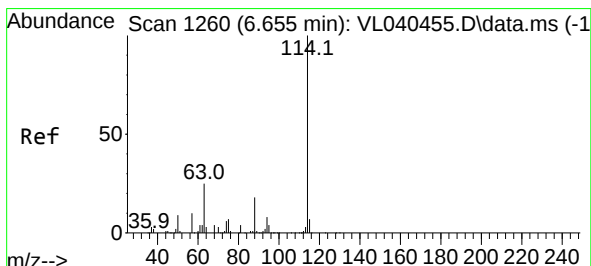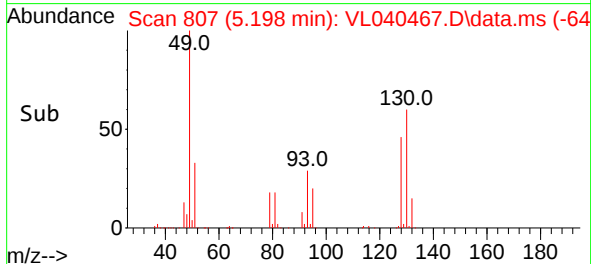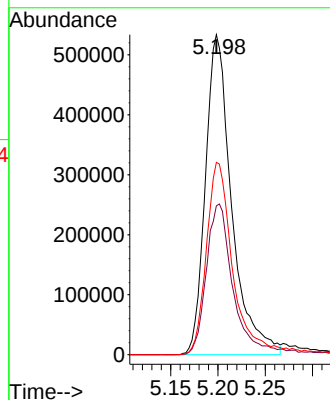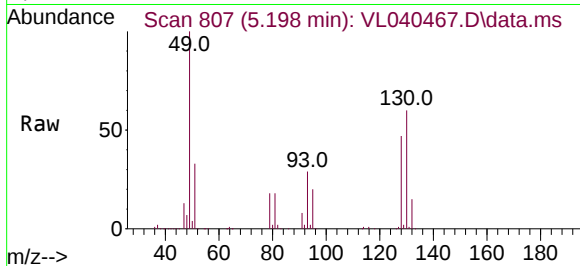

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.664 min Scan# 1263
Delta R.T. 0.010 min
Lab File: VL040467.D
Acq: 15 Jun 2023 14:37

Tgt Ion: 114 Resp: 2629829
Ion Ratio Lower Upper
114 100
63 26.0 21.0 31.6
88 18.0 14.5 21.7


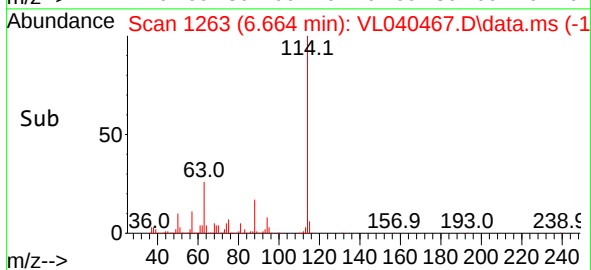
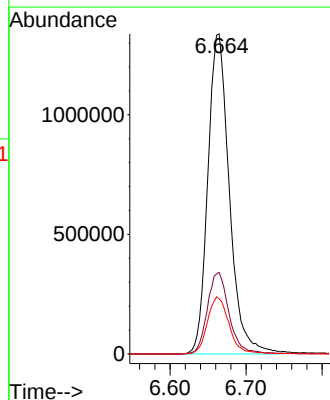
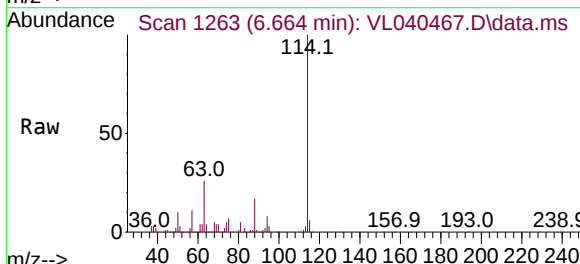


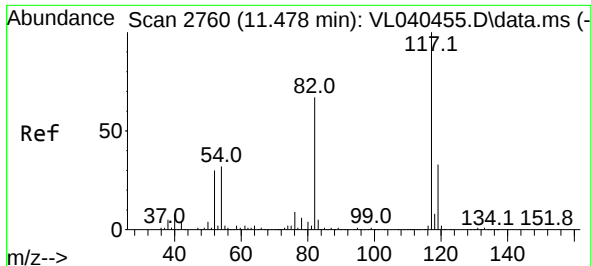

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.484 min Scan# 21
Delta R.T. 0.006 min
Lab File: VL040467.D
Acq: 15 Jun 2023 14:37

Instrument :
MSVOA_1
ClientSampleId :
QC053023 CAN 10294

Tgt Ion:117 Resp: 2209947
Ion Ratio Lower Upper
117 100
82 68.7 53.0 79.4
119 33.1 24.4 36.6

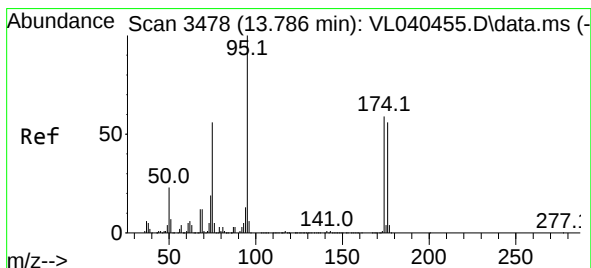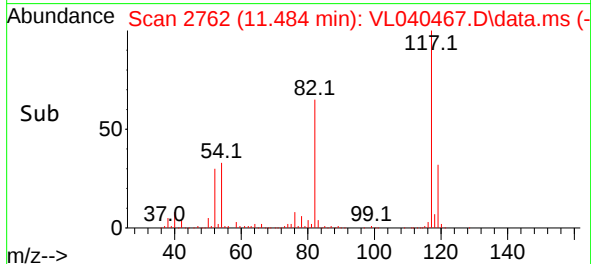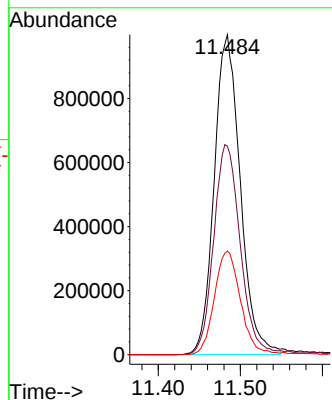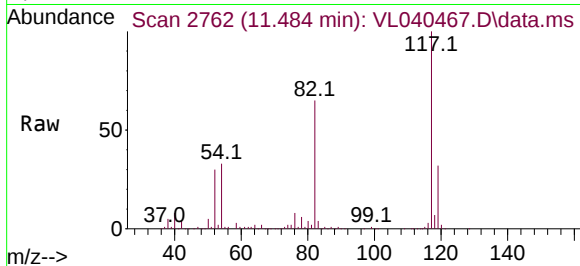

#68
1-Bromo-4-Fluorobenzene
Concen: 9.985 ppbv
RT: 13.796 min Scan# 3481
Delta R.T. 0.010 min
Lab File: VL040467.D
Acq: 15 Jun 2023 14:37

Tgt Ion: 95 Resp: 1821192
Ion Ratio Lower Upper
95 100
174 59.8 47.7 71.5
175 4.2 3.5 5.3

