
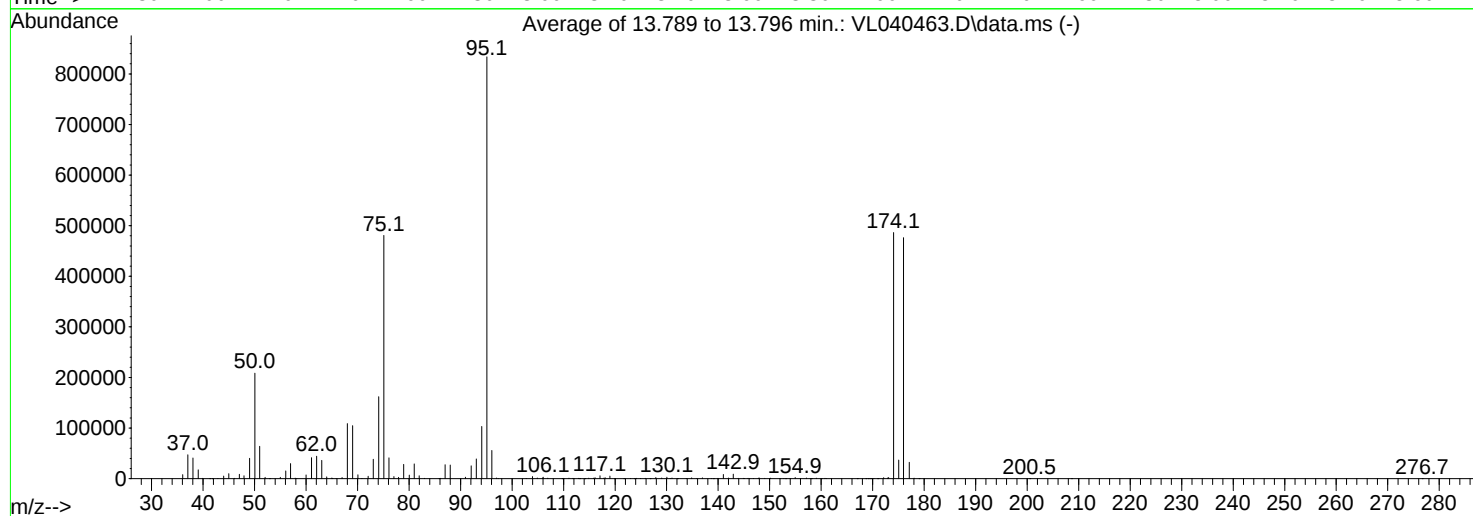


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061523\
 Data File : VL040463.D
 Acq On : 15 Jun 2023 11:04
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL060523AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Tue Jun 06 06:22:12 2023

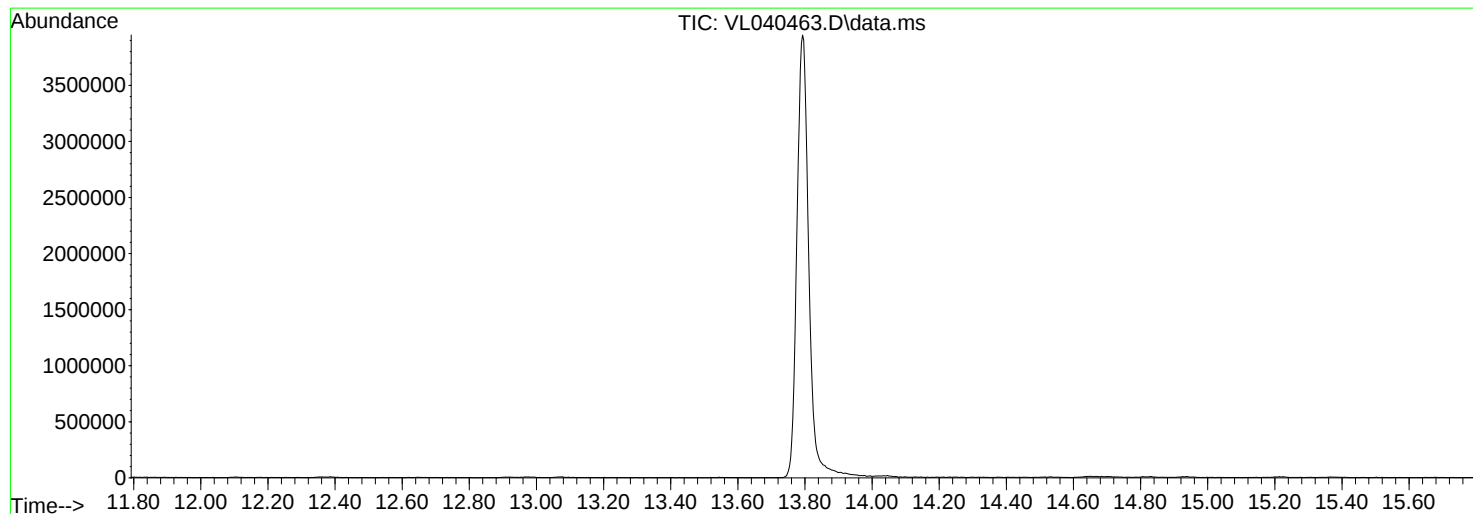

AutoFind: Scans 3479, 3480, 3481; Background Corrected with Scan 3456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.0	208363	PASS
75	95	30	66	57.7	480704	PASS
95	95	100	100	100.0	833792	PASS
96	95	5	9	6.7	55808	PASS
173	174	0.00	2	0.5	2357	PASS
174	95	50	120	58.3	486357	PASS
175	174	4	9	7.5	36557	PASS
176	174	93	101	97.9	476267	PASS
177	176	5	9	6.8	32355	PASS

Average of 13.789 to 13.796 min.: VL040463.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	7857	47.05	8442	58.20	315	69.05	10480
37.05	47008	47.95	5877	60.00	7436	70.05	7531
38.05	40949	49.05	40160	61.05	41477	70.85	191
39.05	17567	50.05	208363	62.05	44419	72.05	481
39.90	807	51.00	63816	63.05	36085	73.05	38269
41.30	70	52.05	2617	64.00	3584	74.10	161792
41.80	96	52.90	84	65.00	1178	75.10	480704
42.90	387	55.00	2571	65.20	701	76.10	41288
44.00	5214	56.05	15125	65.85	240	77.05	4278
45.00	9944	57.00	29811	67.00	2254	77.95	2676
46.10	530	57.90	981	68.00	108811	78.95	28045

Average of 13.789 to 13.796 min.: VL040463.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.05	6992	94.10	103035	109.70	103	117.05	5834
81.00	29219	95.10	833792	110.05	546	117.80	849
81.95	5823	96.05	55808	111.05	928	118.05	2015
83.00	750	97.00	1335	111.80	515	119.00	5038
85.80	147	97.30	320	112.00	415	119.90	70
86.05	566	102.75	466	112.90	693	121.70	134
87.00	27701	103.95	4238	113.10	101	123.00	501
88.00	26816	104.90	1361	114.10	81	123.70	182
90.95	2869	105.90	1284	114.90	1038	124.15	606
92.05	25317	106.05	2799	115.80	970	124.95	270
93.05	38963	106.95	923	116.10	1914	125.85	577

Average of 13.789 to 13.796 min.: VL040463.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.80	107	138.75	265	146.85	442	157.15	1379
127.90	2300	139.10	129	147.80	441	157.90	281
129.05	1436	139.95	564	147.95	1700	158.10	72
130.05	2800	141.00	8274	149.05	672	159.05	983
130.70	344	142.05	1271	150.15	976	160.00	58
131.05	1208	142.95	8975	152.00	385	160.75	612
132.10	102	143.90	676	152.75	244	161.00	385
133.80	192	144.90	674	153.10	167	167.00	137
134.85	1521	145.10	247	154.00	490	168.70	141
135.85	344	145.80	725	154.95	2131	169.15	138
136.95	1565	146.10	345	156.00	193	169.60	171

Average of 13.789 to 13.796 min.: VL040463.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.25	352	179.00	63				
170.95	190	200.50	63				
171.20	254	208.60	51				
172.15	1976	276.70	60				
172.90	1177						
173.10	2357						
174.05	486357						
175.05	36557						
176.00	476267						
177.10	32355						
178.05	1100						