


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL061721\
 Data File : VL037194.D
 Acq On : 17 Jun 2021 8:41
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL061621AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Jun 16 14:06:32 2021
 Last Update : Wed Jun 16 14:06:32 2021

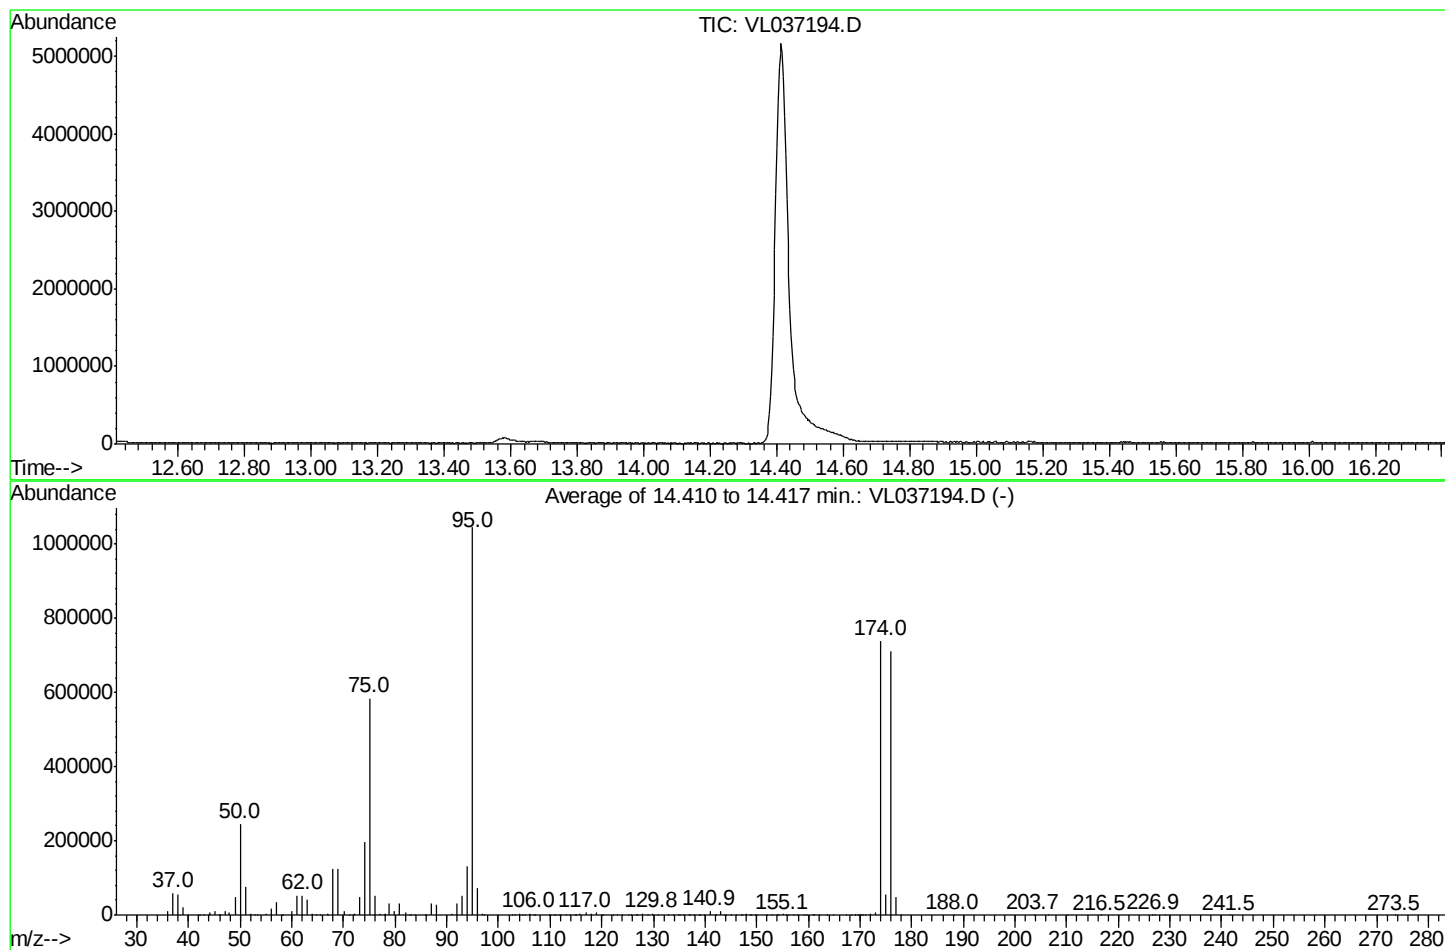

AutoFind: Scans 3615, 3616, 3617; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.5	246165	PASS
75	95	30	66	55.9	583914	PASS
95	95	100	100	100.0	1045333	PASS
96	95	5	9	6.8	71530	PASS
173	174	0.00	2	0.7	5497	PASS
174	95	50	120	70.7	739242	PASS
175	174	4	9	7.6	56512	PASS
176	174	93	101	96.2	711232	PASS
177	176	5	9	6.8	48653	PASS