


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL061920\
 Data File : VL035094.D
 Acq On : 19 Jun 2020 14:35
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL061920AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Sat Jun 20 02:10:36 2020
 Last Update : Sat Jun 20 02:10:36 2020

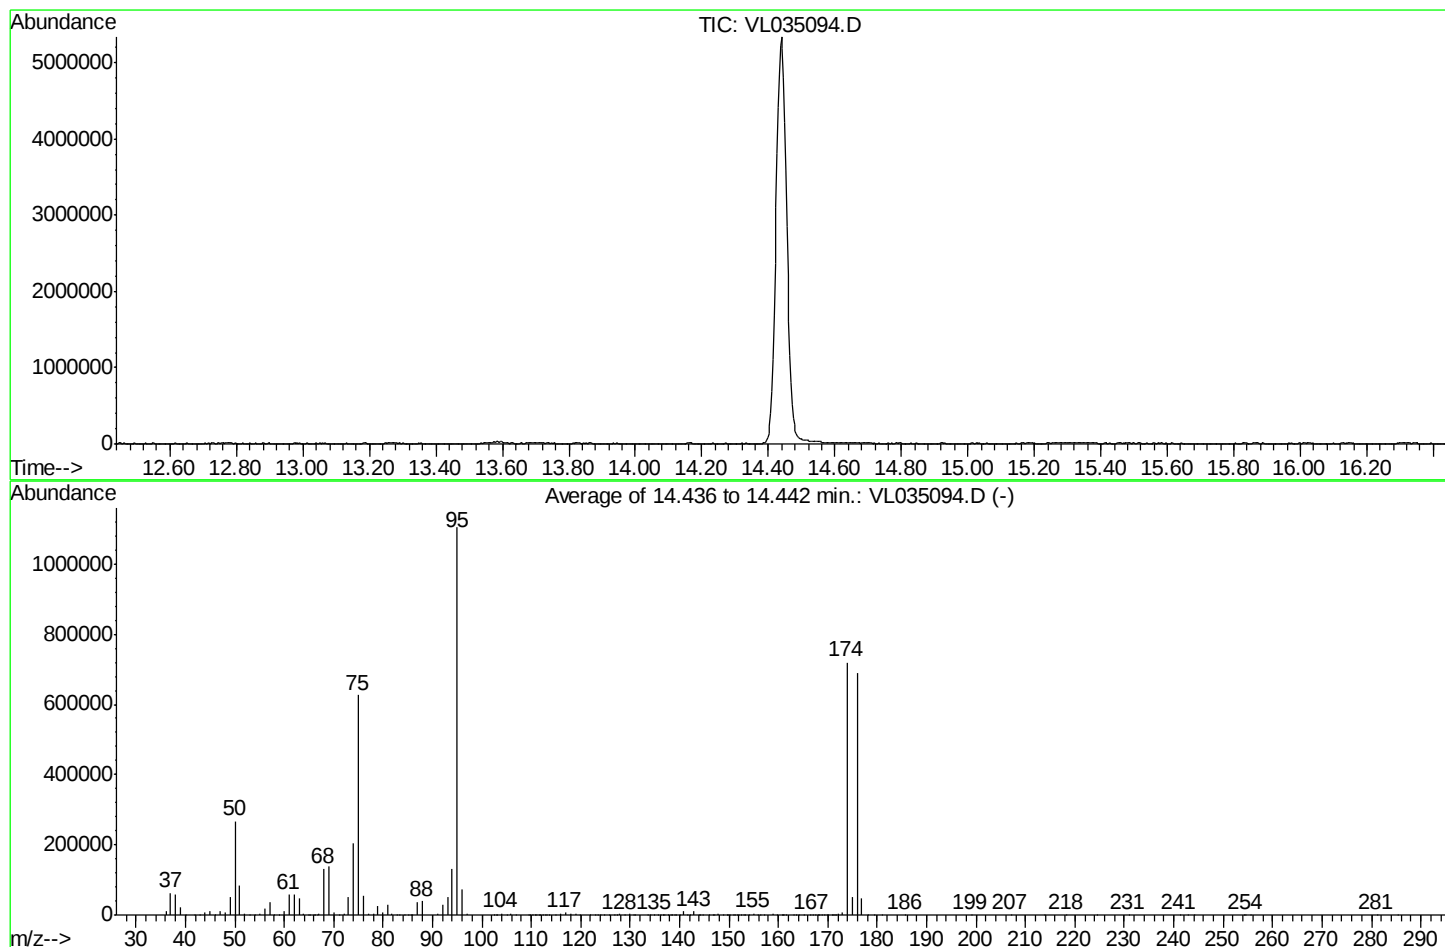

AutoFind: Scans 3623, 3624, 3625; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.3	267989	PASS
75	95	30	66	56.8	627285	PASS
95	95	100	100	100.0	1104554	PASS
96	95	5	9	6.7	73818	PASS
173	174	0.00	2	0.8	5636	PASS
174	95	50	120	65.1	718762	PASS
175	174	4	9	6.9	49677	PASS
176	174	93	101	96.0	690368	PASS
177	176	5	9	6.9	47520	PASS