


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062220\
 Data File : VL035104.D
 Acq On : 22 Jun 2020 7:45
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL061920AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Sat Jun 20 02:10:36 2020
 Last Update : Sat Jun 20 02:10:36 2020

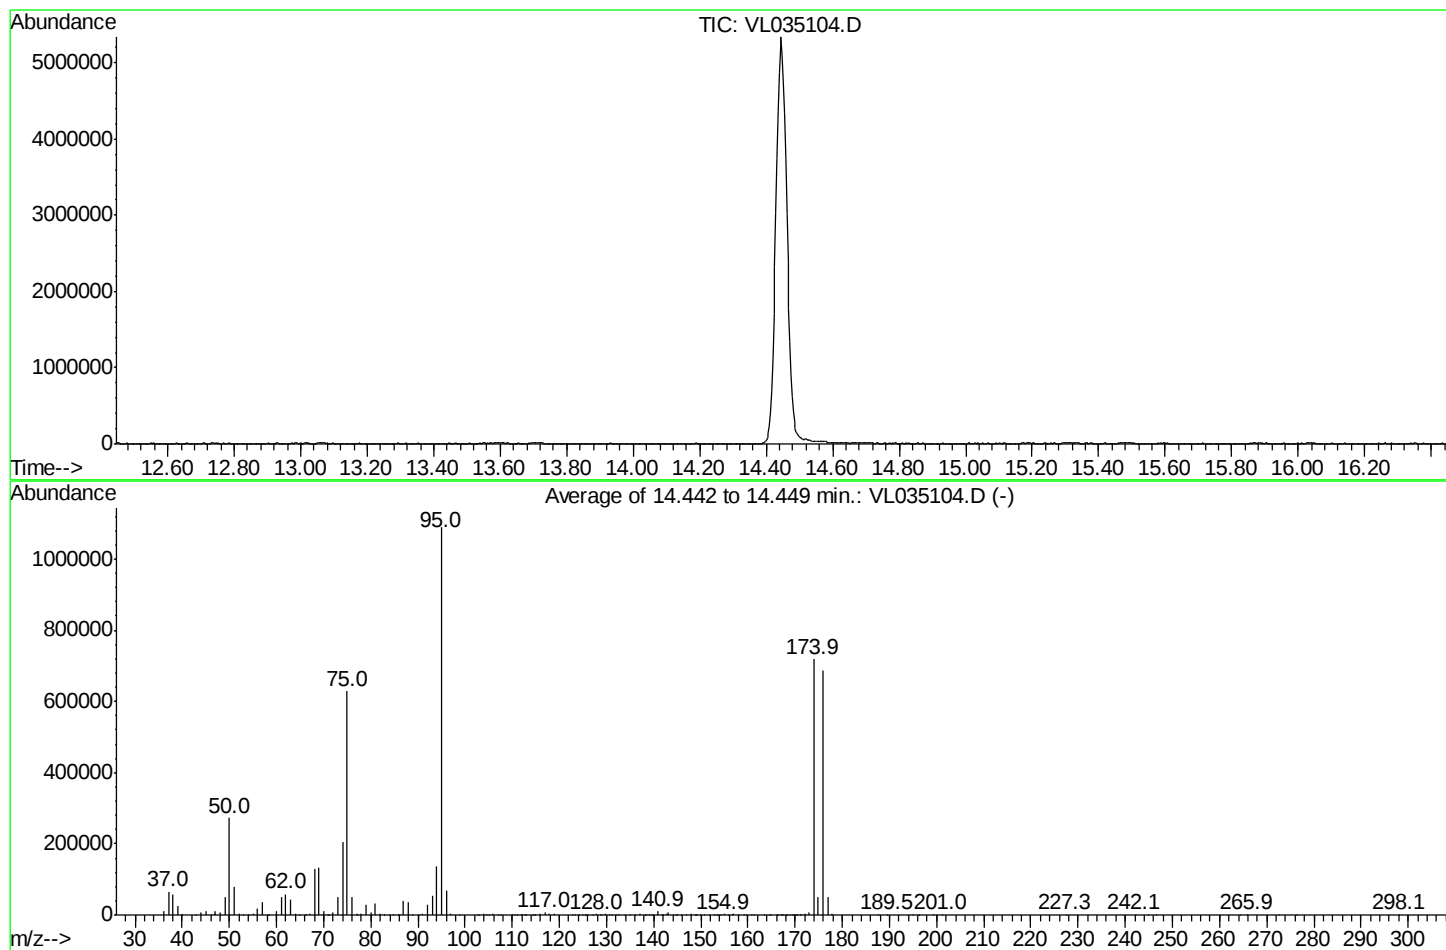

AutoFind: Scans 3625, 3626, 3627; Background Corrected with Scan 3603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.0	272155	PASS
75	95	30	66	57.7	628010	PASS
95	95	100	100	100.0	1088853	PASS
96	95	5	9	6.4	70178	PASS
173	174	0.00	2	0.9	6729	PASS
174	95	50	120	66.0	718634	PASS
175	174	4	9	7.0	50434	PASS
176	174	93	101	95.5	686186	PASS
177	176	5	9	7.3	50090	PASS