

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL062221\
 Data File : VL037223.D
 Acq On : 22 Jun 2021 19:08
 Operator : SY/AP
 Sample : M2807-03
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 IAQ-01

Manual Integrations
 APPROVED

MMDadoda
 6/24/2021 4:32:56 PM

Quant Time: Jun 24 09:19:56 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL061621AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun 1
 QLast Update : Wed Jun 16 14:06:32 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.68	49	1182460	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.19	114	3461185	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.10	117	3309711	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.43	95	2629441	10.48	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	104.80%

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	3.05	85	39189	0.191	ppbv	90
3) Chlorodifluoromethane	3.00	51	54724m	0.238	ppbv	
4) Chloromethane	3.15	50	48905	0.638	ppbv	91
9) Propene	3.03	41	1415175m	19.250	ppbv	
10) Heptane	8.13	43	402109	2.258	ppbv	98
11) Trichlorofluoromethane	3.96	101	51475	0.235	ppbv	92
13) Ethanol	3.61	45	2420173	212.808	ppbv	46
15) Acetone	3.85	43	6283687m	47.124	ppbv	
17) tert-Butyl alcohol	4.31	59	248017	2.012	ppbv	96
19) Isopropyl Alcohol	3.99	45	277453	3.435	ppbv #	1
20) Methylene Chloride	4.36	84	342448	4.290	ppbv	98
26) Hexane	5.70	57	1302305	8.926	ppbv #	62
30) Cyclohexane	7.14	84	210072	1.728	ppbv #	84
34) 2-Butanone	5.26	43	265518	1.973	ppbv	94
35) Carbon Tetrachloride	7.03	117	15751m	0.068	ppbv	
36) Benzene	6.91	78	84544m	0.302	ppbv	
44) 2,2,4-Trimethylpentane	7.88	57	136723	0.290	ppbv #	10
52) Tetrachloroethene	11.24	164	4421m	0.034	ppbv	
53) Toluene	9.82	91	940340	2.813	ppbv	100
58) Ethyl Benzene	12.73	91	580055	1.273	ppbv	96
59) m/p-Xylene	12.98	91	1952490	5.057	ppbv	98
60) o-Xylene	13.71	91	676736	1.841	ppbv	97
61) Styrene	13.55	104	217748m	1.148	ppbv	
62) Isopropylbenzene	14.68	105	80784m	0.155	ppbv	
64) n-propylbenzene	15.58	120	30872	0.236	ppbv	76
65) tert-Butylbenzene	16.78	119	63290	0.136	ppbv #	54
70) n-Butylbenzene	18.57	91	64577m	0.134	ppbv	
72) 4-Ethyltoluene	15.85	105	151819	0.363	ppbv #	90
73) 1,3,5-Trimethylbenzene	16.01	105	192318	0.476	ppbv	95
74) 1,2,4-Trimethylbenzene	16.78	105	565859	1.360	ppbv #	71
79) Naphthalene	22.22	128	54563	0.157	ppbv #	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

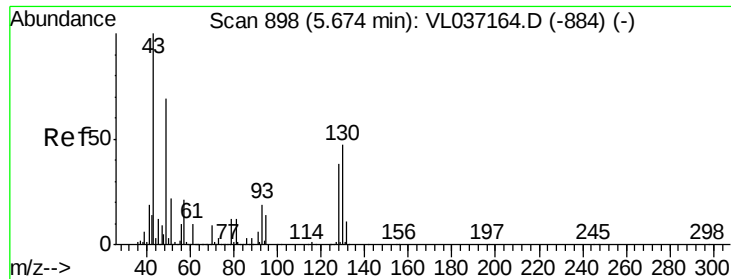

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.68 min Scan# 899

Delta R.T. 0.00 min

Lab File: VL037223.D

Acq: 22 Jun 2021 19:08

Instrument :

MSVOA_L

ClientSampleId :

IAQ-01

Tot Ion: 49 Resp: 1182460

Ion Ratio Lower Upper

49 100


128 55.9 29.3 88.0

130 71.6 35.9 107.8

Manual Integrations
APPROVED

MMDadoda




6/24/2021 4:32:56 PM



Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

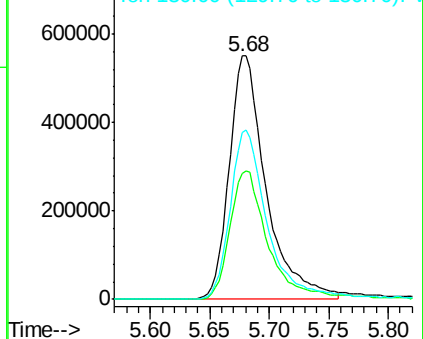

#2

Dichlorodifluoromethane

Concen: 0.191 ppbv

RT: 3.05 min Scan# 83

Delta R.T. 0.00 min

Lab File: VL037223.D


Acq: 22 Jun 2021 19:08

Tgt Ion: 85 Resp: 39189

Ion Ratio Lower Upper



85 100


87 26.5 25.8 38.6



Abundance Ion 85.00 (84.70 to 85.70): VL0

Ion 87.00 (86.70 to 87.70): VL0

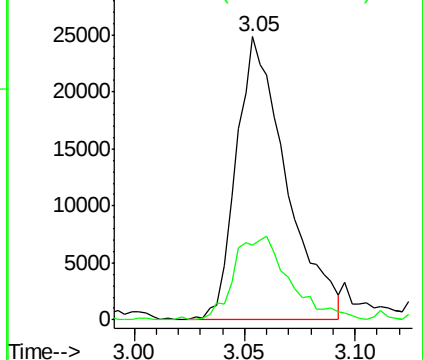

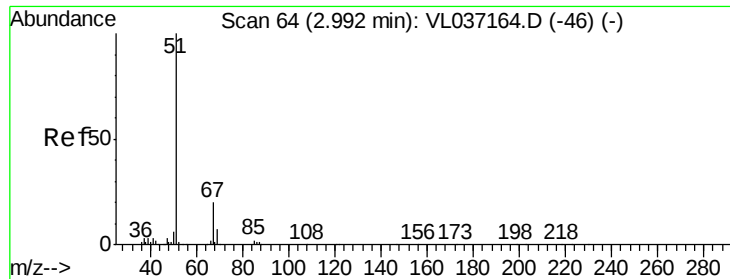

#3

Chlorodifluoromethane

Concen: 0.238 ppbv

RT: 3.00 min Scan# 65

Delta R.T. 0.00 min

Lab File: VL037223.D

Acq: 22 Jun 2021 19:08

Instrument :

MSVOA_L

ClientSampleId :

IAQ-01

Tot Ion: 51 Resp: 54724

Ion Ratio Lower Upper

51 100


67 19.0 15.8 23.6

Manual Integrations

APPROVED




MMDadoda

6/24/2021 4:32:56 PM

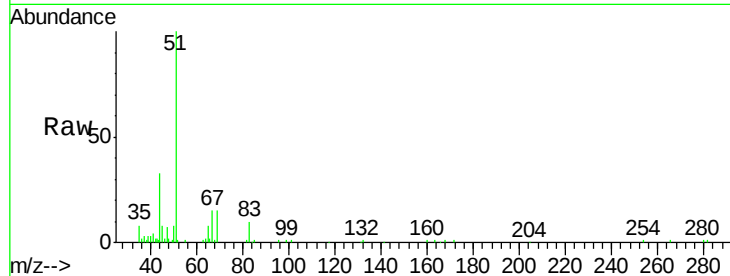

Abundance Ion 51.00 (50.70 to 51.70): VL0

Ion 67.00 (66.70 to 67.70): VL0

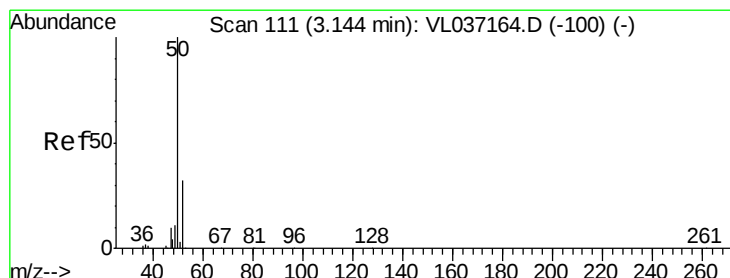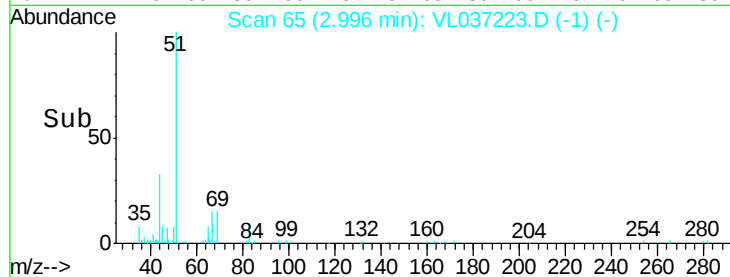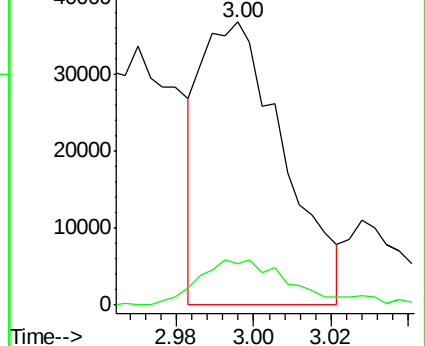

#4

Chloromethane

Concen: 0.638 ppbv

RT: 3.15 min Scan# 112

Delta R.T. 0.00 min

Lab File: VL037223.D


Acq: 22 Jun 2021 19:08

Tgt Ion: 50 Resp: 48905

Ion Ratio Lower Upper



50 100


52 27.1 25.8 38.8

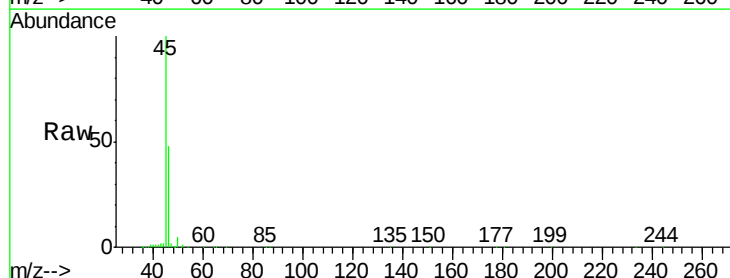

Abundance Ion 50.10 (49.80 to 50.80): VL0

Ion 52.10 (51.80 to 52.80): VL0

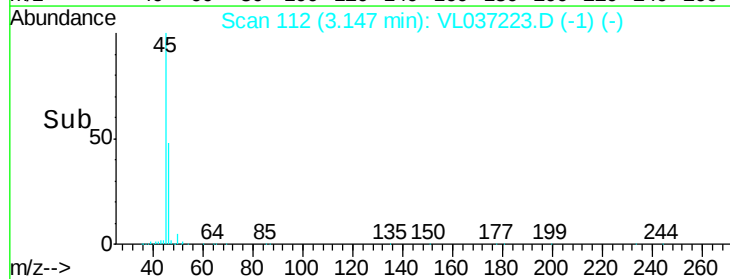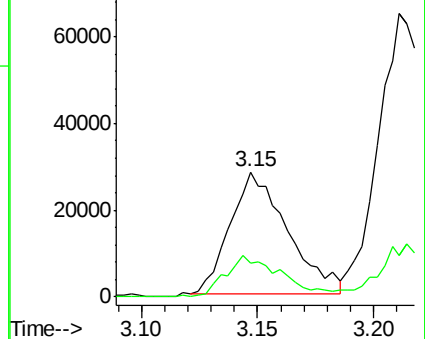

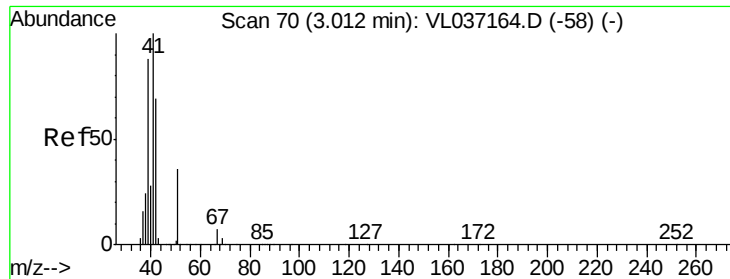

#9

Propene

Concen: 19.250 ppbv m

RT: 3.03 min Scan# 76

Delta R.T. 0.02 min

Lab File: VL037223.D

Acq: 22 Jun 2021 19:08

Instrument :

MSVOA_L

ClientSampleId :

IAQ-01

Tot Ion: 41 Resp: 1415175

Ion Ratio Lower Upper


41 100

42 185.3 54.5 81.7#

Manual Integrations
APPROVED




MMDadoda

6/24/2021 4:32:56 PM

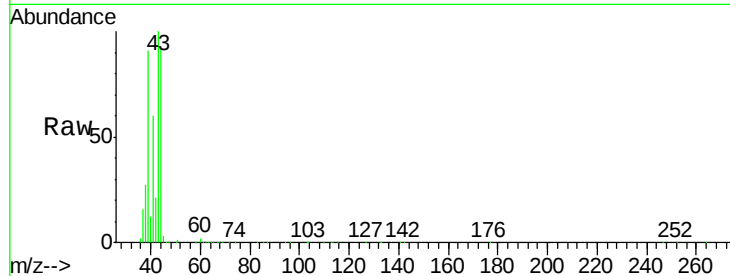

Abundance Ion 41.10 (40.80 to 41.80): VL0

Ion 42.10 (41.80 to 42.80): VL0

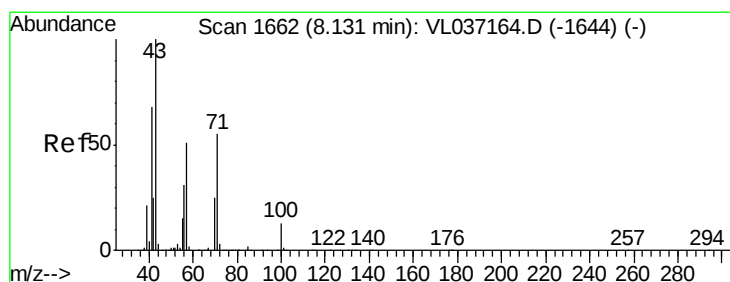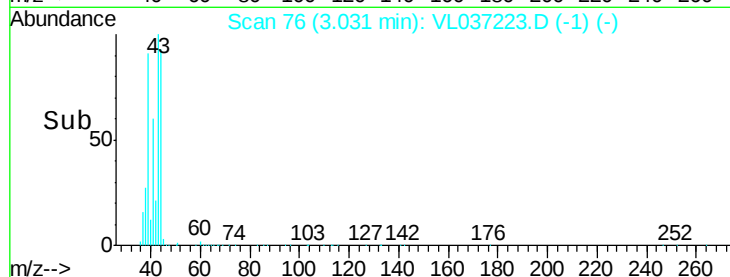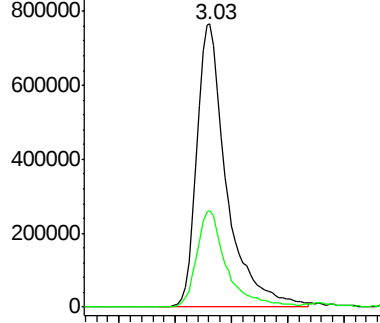

#10

Heptane

Concen: 2.258 ppbv

RT: 8.13 min Scan# 1663

Delta R.T. 0.00 min

Lab File: VL037223.D


Acq: 22 Jun 2021 19:08

Tgt Ion: 43 Resp: 402109

Ion Ratio Lower Upper



43 100


57 49.7 40.6 61.0

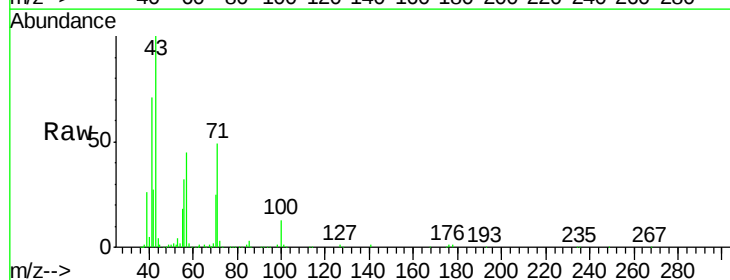

Abundance Ion 43.10 (42.80 to 43.80): VL0

Ion 57.10 (56.80 to 57.80): VL0

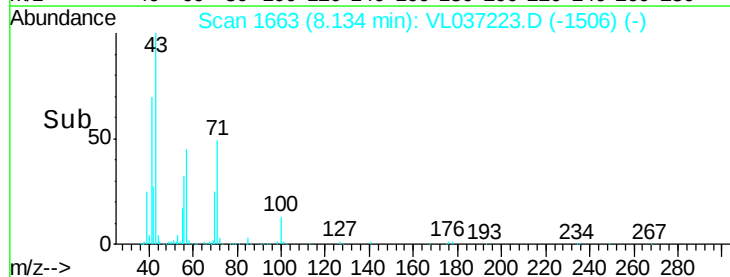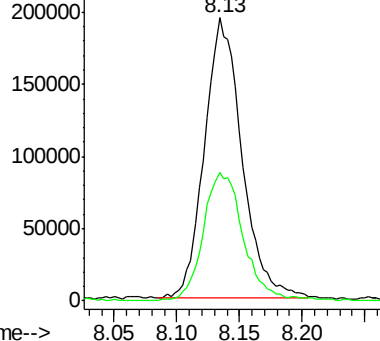

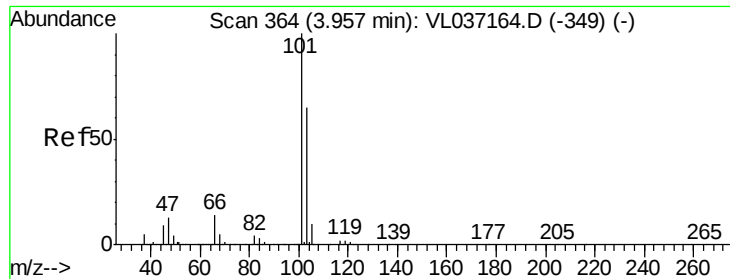





#11
 Trichlorofluoromethane
 Concen: 0.235 ppbv
 RT: 3.96 min Scan# 364
 Delta R.T. 0.00 min
 Lab File: VL037223.D
 Acq: 22 Jun 2021 19:08

Instrument :
 MSVOA_L
 ClientSampleId :
 IAQ-01

Tot Ion	Ratio	Lower	Upper
101	100		
103	59.0	52.2	78.4




Manual Integrations
 APPROVED


MMDadoda
 6/24/2021 4:32:56 PM

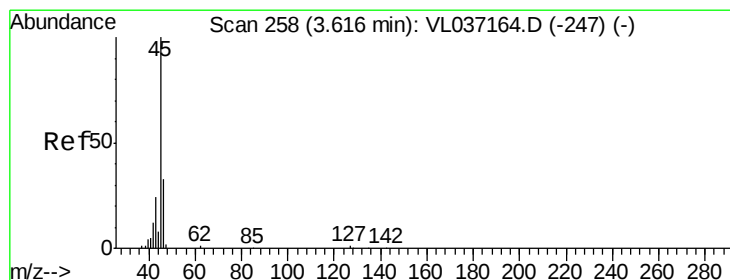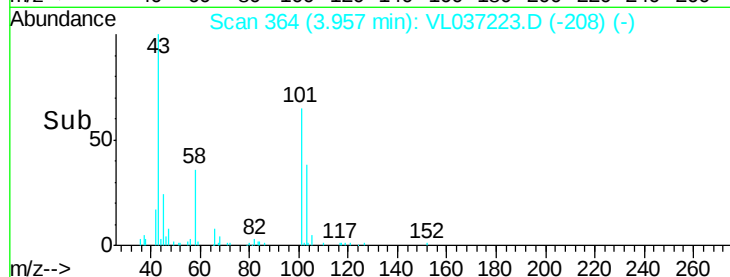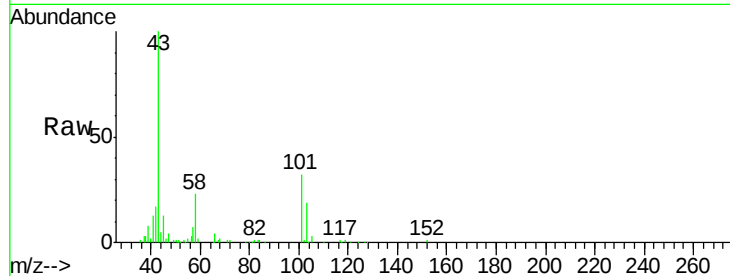

#13
 Ethanol
 Concen: 212.808 ppbv
 RT: 3.61 min Scan# 256
 Delta R.T. -0.01 min
 Lab File: VL037223.D
 Acq: 22 Jun 2021 19:08

Tgt Ion	Ratio	Lower	Upper
45	100		
46	36.2	34.2	137.0

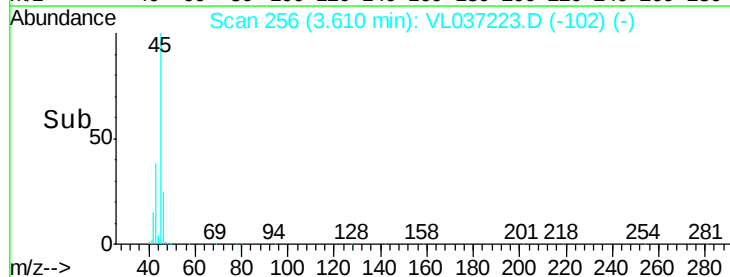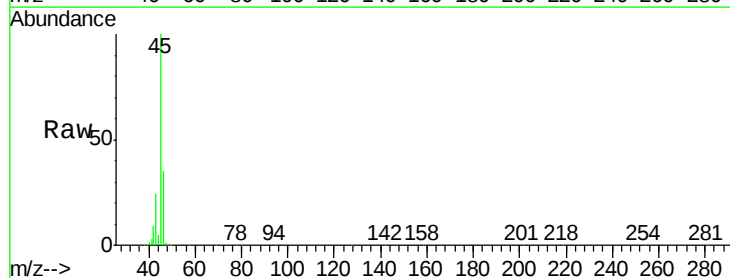

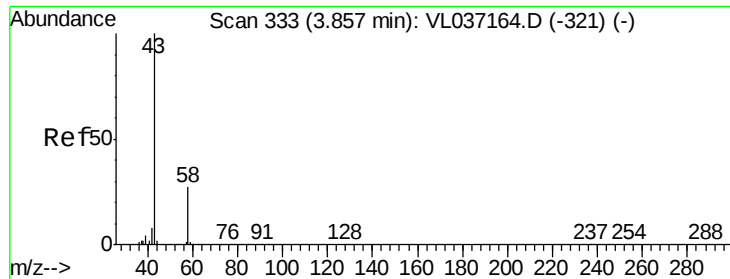





#15
Acetone
Concen: 47.124 ppbv m
RT: 3.85 min Scan# 332
Delta R.T. -0.00 min
Lab File: VL037223.D
Acq: 22 Jun 2021 19:08

Instrument :
MSVOA_L
ClientSampleId :
IAQ-01

Tot Ion: 43 Resp: 6283687
Ion Ratio Lower Upper
43 100
58 34.4 23.7 35.5




Manual Integrations
APPROVED


MMDadoda
6/24/2021 4:32:56 PM

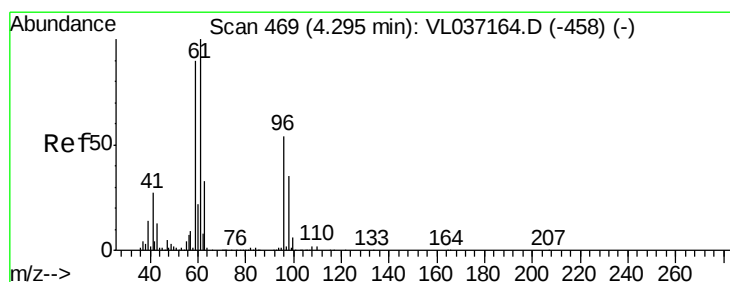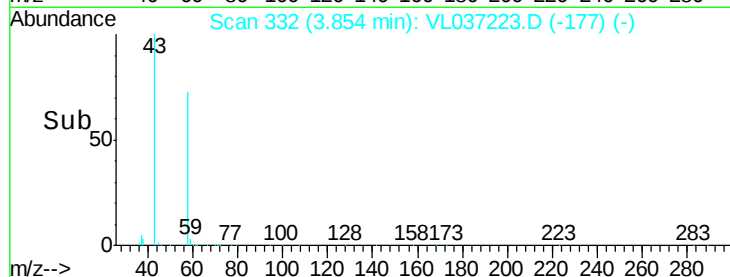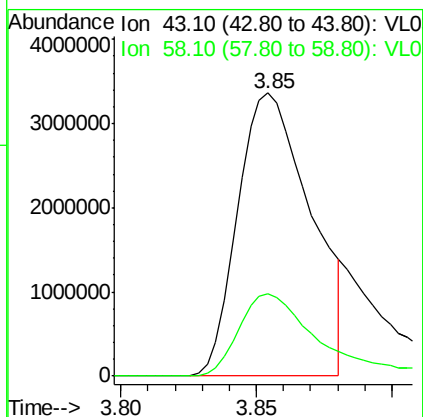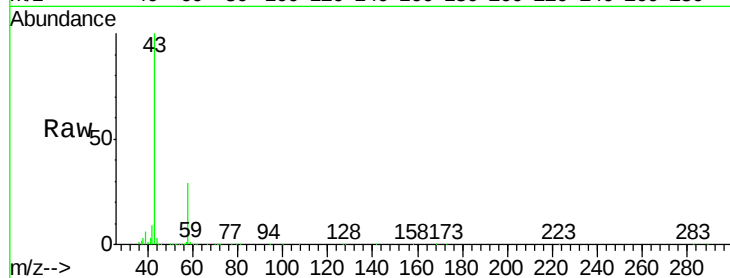

#17
tert-Butyl alcohol
Concen: 2.012 ppbv
RT: 4.31 min Scan# 475
Delta R.T. 0.02 min
Lab File: VL037223.D
Acq: 22 Jun 2021 19:08

Tgt Ion: 59 Resp: 248017
Ion Ratio Lower Upper
59 100
57 12.5 8.8 13.2

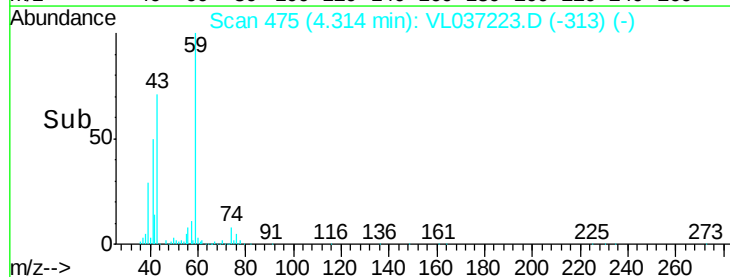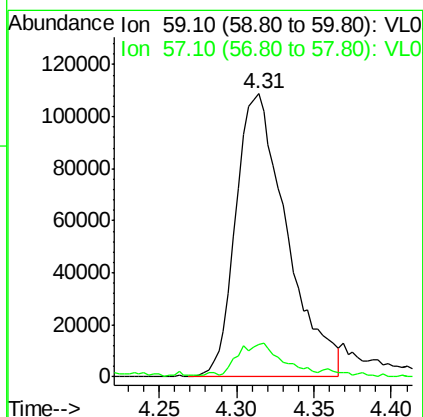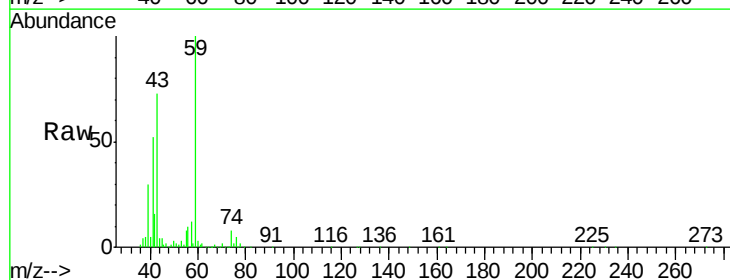



#19

Isopropyl Alcohol

Concen: 3.435 ppbv

RT: 3.99 min Scan# 373

Delta R.T. 0.01 min

Lab File: VL037223.D

Acq: 22 Jun 2021 19:08

Instrument :

MSVOA_L

ClientSampleId :

IAQ-01

Tot Ion: 45 Resp: 277453

Ion Ratio Lower Upper

45 100





58 778.1 2.4 3.6#

Manual Integrations

APPROVED

MMDadoda

6/24/2021 4:32:56 PM

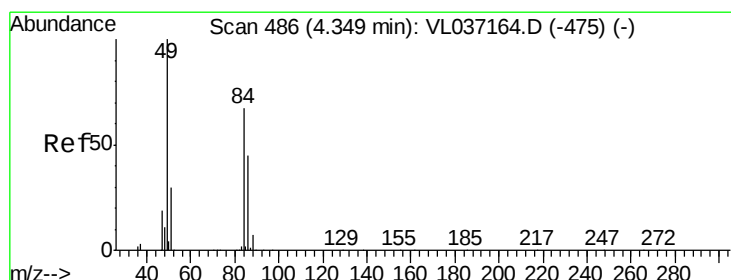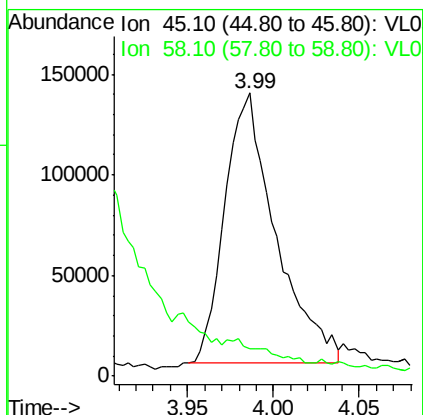

#20

Methylene Chloride

Concen: 4.290 ppbv

RT: 4.36 min Scan# 488

Delta R.T. 0.01 min

Lab File: VL037223.D

Acq: 22 Jun 2021 19:08

Tgt Ion: 84 Resp: 342448




Ion Ratio Lower Upper


84 100

49 151.7 119.7 179.5

51 46.9 36.1 54.1

86 66.8 53.7 80.5

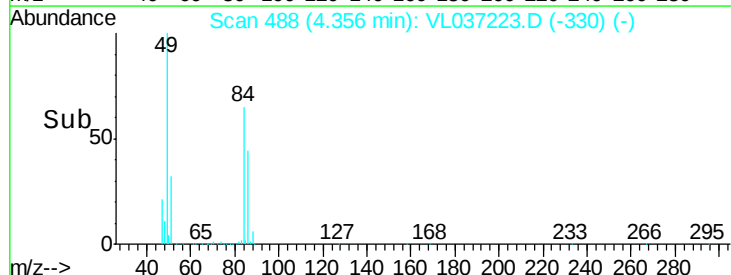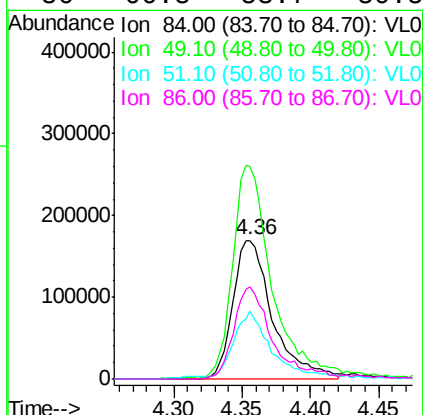

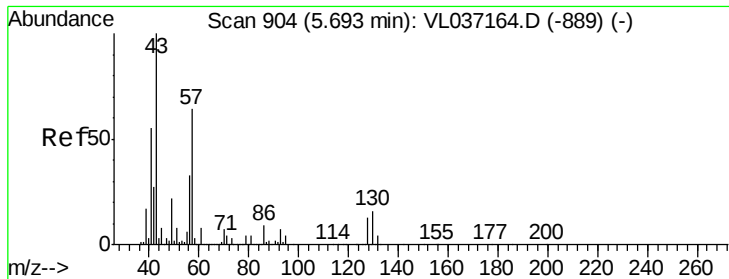





#26
Hexane
Concen: 8.926 ppbv
RT: 5.70 min Scan# 906
Delta R.T. 0.01 min
Lab File: VL037223.D
Acq: 22 Jun 2021 19:08

Instrument :
MSVOA_L
ClientSampleId :
IAQ-01

Tot Ion	Ratio	Lower	Upper
57	100		
41	93.2	73.5	110.3
43	115.0	170.7	256.1#
56	53.0	42.4	63.6




Manual Integrations
APPROVED


MMDadoda
6/24/2021 4:32:56 PM

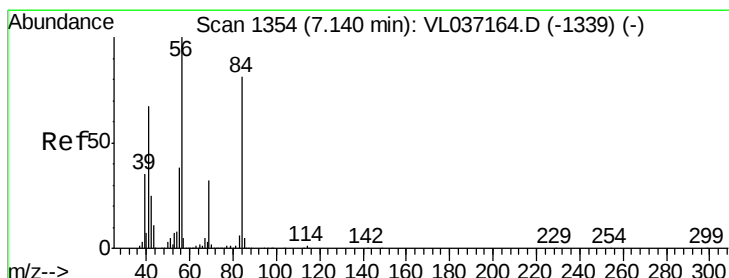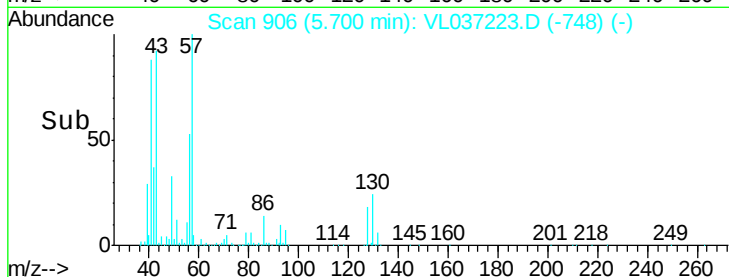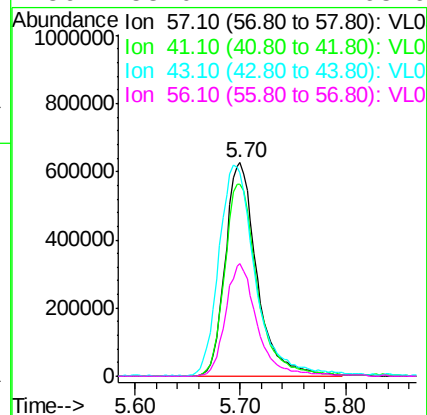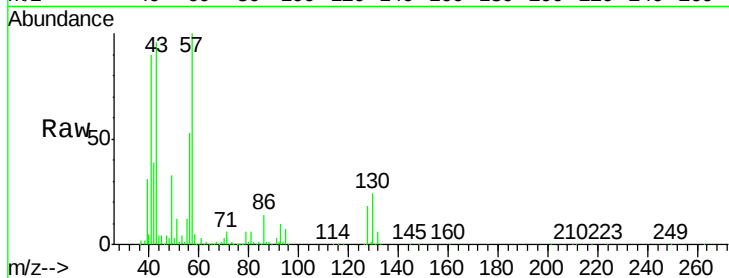

#30
Cyclohexane
Concen: 1.728 ppbv
RT: 7.14 min Scan# 1355
Delta R.T. 0.00 min
Lab File: VL037223.D
Acq: 22 Jun 2021 19:08

Tgt Ion	Ratio	Lower	Upper
84	100		
56	163.5	107.7	161.5#
41	88.0	69.0	103.6

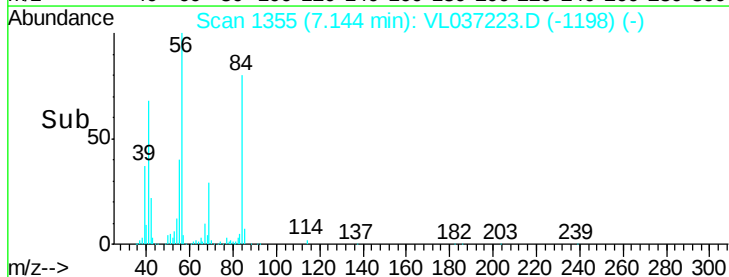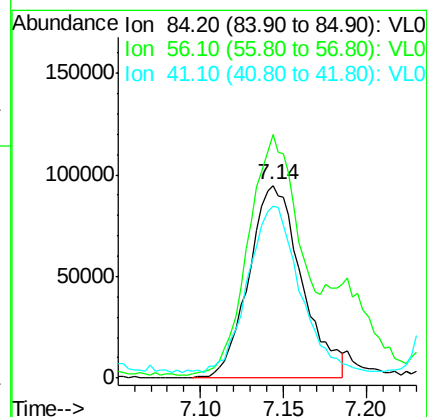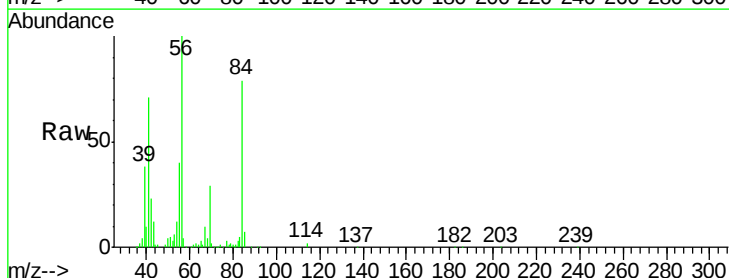







#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.19 min Scan# 1369
 Delta R.T. 0.00 min
 Lab File: VL037223.D
 Acq: 22 Jun 2021 19:08

Instrument :
 MSVOA_L
 ClientSampleId :
 IAQ-01

Tot Ion	Ratio	Lower	Upper
114	100		
63	24.7	19.6	29.4
88	17.6	14.2	21.2




Manual Integrations
 APPROVED


MMDadoda
 6/24/2021 4:32:56 PM

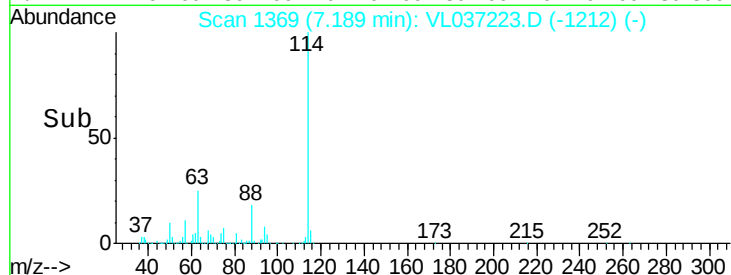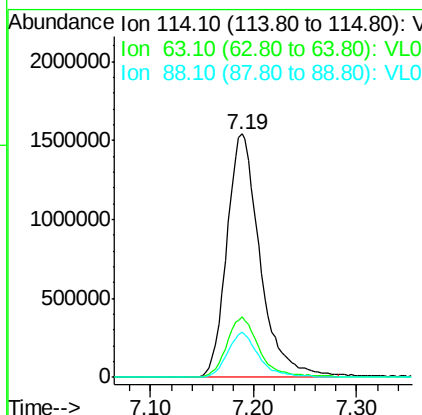

#34
 2-Butanone
 Concen: 1.973 ppbv
 RT: 5.26 min Scan# 769
 Delta R.T. 0.01 min
 Lab File: VL037223.D
 Acq: 22 Jun 2021 19:08

Tgt Ion	Ratio	Lower	Upper
43	100		
72	26.4	18.9	28.3



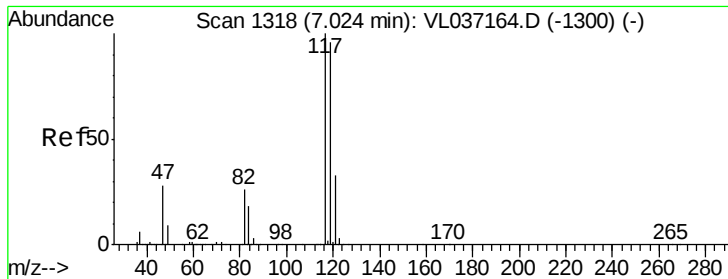





#35
Carbon Tetrachloride
Concen: 0.068 ppbv m
RT: 7.03 min Scan# 1319
Delta R.T. 0.00 min
Lab File: VL037223.D
Acq: 22 Jun 2021 19:08

Instrument :
MSVOA_L
ClientSampleId :
IAQ-01

Tot Ion	Ratio	Lower	Upper
117	100		
119	91.5	76.6	114.8
121	30.4	26.4	39.6




Manual Integrations
APPROVED


MMDadoda
6/24/2021 4:32:56 PM

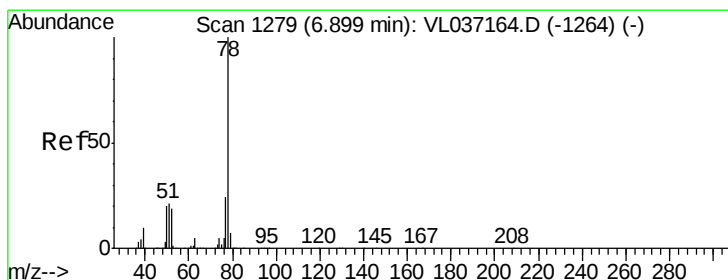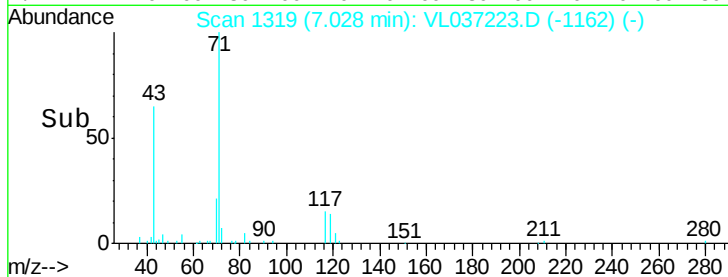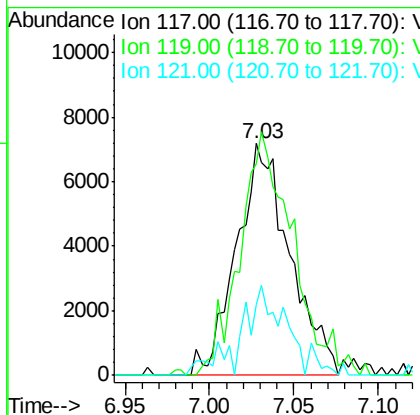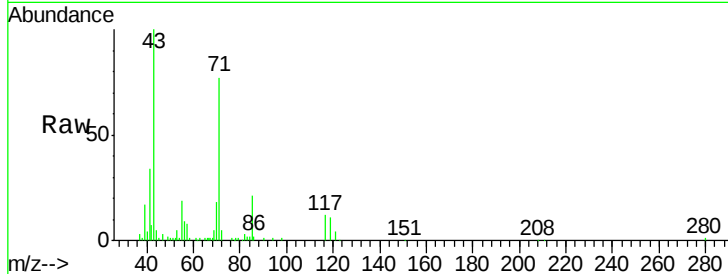

#36
Benzene
Concen: 0.302 ppbv m
RT: 6.91 min Scan# 1281
Delta R.T. 0.01 min
Lab File: VL037223.D
Acq: 22 Jun 2021 19:08

Tgt Ion	Ratio	Lower	Upper
78	100		
77	18.8	19.0	28.6#
50	23.7	15.7	23.5#

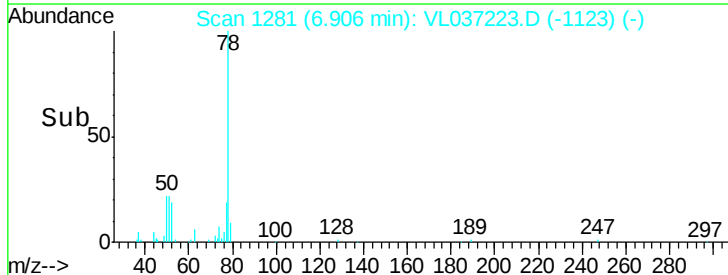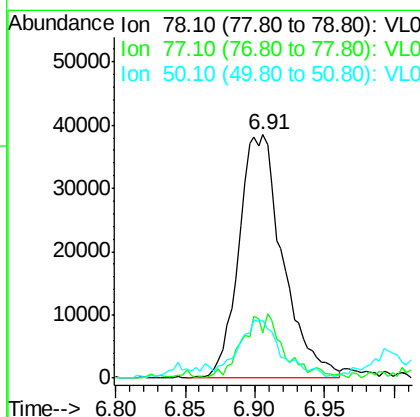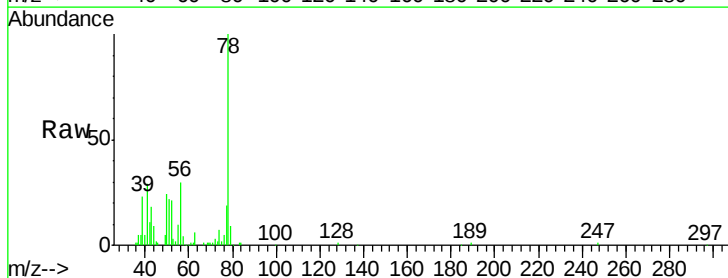



#44

2,2,4-Trimethylpentane

Concen: 0.290 ppbv

RT: 7.88 min Scan# 1585

Delta R.T. 0.00 min

Lab File: VL037223.D

Acq: 22 Jun 2021 19:08

Instrument :

MSVOA_L

ClientSampleId :

IAQ-01

Tot Ion: 57 Resp: 136723

Ion Ratio Lower Upper

57 100





41 0.0 27.6 41.4#

56 100.2 25.3 37.9#

Manual Integrations
APPROVED

MMDadoda

6/24/2021 4:32:56 PM

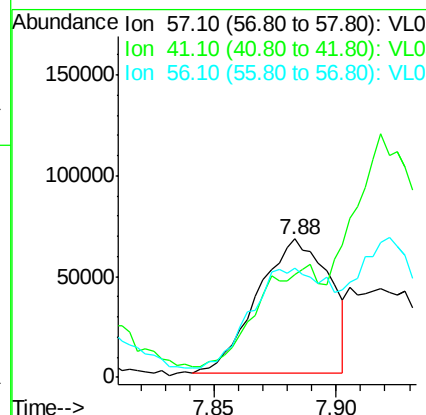

#52

Tetrachloroethene

Concen: 0.034 ppbv m

RT: 11.24 min Scan# 2630

Delta R.T. 0.01 min

Lab File: VL037223.D

Acq: 22 Jun 2021 19:08

Tgt Ion:164 Resp: 4421




Ion Ratio Lower Upper


164 100

166 109.7 97.6 146.4

129 103.7 82.9 124.3

131 84.9 80.6 120.8

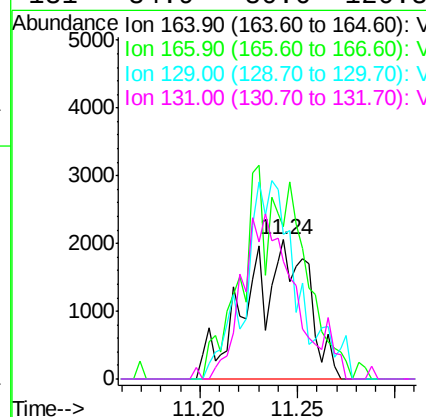







#53
Toluene
Concen: 2.813 ppbv
RT: 9.82 min Scan# 2187
Delta R.T. 0.00 min
Lab File: VL037223.D
Acq: 22 Jun 2021 19:08

Instrument :
MSVOA_L
ClientSampleId :
IAQ-01

Tot Ion	Ratio	Lower	Upper
91	100		
92	60.0	48.3	72.5




Manual Integrations
APPROVED


MMDadoda
6/24/2021 4:32:56 PM

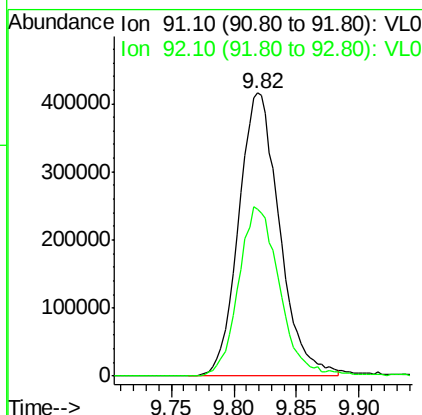

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.10 min Scan# 2896
Delta R.T. 0.00 min
Lab File: VL037223.D
Acq: 22 Jun 2021 19:08

Tgt Ion	Ratio	Lower	Upper
117	100		
82	62.4	51.7	77.5
119	33.6	47.6	71.4#



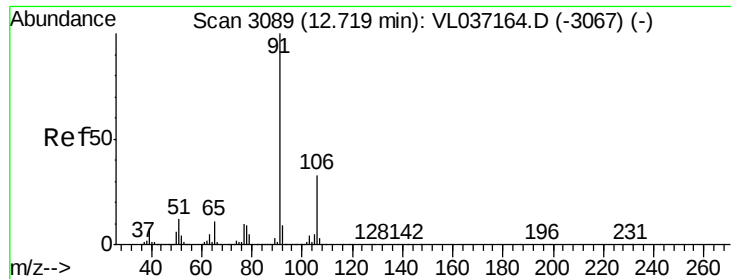





#58
Ethyl Benzene
Concen: 1.273 ppbv
RT: 12.73 min Scan# 3091
Delta R.T. 0.01 min
Lab File: VL037223.D
Acq: 22 Jun 2021 19:08

Instrument :
MSVOA_L
ClientSampled :
IAQ-01

Tot Ion: 91 Resp: 580055
Ion Ratio Lower Upper
91 100
106 30.8 26.3 39.5




Manual Integrations
APPROVED


MMDadoda
6/24/2021 4:32:56 PM

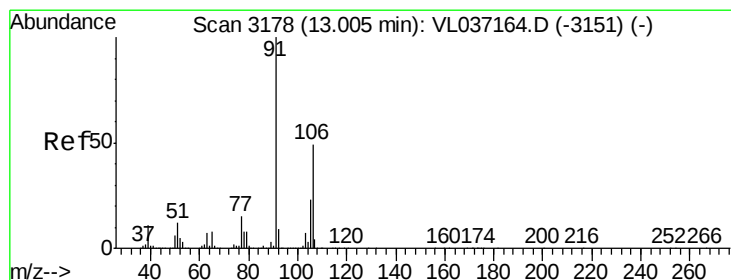

#59
m/p-Xylene
Concen: 5.057 ppbv
RT: 12.98 min Scan# 3171
Delta R.T. -0.02 min
Lab File: VL037223.D
Acq: 22 Jun 2021 19:08

Tgt Ion: 91 Resp: 1952490
Ion Ratio Lower Upper
91 100
106 47.6 37.0 55.4



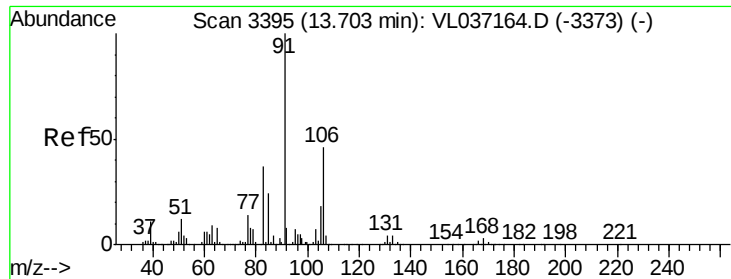





#60
o-Xylene
Concen: 1.841 ppbv
RT: 13.71 min Scan# 3396
Delta R.T. 0.00 min
Lab File: VL037223.D
Acq: 22 Jun 2021 19:08

Instrument :
MSVOA_L
ClientSampleId :
IAQ-01

Tot Ion: 91 Resp: 676736
Ion Ratio Lower Upper
91 100
106 43.8 23.0 69.0




Manual Integrations
APPROVED


MMDadoda
6/24/2021 4:32:56 PM

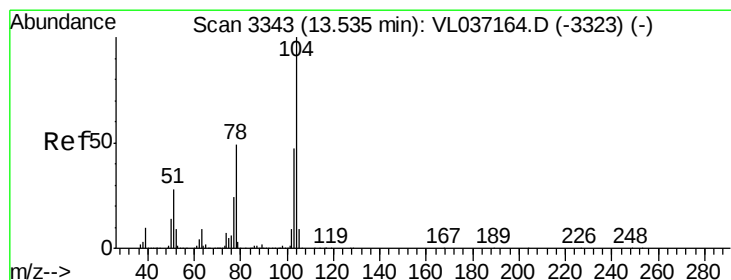

#61
Styrene
Concen: 1.148 ppbv m
RT: 13.55 min Scan# 3346
Delta R.T. 0.01 min
Lab File: VL037223.D
Acq: 22 Jun 2021 19:08

Tgt Ion: 104 Resp: 217748
Ion Ratio Lower Upper
104 100
78 0.0 39.7 59.5#
103 48.1 37.6 56.4



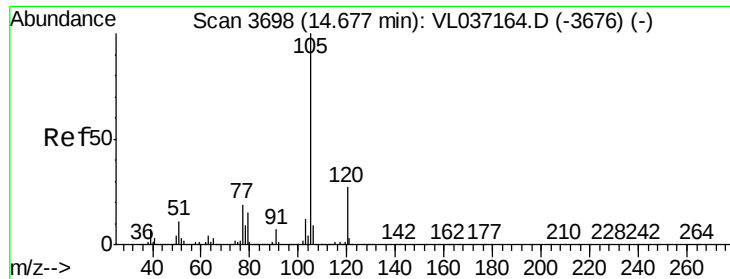

#62

Isopropylbenzene

Concen: 0.155 ppbv m

RT: 14.68 min Scan# 3699

Delta R.T. 0.00 min

Lab File: VL037223.D

Acq: 22 Jun 2021 19:08

Instrument :

MSVOA_L

ClientSampleId :

IAQ-01

Tot Ion:105 Resp: 80784

Ion Ratio Lower Upper


105 100

120 28.3 21.6 32.4

Manual Integrations
APPROVED

MMDadoda

6/24/2021 4:32:56 PM

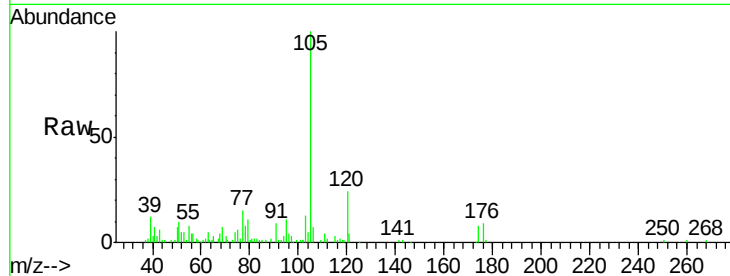

Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

14.68



30000

20000

10000

0

Time-->

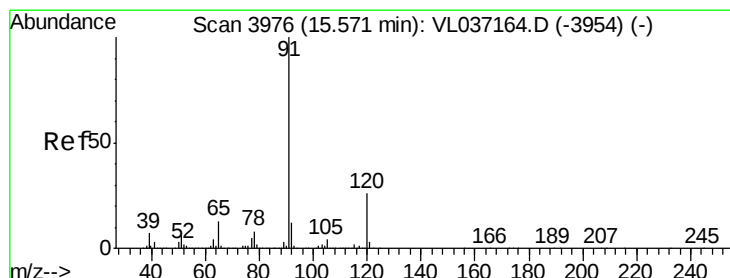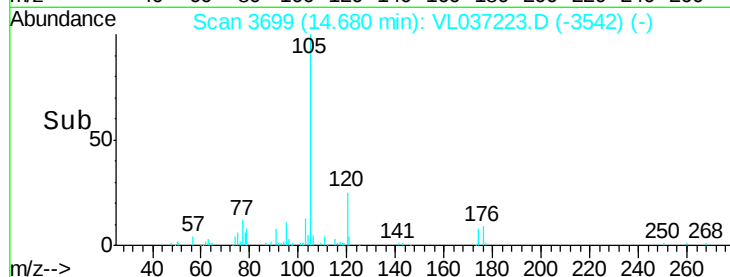

#64

n-propylbenzene

Concen: 0.236 ppbv

RT: 15.58 min Scan# 3978

Delta R.T. 0.01 min

Lab File: VL037223.D


Acq: 22 Jun 2021 19:08

Tgt Ion:120 Resp: 30872

Ion Ratio Lower Upper

120 100

91 489.5 343.3 514.9

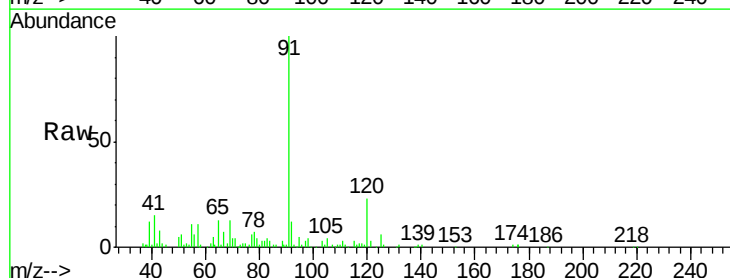

Abundance Ion 120.20 (119.90 to 120.90): V

Ion 91.10 (90.80 to 91.80): V

15.58


60000


40000

20000

0

Time-->

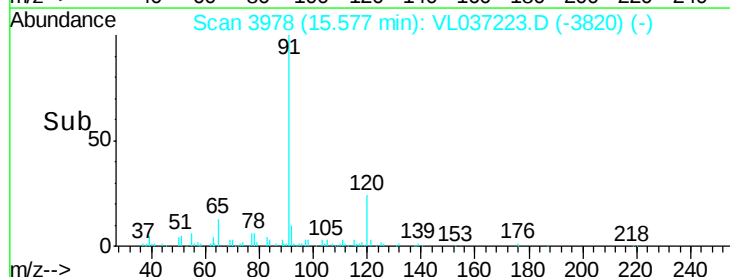

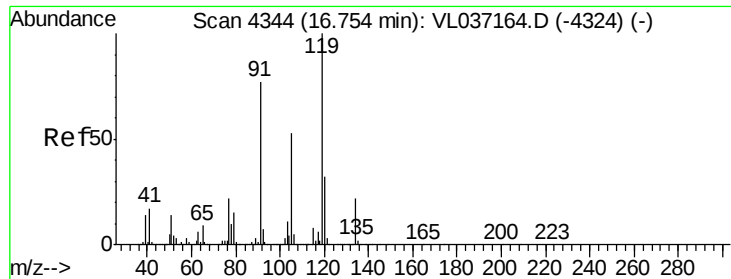

#65

tert-Butylbenzene

Concen: 0.136 ppbv

RT: 16.78 min Scan# 4351

Delta R.T. 0.02 min

Lab File: VL037223.D

Acq: 22 Jun 2021 19:08

Instrument :

MSVOA_L





ClientSampleId :

IAQ-01

Tot Ion:	119	Resp:	63290
Ion Ratio	Lower	Upper	
119	100		
91	119.5	62.6	93.8#
134	2.5	16.2	24.4#

Manual Integrations
APPROVED

MMDadoda
6/24/2021 4:32:56 PM

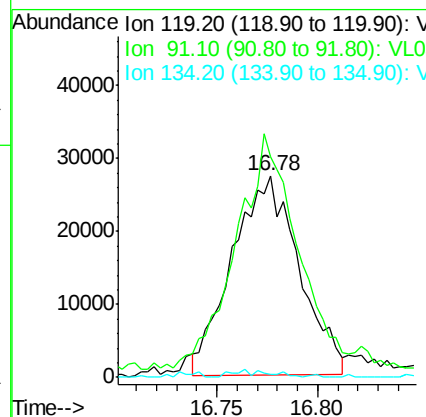

#68

1-Bromo-4-Fluorobenzene

Concen: 10.484 ppbv




RT: 14.43 min Scan# 3621


Delta R.T. 0.00 min

Lab File: VL037223.D

Acq: 22 Jun 2021 19:08

Tgt Ion:	95	Resp:	2629441
Ion Ratio	Lower	Upper	
95	100		
174	72.7	57.0	85.4
175	5.4	4.4	6.6

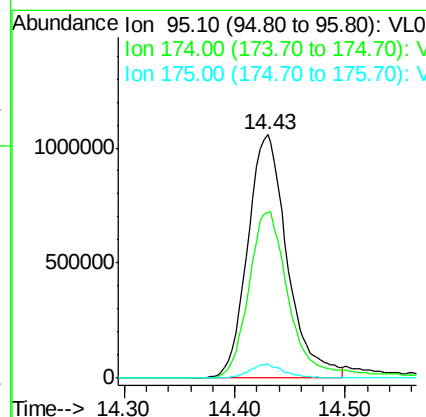

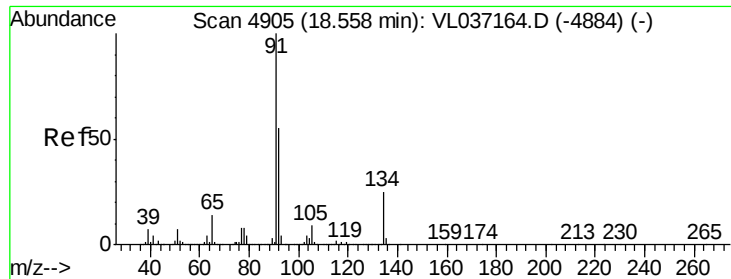





#70
n-Butylbenzene
Concen: 0.134 ppbv m
RT: 18.57 min Scan# 4909
Delta R.T. 0.01 min
Lab File: VL037223.D
Acq: 22 Jun 2021 19:08

Instrument :
MSVOA_L
ClientSampled :
IAQ-01

Tot Ion	Ratio	Lower	Upper
91	100		
92	40.5	44.0	66.0#
134	0.0	20.2	30.4#




Manual Integrations
APPROVED


MMDadoda
6/24/2021 4:32:56 PM



#72
4-Ethyltoluene
Concen: 0.363 ppbv
RT: 15.85 min Scan# 4064
Delta R.T. 0.01 min
Lab File: VL037223.D
Acq: 22 Jun 2021 19:08

Tgt Ion	Ratio	Lower	Upper
105	100		
120	36.9	24.7	37.1
91	16.5	10.2	15.4#
77	17.6	11.0	16.6#



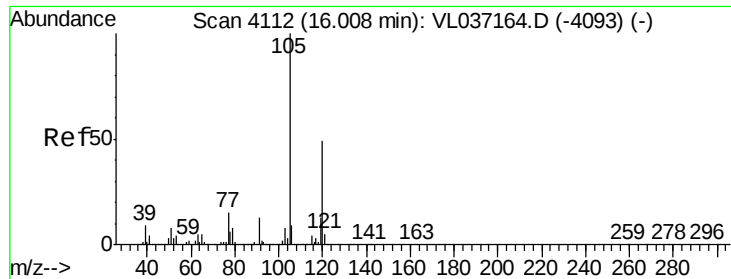

#73

1,3,5-Trimethylbenzene

Concen: 0.476 ppbv

RT: 16.01 min Scan# 4113

Delta R.T. 0.00 min

Lab File: VL037223.D

Acq: 22 Jun 2021 19:08

Instrument :

MSVOA_L

ClientSampleId :

IAQ-01

Tot Ion:105 Resp: 192318

Ion Ratio Lower Upper





105 100

120 46.0 39.4 59.2

Manual Integrations
APPROVED

MMDadoda

6/24/2021 4:32:56 PM

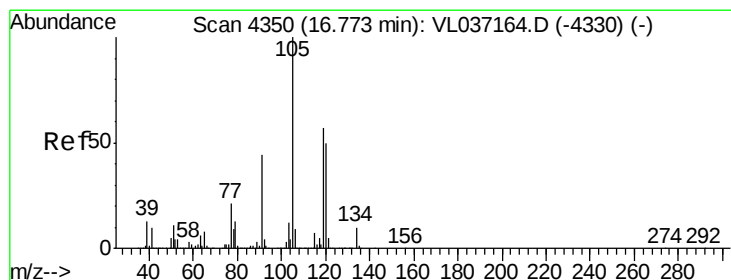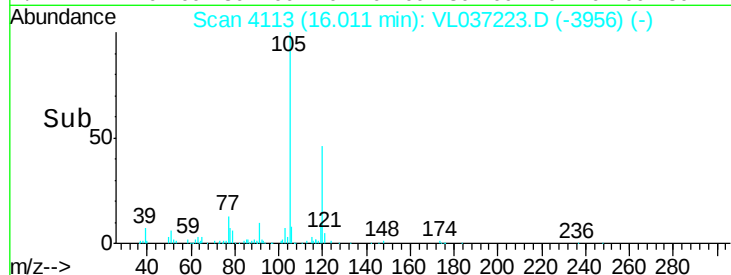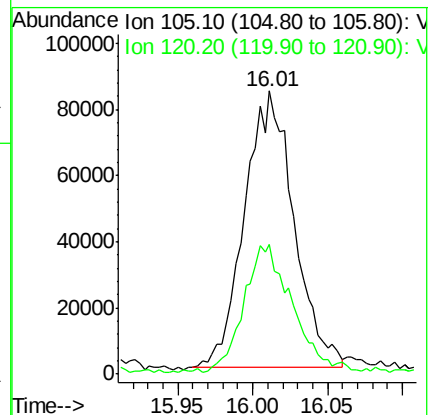

#74

1,2,4-Trimethylbenzene

Concen: 1.360 ppbv

RT: 16.78 min Scan# 4351

Delta R.T. 0.00 min

Lab File: VL037223.D

Acq: 22 Jun 2021 19:08

Tgt Ion:105 Resp: 565859




Ion Ratio Lower Upper


105 100

120 39.5 39.8 59.8#

91 12.2 37.0 55.4#

77 14.7 17.0 25.4#

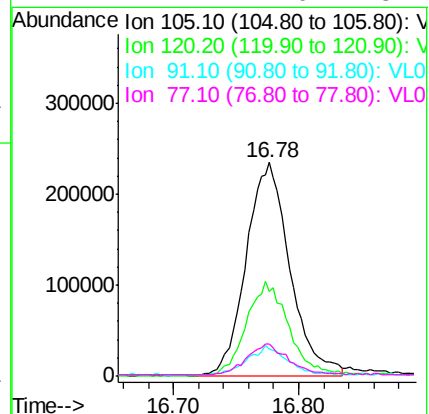

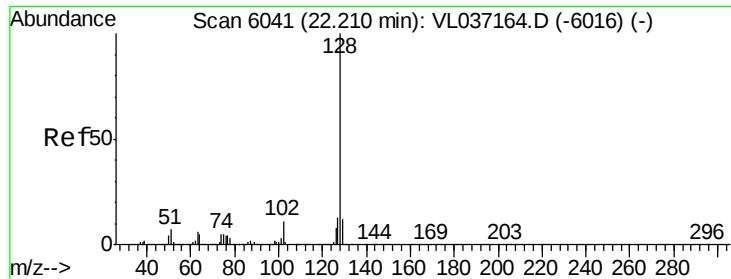

#79
Naphthalene
Concen: 0.157 ppbv
RT: 22.22 min Scan# 6045
Delta R.T. 0.01 min
Lab File: VL037223.D
Acq: 22 Jun 2021 19:08

Instrument :
MSVOA_L
ClientSampleId :
IAQ-01

Tot Ion	Ratio	Lower	Upper
128	100		
127	7.8	10.7	16.1#
129	11.4	9.3	13.9

Manual Integrations
APPROVED

MMDadoda
6/24/2021 4:32:56 PM

