
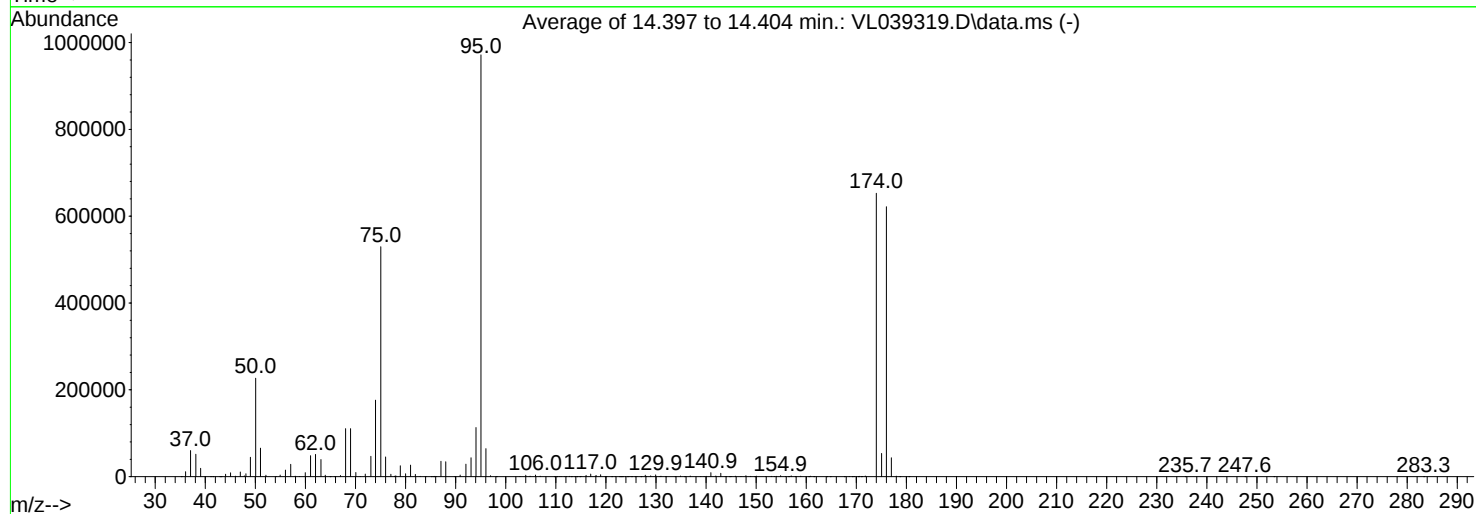


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062222\
Data File : VL039319.D
Acq On : 22 Jun 2022 12:18
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jun 23 11:28:24 2022

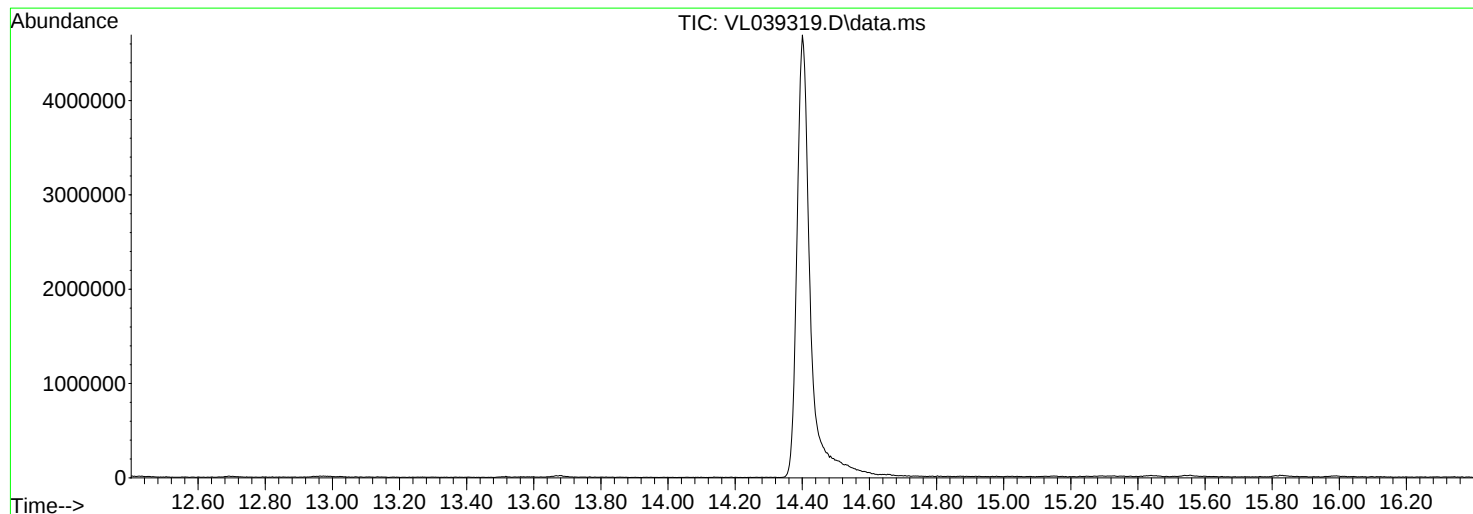

AutoFind: Scans 3611, 3612, 3613; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.3	226752	PASS
75	95	30	80	54.5	529813	PASS
95	95	100	100	100.0	971797	PASS
96	95	5	9	6.6	64547	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.2	652843	PASS
175	174	5	9	8.2	53480	PASS
176	174	95	105	95.2	621760	PASS
177	176	5	10	7.0	43619	PASS