

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL062419\
 Data File : VL033952.D
 Acq On : 25 Jun 2019 1:16
 Operator : SY/AP
 Sample : K3481-07
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 TZC-SSDS-AREA-D-1

Manual Integrations
 APPROVED

MMDadoda
 6/26/2019 8:15:51 AM

Quant Time: Jun 25 05:07:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL060719AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Jun 0
 QLast Update : Fri Jun 07 08:53:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.75	49	890189	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.28	114	2235509	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.22	117	2240413	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.56	95	1982295	10.77	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	107.70%

Target Compounds					Ovalue
2) Dichlorodifluoromethane	3.07	85	46536	0.322 ppbv	97
3) Chlorodifluoromethane	3.00	51	167075m	1.594 ppbv	
9) Propene	3.04	41	30438m	0.776 ppbv	
10) Heptane	8.23	43	755115	7.619 ppbv #	78
11) Trichlorofluoromethane	3.99	101	546085	2.930 ppbv	93
13) Ethanol	3.65	45	144837	11.353 ppbv	99
15) Acetone	3.89	43	19791748	152.443 ppbv #	66
17) tert-Butyl alcohol	4.35	59	3223182	31.758 ppbv	98
19) Isopropyl Alcohol	4.02	45	417395	5.628 ppbv #	94
20) Methylene Chloride	4.41	84	42593	0.841 ppbv #	90
26) Hexane	5.76	57	129925	1.443 ppbv #	41
27) Carbon Disulfide	4.60	76	108846	0.870 ppbv	95
29) Chloroform	5.84	83	34137	0.221 ppbv	93
34) 2-Butanone	5.31	43	2416236	19.159 ppbv	99
35) Carbon Tetrachloride	7.11	117	9068m	0.053 ppbv	
36) Benzene	6.99	78	1932900	11.319 ppbv	99
38) Trichloroethene	7.95	130	27199	0.409 ppbv	94
52) Tetrachloroethene	11.35	164	167701	2.791 ppbv	91
53) Toluene	9.92	91	2681810	14.191 ppbv	98
58) Ethyl Benzene	12.84	91	12451876	49.296 ppbv	90
59) m/p-Xylene	13.11	91	27697221	120.580 ppbv #	83
60) o-Xylene	13.83	91	14606422	61.588 ppbv	91
61) Styrene	13.68	104	16622104	108.303 ppbv	95
62) Isopropylbenzene	14.80	105	408141	1.277 ppbv	99
64) n-propylbenzene	15.70	120	109359	1.336 ppbv	86
70) n-Butylbenzene	18.69	91	55456	0.147 ppbv #	90
73) 1,3,5-Trimethylbenzene	16.14	105	33018	0.124 ppbv #	80
74) 1,2,4-Trimethylbenzene	16.90	105	87425m	0.285 ppbv	
80) Naphthalene,2-methyl-	25.09	142	5494	0.056 ppbv #	66

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL062419\
Data File : VL033952.D
Acq On : 25 Jun 2019 1:16
Operator : SY/AP
Sample : K3481-07
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
TZC-SSDS-AREA-D-1

Manual Integrations
APPROVED

MMDadoda
6/26/2019 8:15:51 AM

Quant Time: Jun 25 05:07:43 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL060719AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Jun
QLast Update : Fri Jun 07 08:53:27 2019
Response via : Initial Calibration

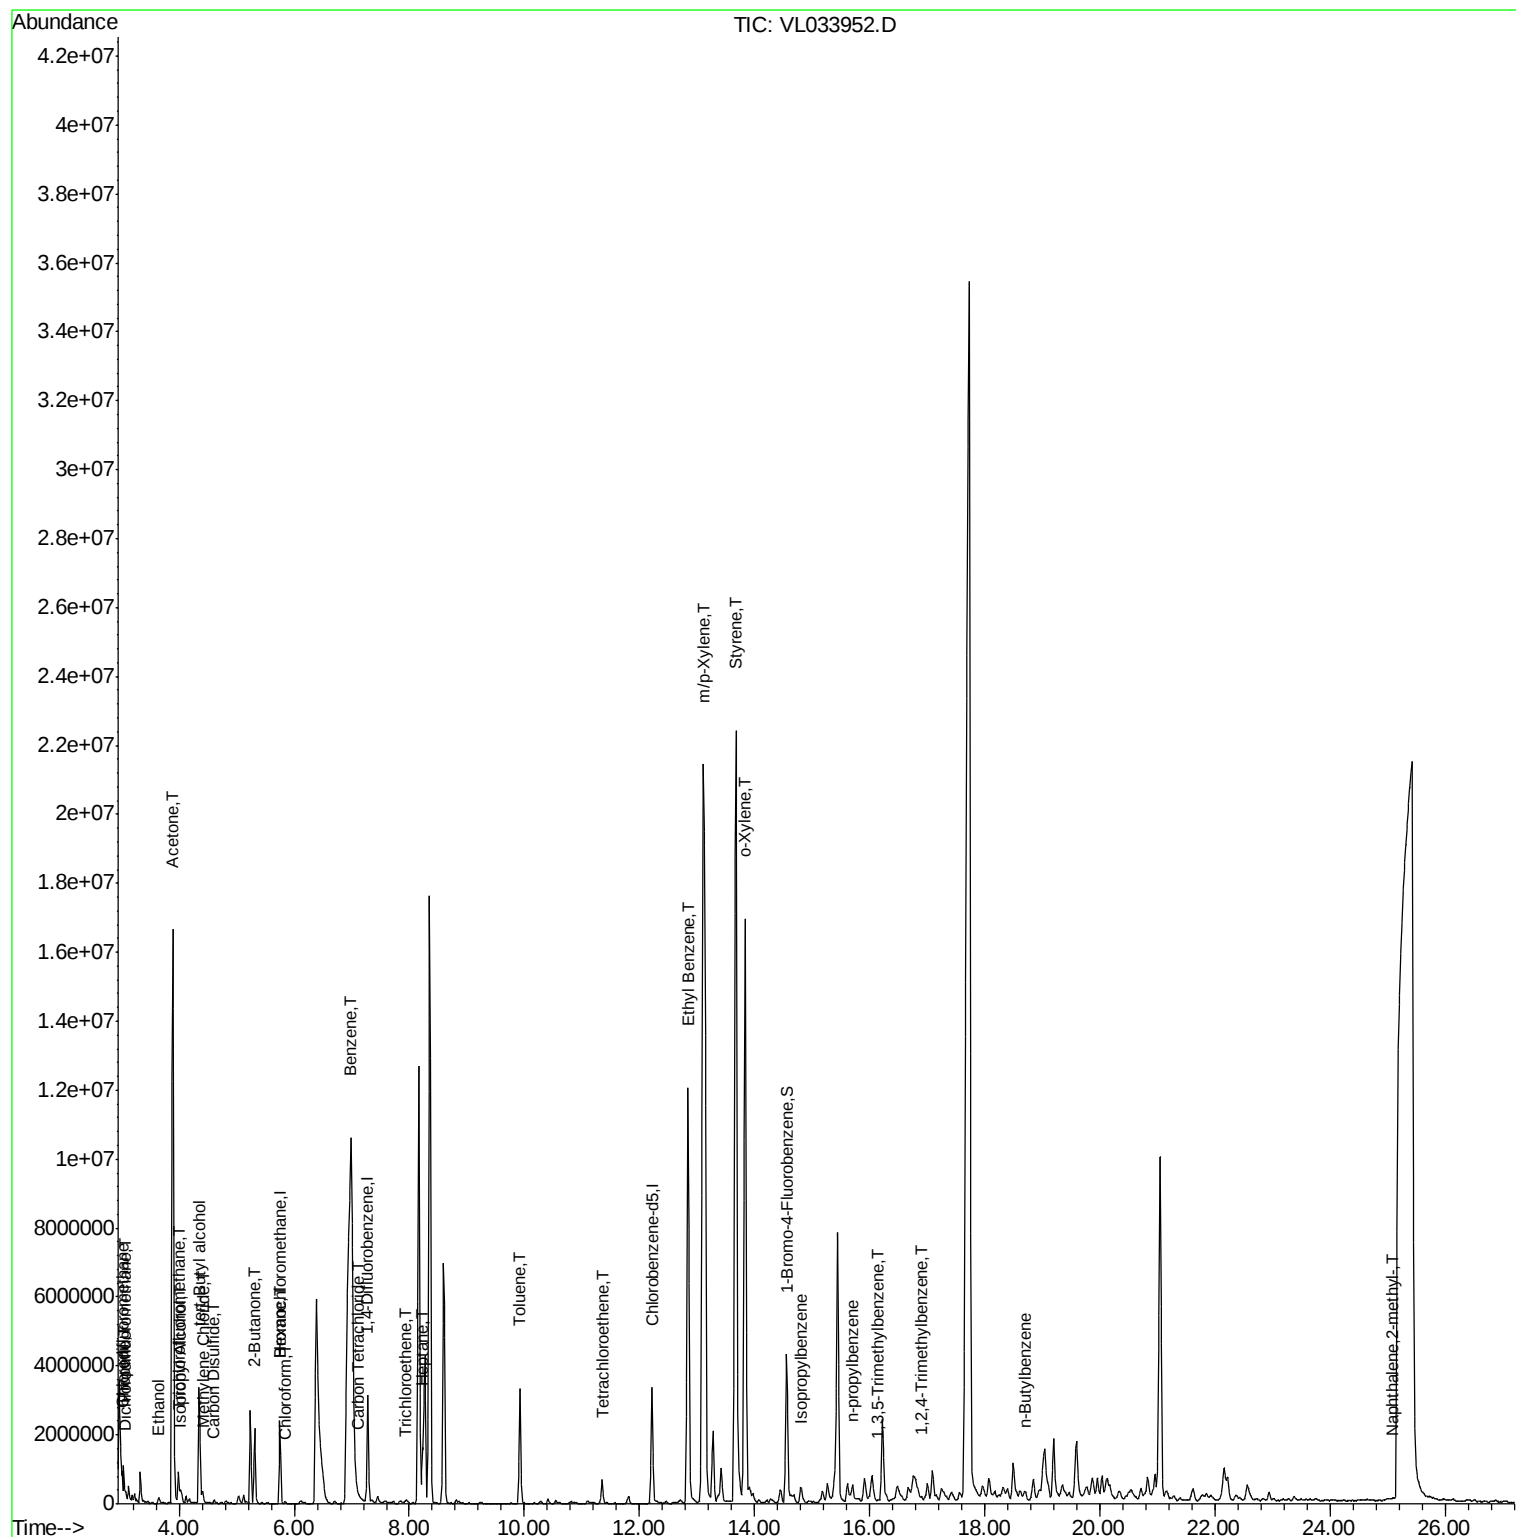

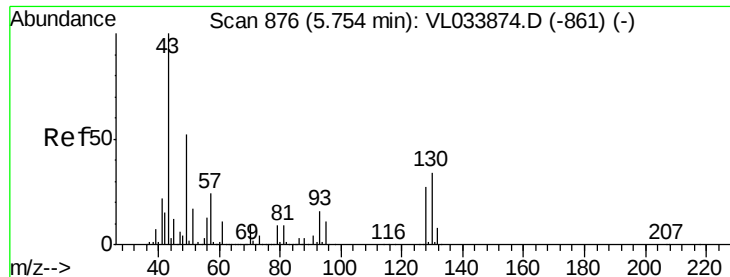

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.75 min Scan# 876

Delta R.T. -0.00 min

Lab File: VL033952.D

Acq: 25 Jun 2019 1:16

Instrument :

MSVOA_L


ClientSampleId :

TZC-SSDS-AREA-D-1

Tot Ion	Ratio	Lower	Upper
49	100		
128	50.7	25.5	76.5
130	65.1	32.5	97.4

Manual Integrations
APPROVED




MMDadoda
6/26/2019 8:15:51 AM

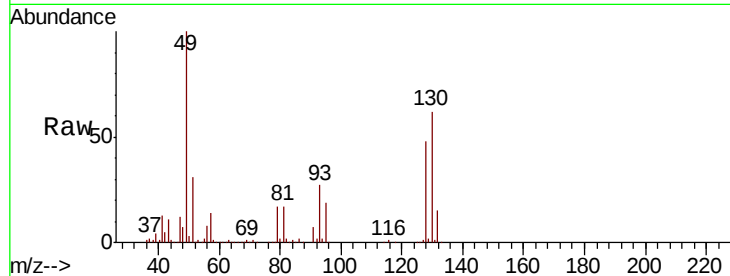

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): V

Ion 130.00 (129.70 to 130.70): V

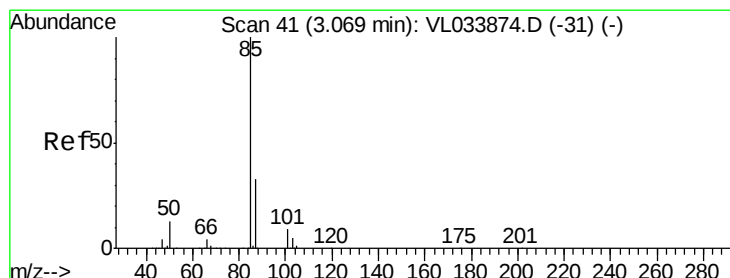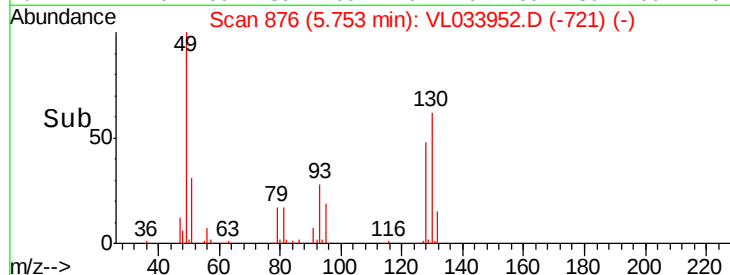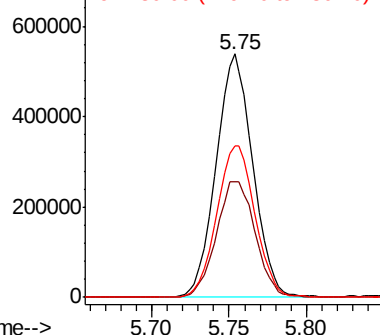

#2

Dichlorodifluoromethane

Concen: 0.322 ppbv


RT: 3.07 min Scan# 40

Delta R.T. -0.00 min

Lab File: VL033952.D



Acq: 25 Jun 2019 1:16


Tgt Ion	Ratio	Lower	Upper
85	100		
87	31.7	26.6	40.0

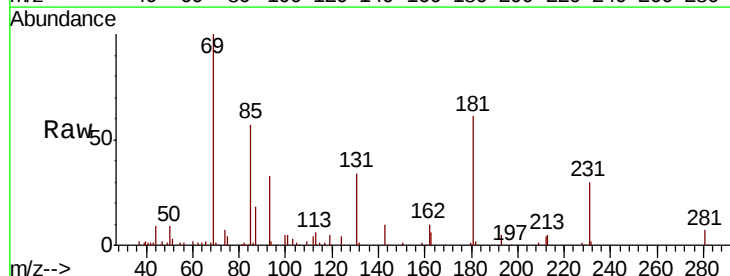

Abundance Ion 85.00 (84.70 to 85.70): VL0

Ion 87.00 (86.70 to 87.70): VL0

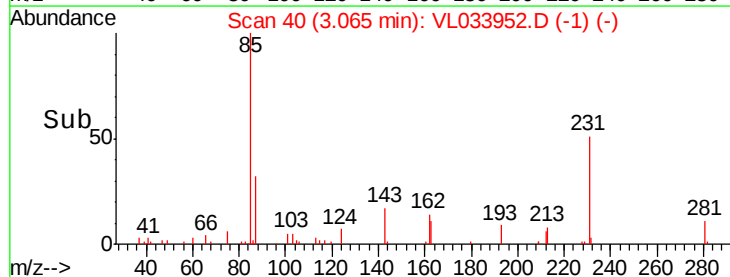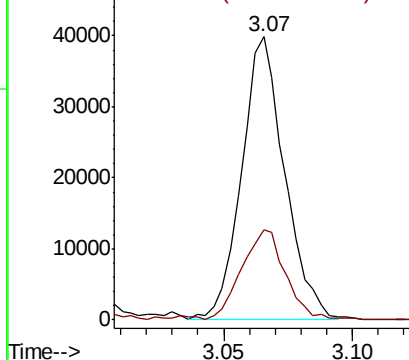

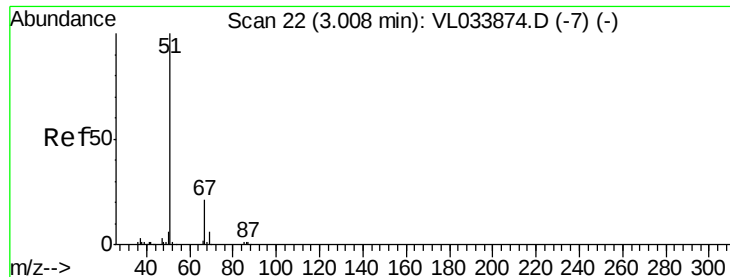





#3
Chlorodifluoromethane
Concen: 1.594 ppbv m
RT: 3.00 min Scan# 20
Delta R.T. -0.01 min
Lab File: VL033952.D
Acq: 25 Jun 2019 1:16

Instrument :
MSVOA_L
ClientSampleId :
TZC-SSDS-AREA-D-1

Tot Ion: 51 Resp: 167075
Ion Ratio Lower Upper
51 100
67 15.3 16.4 24.6#




Manual Integrations
APPROVED


MMDadoda
6/26/2019 8:15:51 AM

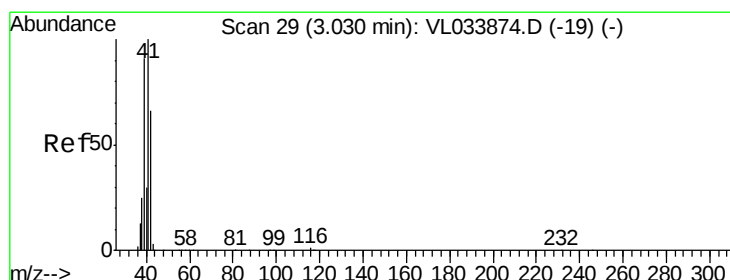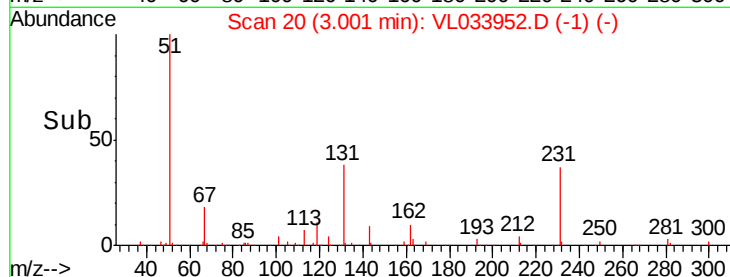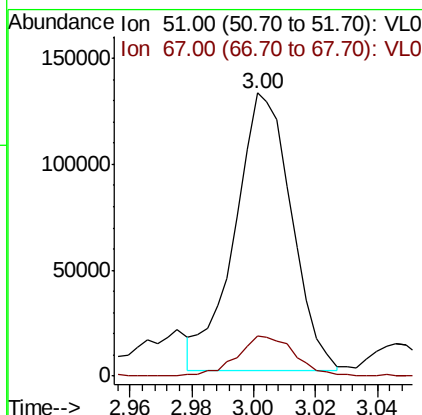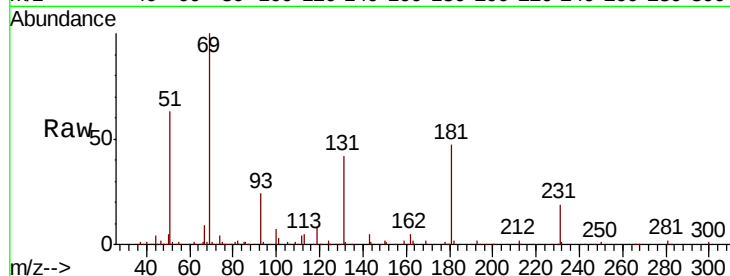

#9
Propene
Concen: 0.776 ppbv m
RT: 3.04 min Scan# 31
Delta R.T. 0.01 min
Lab File: VL033952.D
Acq: 25 Jun 2019 1:16

Tgt Ion: 41 Resp: 30438
Ion Ratio Lower Upper
41 100
42 60.2 56.3 84.5

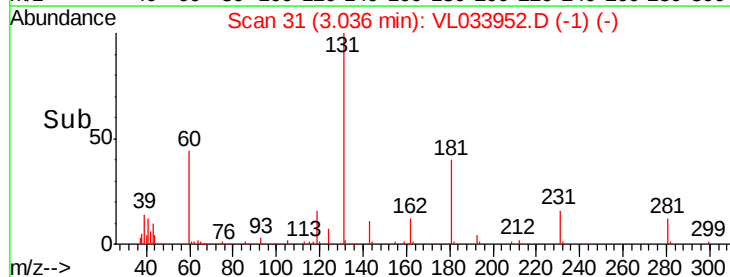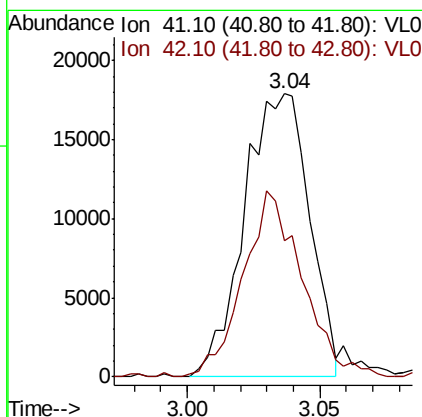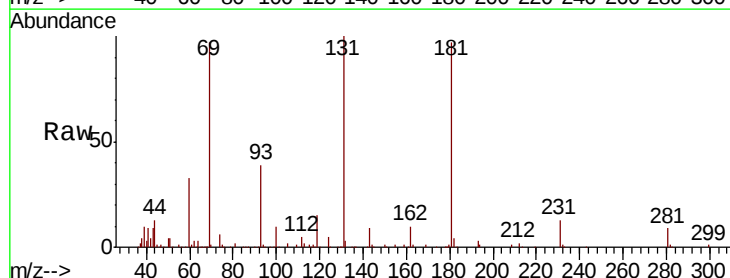







#10
Heptane
Concen: 7.619 ppbv
RT: 8.23 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VL033952.D
Acq: 25 Jun 2019 1:16

Instrument :
MSVOA_L
ClientSampleId :
TZC-SSDS-AREA-D-1

Tot Ion: 43 Resp: 755115
Ion Ratio Lower Upper
43 100
57 67.4 41.7 62.5#




Manual Integrations
APPROVED


MMDadoda
6/26/2019 8:15:51 AM

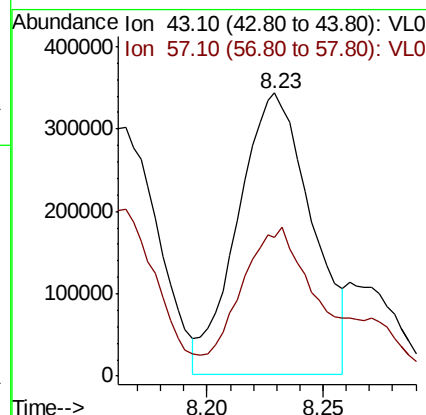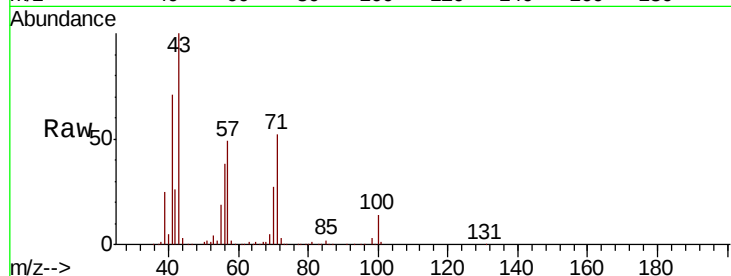

#11
Trichlorofluoromethane
Concen: 2.930 ppbv
RT: 3.99 min Scan# 327
Delta R.T. -0.01 min
Lab File: VL033952.D
Acq: 25 Jun 2019 1:16

Tgt Ion: 101 Resp: 546085
Ion Ratio Lower Upper
101 100
103 61.3 53.6 80.4

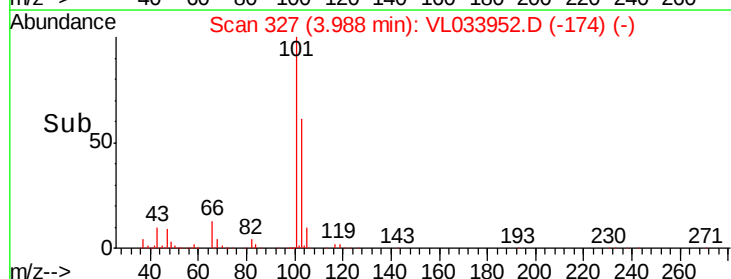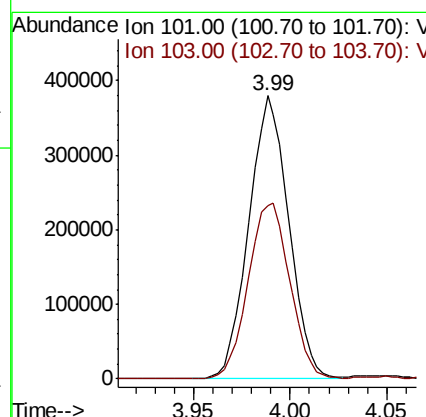



#13

Ethanol

Concen: 11.353 ppbv

RT: 3.65 min Scan# 221

Delta R.T. 0.01 min

Lab File: VL033952.D

Acq: 25 Jun 2019 1:16

Instrument :

MSVOA_L

ClientSampleId :

TZC-SSDS-AREA-D-1

Tot Ion: 45 Resp: 144837

Ion Ratio Lower Upper

45 100





46 37.8 15.3 61.1

Manual Integrations

APPROVED

MMDadoda

6/26/2019 8:15:51 AM

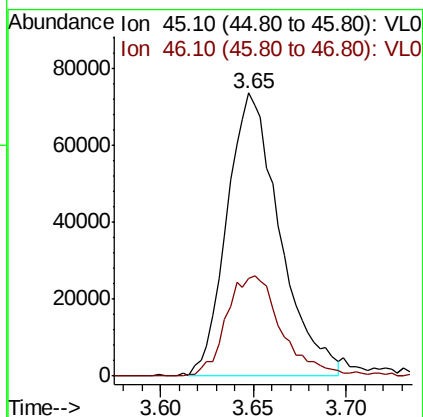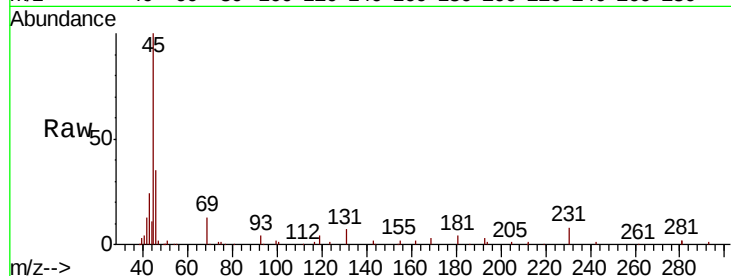

#15

Acetone

Concen: 152.443 ppbv

RT: 3.89 min Scan# 296

Delta R.T. -0.00 min

Lab File: VL033952.D




Acq: 25 Jun 2019 1:16


Tgt Ion: 43 Resp:19791748

Ion Ratio Lower Upper

43 100

58 44.1 21.3 31.9#

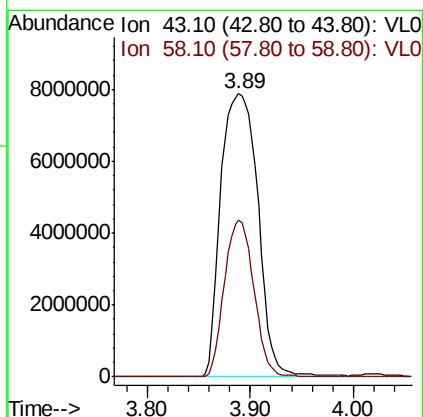

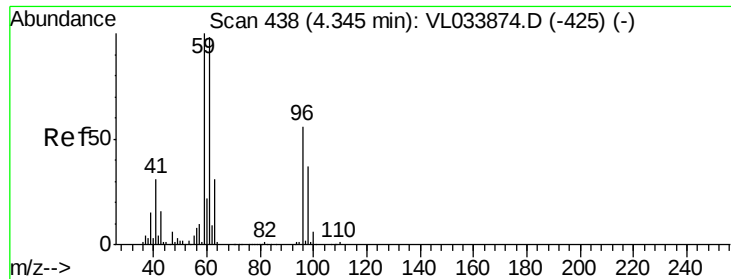

#17





tert-Butyl alcohol
Concen: 31.758 ppbv
RT: 4.35 min Scan# 439
Delta R.T. 0.00 min
Lab File: VL033952.D
Acq: 25 Jun 2019 1:16

Instrument :
MSVOA_L
ClientSampleId :
TZC-SSDS-AREA-D-1

Tot Ion: 59 Resp: 3223182
Ion Ratio Lower Upper
59 100
57 11.1 8.4 12.6

Manual Integrations
APPROVED




MMDadoda
6/26/2019 8:15:51 AM

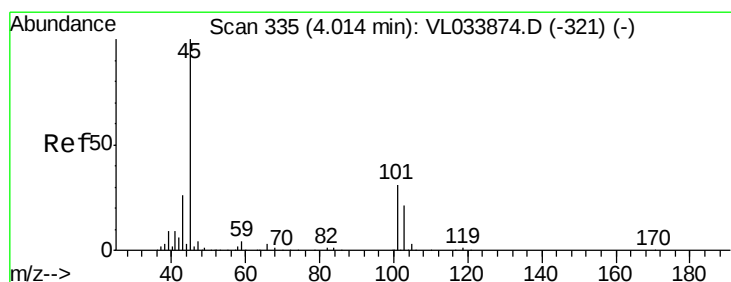
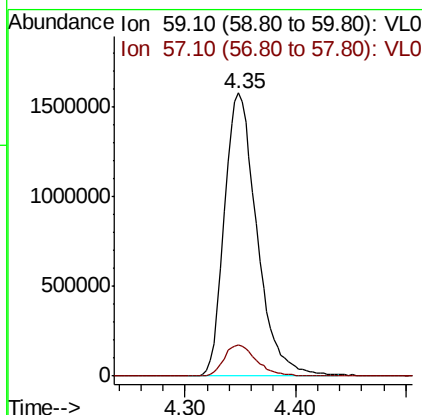
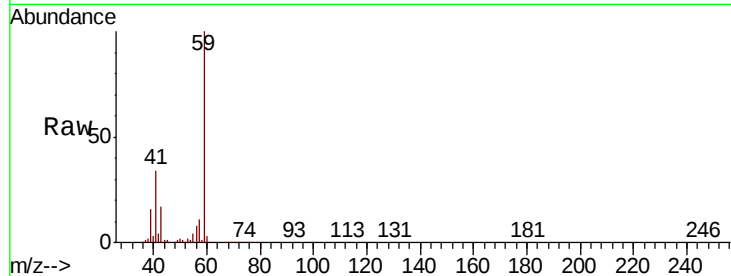


#19

Isopropyl Alcohol
Concen: 5.628 ppbv
RT: 4.02 min Scan# 337
Delta R.T. 0.01 min
Lab File: VL033952.D
Acq: 25 Jun 2019 1:16

Tgt Ion: 45 Resp: 417395
Ion Ratio Lower Upper
45 100
58 0.0 1.8 2.6#

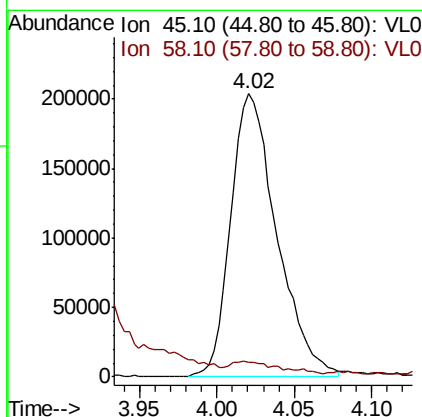

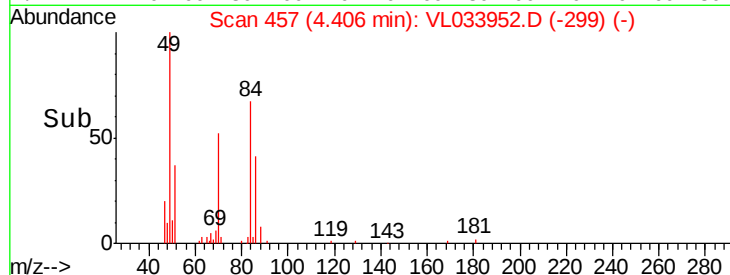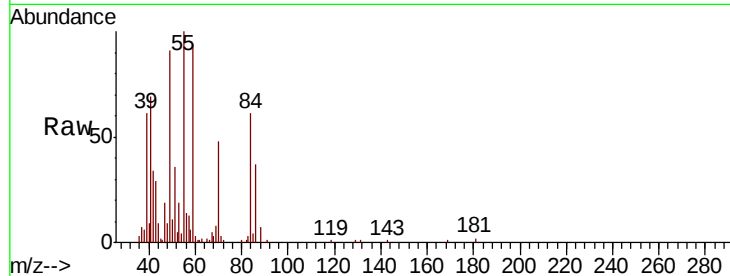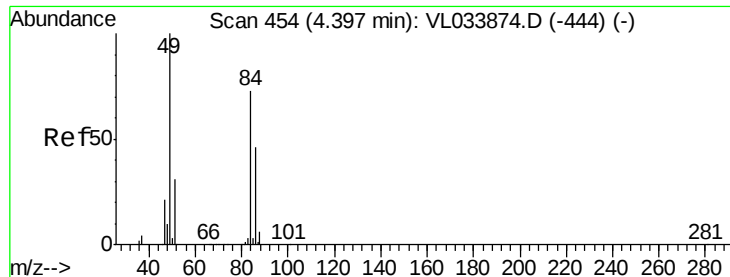





#20
Methvlene Chloride
Concen: 0.841 ppbv
RT: 4.41 min Scan# 457
Delta R.T. 0.01 min
Lab File: VL033952.D
Acq: 25 Jun 2019 1:16

Tot Ion	Ion	Ratio	Lower	Upper
84	100			
49	148.7	110.0	165.0	
51	58.1	34.6	51.8	
86	61.7	50.6	75.8	

Instrument :
MSVOA_L
ClientSampleId :
TZC-SSDS-AREA-D-1


Manual Integrations
APPROVED


MMDadoda
6/26/2019 8:15:51 AM

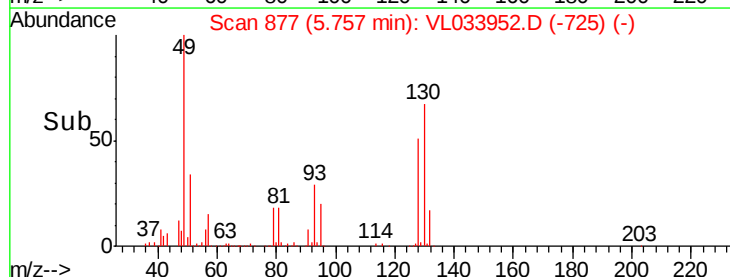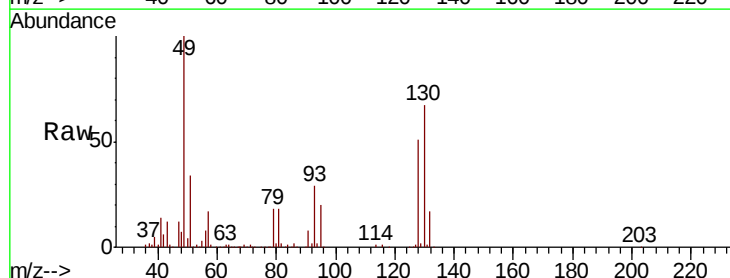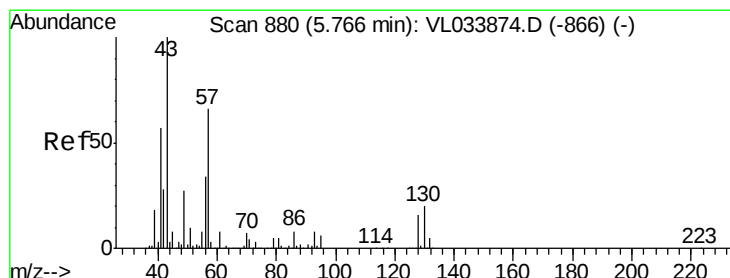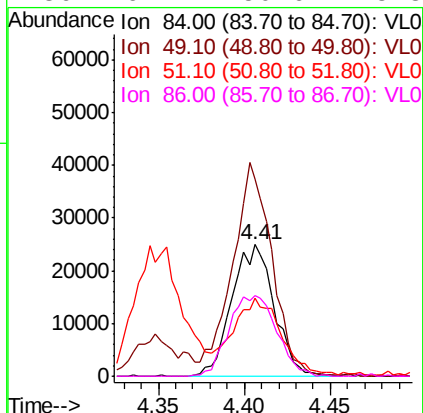

#26
Hexane
Concen: 1.443 ppbv
RT: 5.76 min Scan# 877
Delta R.T. -0.01 min
Lab File: VL033952.D
Acq: 25 Jun 2019 1:16

Tgt Ion	Ion	Ratio	Lower	Upper
57	100			
41	93.6	71.4	107.2	
43	76.7	183.7	275.5	
56	55.2	42.7	64.1	

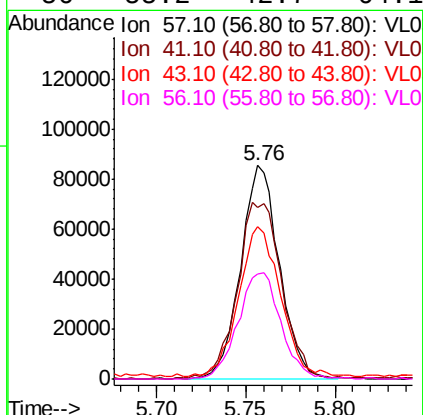







#27
Carbon Disulfide
Concen: 0.870 ppbv
RT: 4.60 min Scan# 518
Delta R.T. -0.01 min
Lab File: VL033952.D
Acq: 25 Jun 2019 1:16

Instrument :
MSVOA_L
ClientSampleId :
TZC-SSDS-AREA-D-1

Tot Ion	Ratio	Lower	Upper
76	100		
44	21.0	14.4	21.6
78	9.3	7.5	11.3




Manual Integrations
APPROVED


MMDadoda
6/26/2019 8:15:51 AM

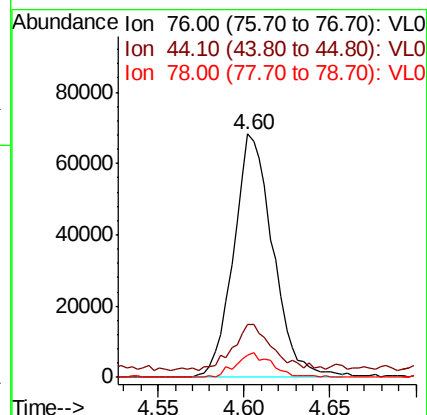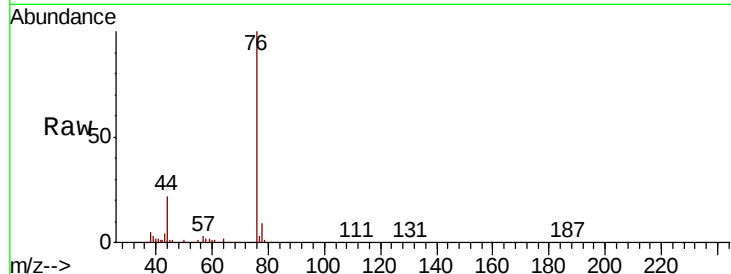

#29
Chloroform
Concen: 0.221 ppbv
RT: 5.84 min Scan# 903
Delta R.T. 0.00 min
Lab File: VL033952.D
Acq: 25 Jun 2019 1:16

Tgt Ion	Ratio	Lower	Upper
83	100		
85	68.4	50.5	75.7

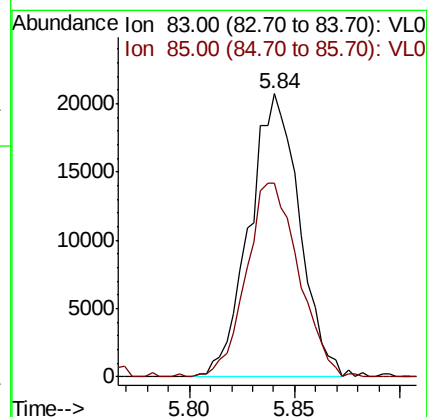

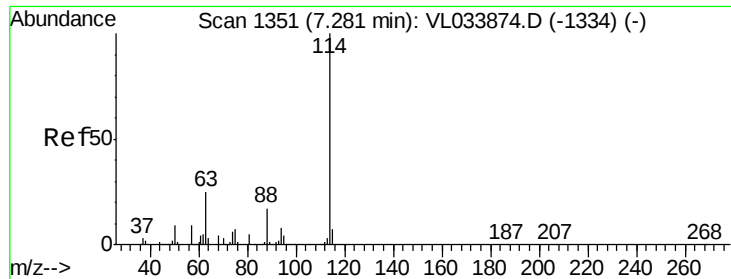





#33
 1,4-Difluorobenzene
 Concen: 10.000 ppbv
 RT: 7.28 min Scan# 1350
 Delta R.T. -0.00 min
 Lab File: VL033952.D
 Acq: 25 Jun 2019 1:16

Instrument :
 MSVOA_L
 ClientSampleId :
 TZC-SSDS-AREA-D-1

Tot Ion	Ratio	Lower	Upper
114	100		
63	25.2	21.1	31.7
88	17.8	14.2	21.4




Manual Integrations
 APPROVED


MMDadoda
 6/26/2019 8:15:51 AM

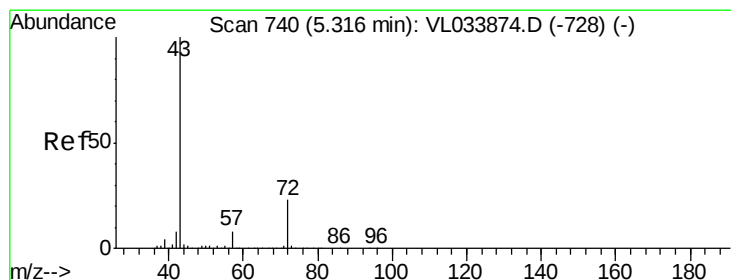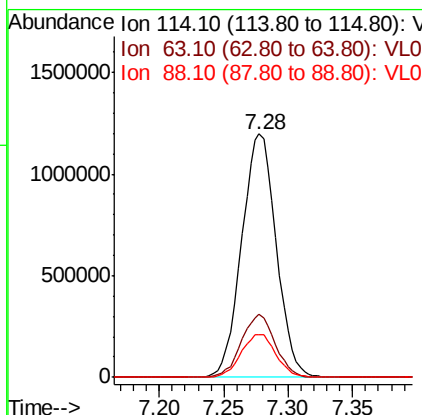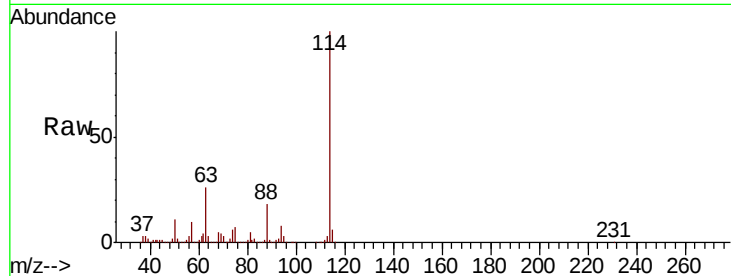

#34
 2-Butanone
 Concen: 19.159 ppbv
 RT: 5.31 min Scan# 739
 Delta R.T. -0.00 min
 Lab File: VL033952.D
 Acq: 25 Jun 2019 1:16

Tgt Ion	Ratio	Lower	Upper
43	100		
72	22.7	17.9	26.9

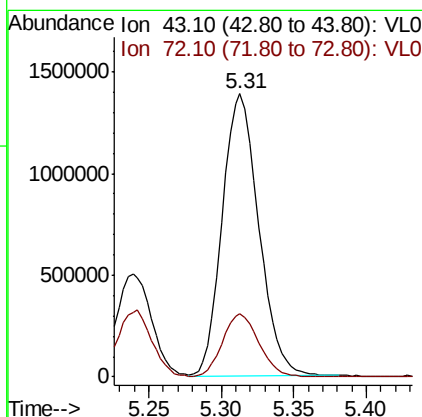

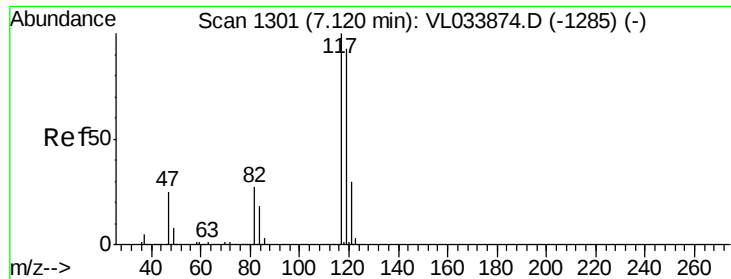





#35
Carbon Tetrachloride
Concen: 0.053 ppbv m
RT: 7.11 min Scan# 1299
Delta R.T. -0.01 min
Lab File: VL033952.D
Acq: 25 Jun 2019 1:16

Instrument :
MSVOA_L
ClientSampleId :
TZC-SSDS-AREA-D-1

Tot Ion	Ratio	Lower	Upper
117	100		
119	79.8	74.6	111.8
121	26.2	24.0	36.0




Manual Integrations
APPROVED


MMDadoda
6/26/2019 8:15:51 AM

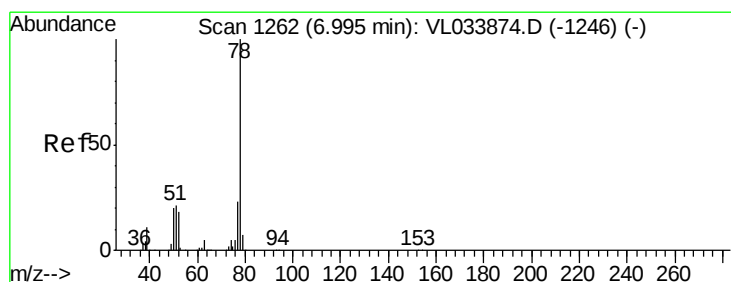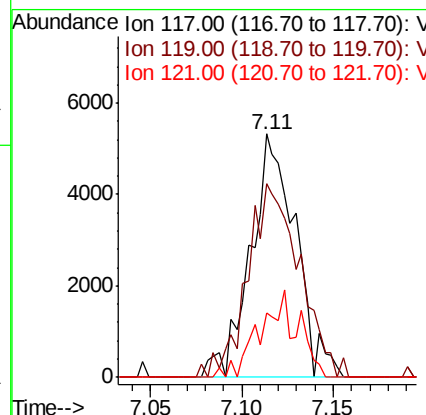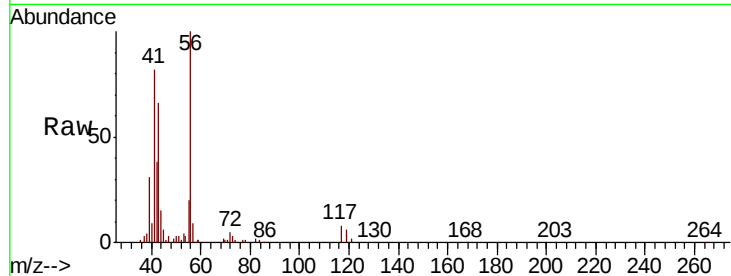

#36
Benzene
Concen: 11.319 ppbv
RT: 6.99 min Scan# 1261
Delta R.T. -0.00 min
Lab File: VL033952.D
Acq: 25 Jun 2019 1:16

Tgt Ion	Ratio	Lower	Upper
78	100		
77	22.2	18.2	27.2
50	18.9	15.9	23.9

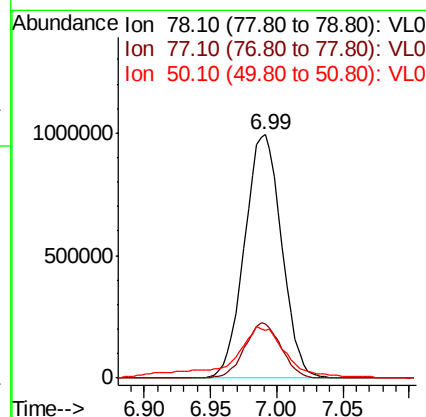







#38
 Trichloroethene
 Concen: 0.409 ppbv
 RT: 7.95 min Scan# 1558
 Delta R.T. -0.00 min
 Lab File: VL033952.D
 Acq: 25 Jun 2019 1:16

Instrument :
 MSVOA_L
 ClientSampleId :
 TZC-SSDS-AREA-D-1

Tot Ion	Ratio	Lower	Upper
130	100		
95	110.2	92.0	138.0
132	88.8	73.8	110.8
97	61.8	57.2	85.8




Manual Integrations
 APPROVED


MMDadoda
 6/26/2019 8:15:51 AM

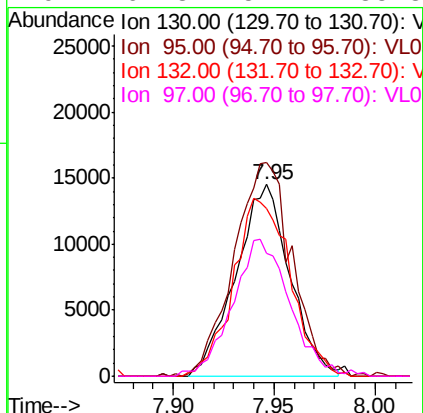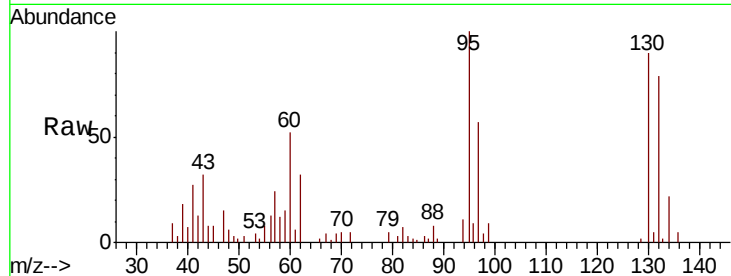

#52
 Tetrachloroethene
 Concen: 2.791 ppbv
 RT: 11.35 min Scan# 2616
 Delta R.T. -0.01 min
 Lab File: VL033952.D
 Acq: 25 Jun 2019 1:16

Tgt Ion	Ratio	Lower	Upper
164	100		
166	120.3	103.1	154.7
129	98.7	83.9	125.9
131	93.0	85.1	127.7

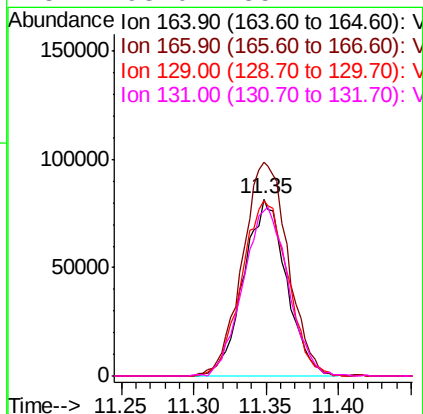



#53

Toluene

Concen: 14.191 ppbv

RT: 9.92 min Scan# 2173

Delta R.T. -0.01 min

Lab File: VL033952.D

Acq: 25 Jun 2019 1:16

Instrument :

MSVOA_L

ClientSampleId :

TZC-SSDS-AREA-D-1

Tot Ion: 91 Resp: 2681810

Ion Ratio Lower Upper

91 100





92 59.9 47.0 70.6

Manual Integrations

APPROVED

MMDadoda

6/26/2019 8:15:51 AM

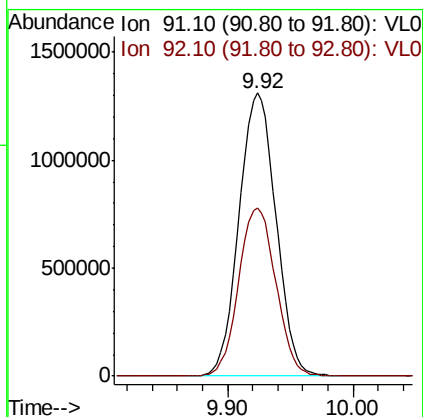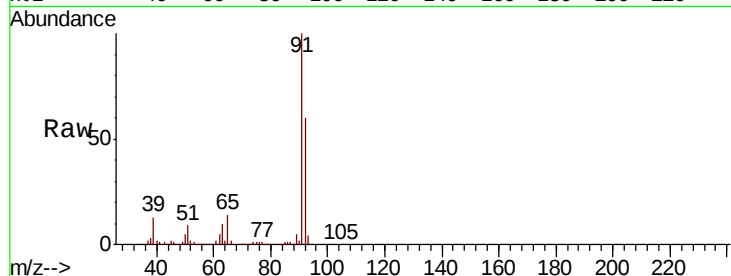

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 12.22 min Scan# 2886

Delta R.T. -0.01 min

Lab File: VL033952.D

Acq: 25 Jun 2019 1:16




Tgt Ion: 117 Resp: 2240413


Ion Ratio Lower Upper

117 100

82 65.1 50.2 75.2

119 32.5 24.8 37.2

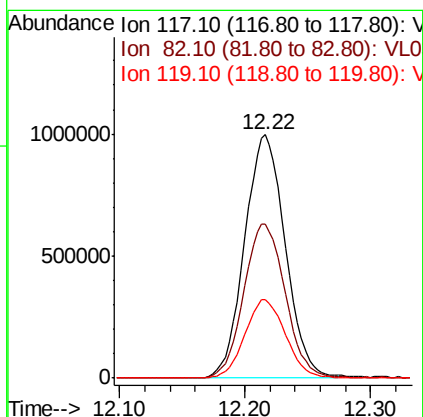

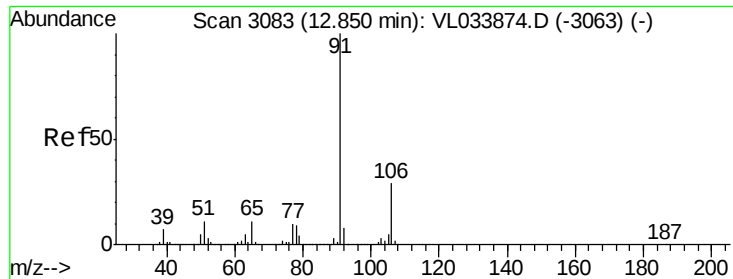





#58
Ethyl Benzene
Concen: 49.296 ppbv
RT: 12.84 min Scan# 3081
Delta R.T. -0.01 min
Lab File: VL033952.D
Acq: 25 Jun 2019 1:16

Instrument :
MSVOA_L
ClientSampleId :
TZC-SSDS-AREA-D-1

Tot Ion: 91 Resp:12451876
Ion Ratio Lower Upper
91 100
106 34.0 23.0 34.6




Manual Integrations
APPROVED


MMDadoda
6/26/2019 8:15:51 AM

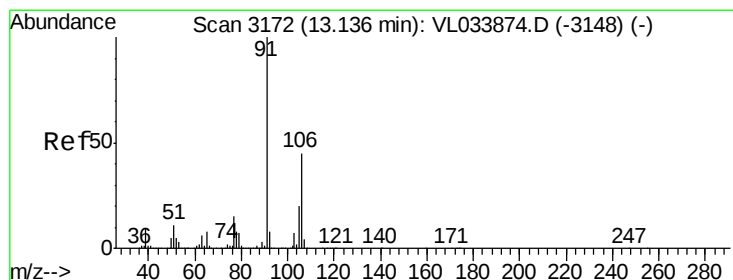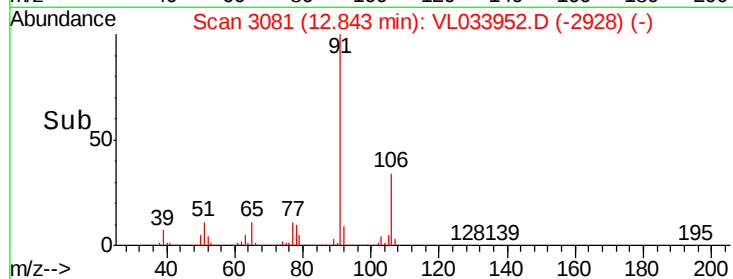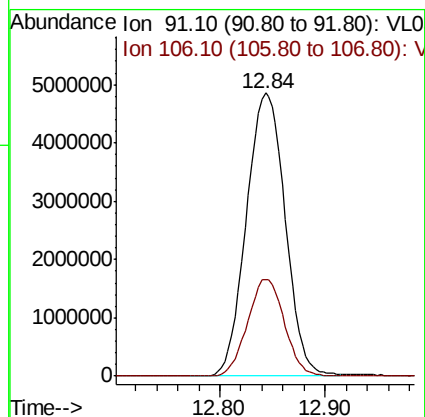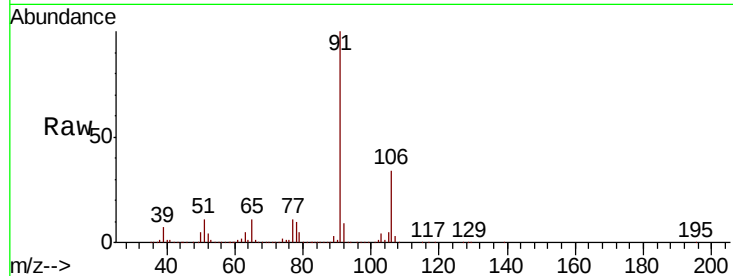

#59
m/p-Xylene
Concen: 120.580 ppbv
RT: 13.11 min Scan# 3165
Delta R.T. -0.02 min
Lab File: VL033952.D
Acq: 25 Jun 2019 1:16

Tgt Ion: 91 Resp:27697221
Ion Ratio Lower Upper
91 100
106 55.6 35.8 53.8#

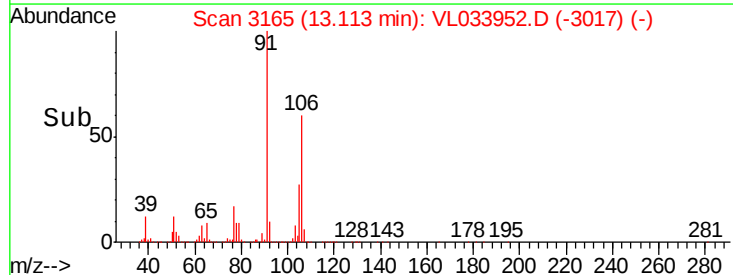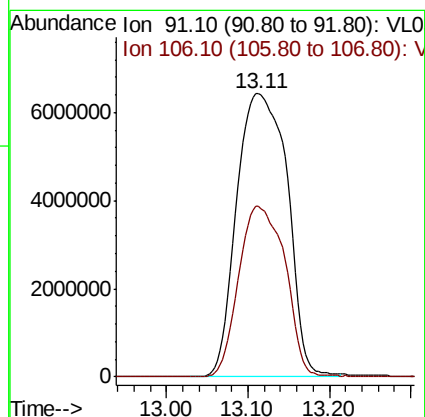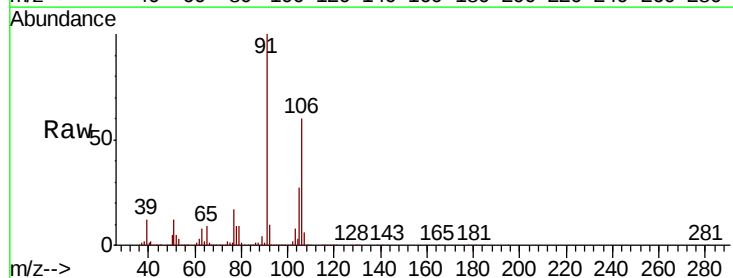



#60

o-Xylene

Concen: 61.588 ppbv

RT: 13.83 min Scan# 3389

Delta R.T. -0.00 min

Lab File: VL033952.D

Acq: 25 Jun 2019 1:16

Instrument :

MSVOA_L

ClientSampleId :

TZC-SSDS-AREA-D-1

Tot Ion: 91 Resp:14606422





Ion Ratio Lower Upper

91 100

106 49.1 21.7 65.1

Manual Integrations
APPROVED

MMDadoda
6/26/2019 8:15:51 AM

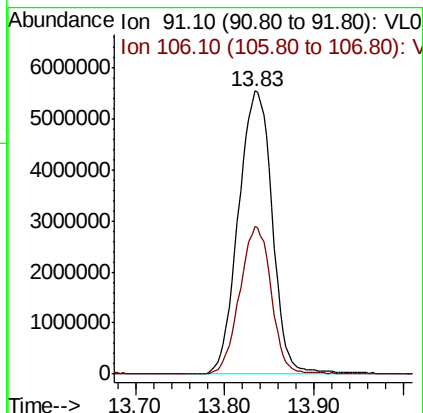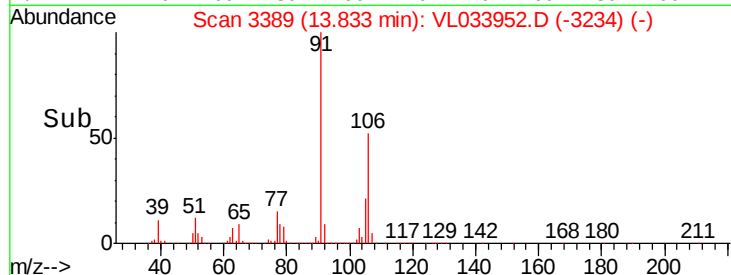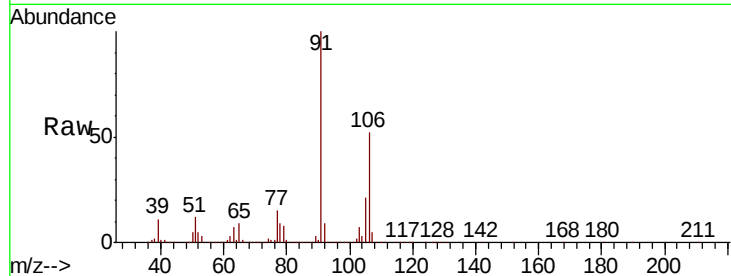

#61

Styrene

Concen: 108.303 ppbv

RT: 13.68 min Scan# 3340

Delta R.T. 0.00 min

Lab File: VL033952.D

Acq: 25 Jun 2019 1:16




Tgt Ion:104 Resp:16622104


Ion Ratio Lower Upper

104 100

78 51.7 43.4 65.0

103 51.2 37.6 56.4

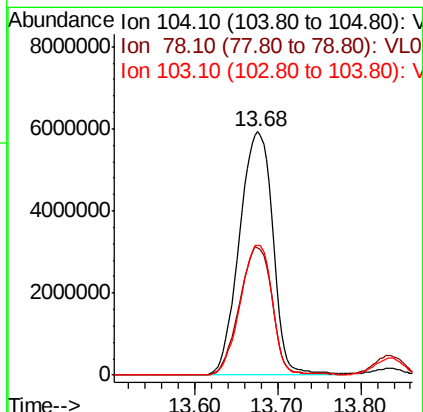

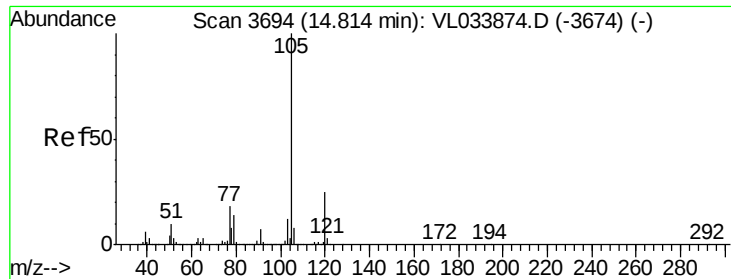

#62

Isopropylbenzene

Concen: 1.277 ppbv

RT: 14.80 min Scan# 3691

Delta R.T. -0.01 min

Lab File: VL033952.D

Acq: 25 Jun 2019 1:16

Instrument :

MSVOA_L

ClientSampleId :

TZC-SSDS-AREA-D-1

Tot Ion:105 Resp: 408141

Ion Ratio Lower Upper





105 100

120 25.8 20.3 30.5

Manual Integrations
APPROVED

MMDadoda

6/26/2019 8:15:51 AM

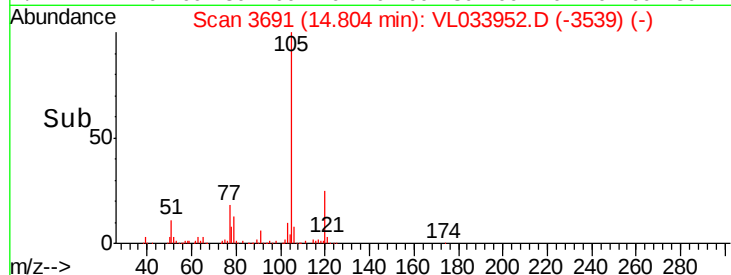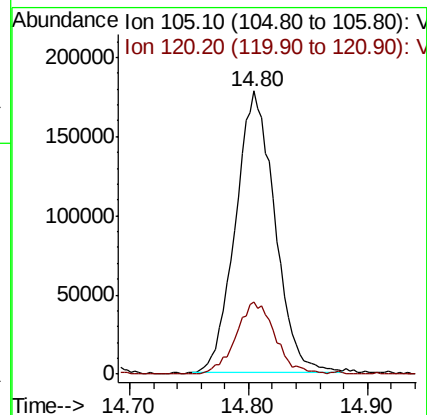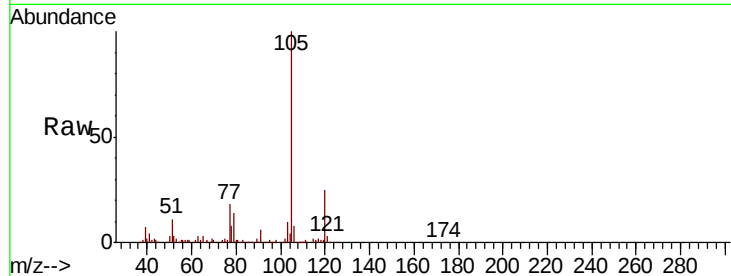

#64

n-propylbenzene

Concen: 1.336 ppbv

RT: 15.70 min Scan# 3969

Delta R.T. -0.01 min

Lab File: VL033952.D




Acq: 25 Jun 2019 1:16


Tgt Ion:120 Resp: 109359

Ion Ratio Lower Upper

120 100

91 521.6 387.0 580.6

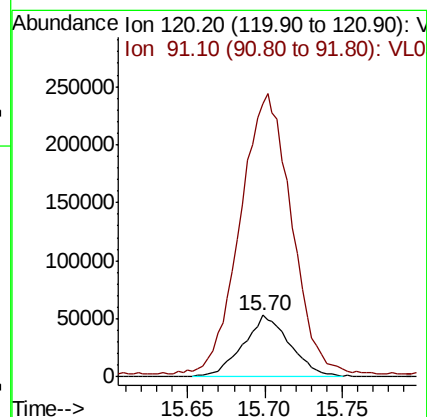







#68
 1-Bromo-4-Fluorobenzene
 Concen: 10.772 ppbv
 RT: 14.56 min Scan# 3614
 Delta R.T. -0.01 min
 Lab File: VL033952.D
 Acq: 25 Jun 2019 1:16

Instrument :
 MSVOA_L
 ClientSampleId :
 TZC-SSDS-AREA-D-1

Tot Ion: 95 Resp: 1982295
 Ion Ratio Lower Upper
 95 100
 174 68.5 54.0 81.0
 175 5.0 3.8 5.8




Manual Integrations
 APPROVED


MMDadoda
 6/26/2019 8:15:51 AM

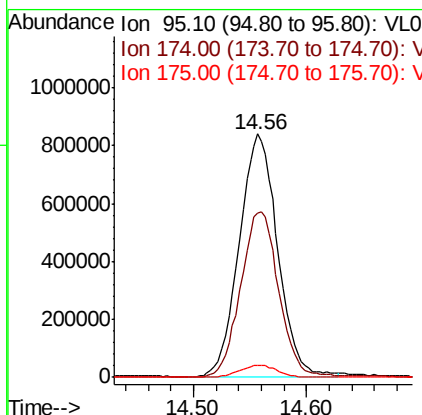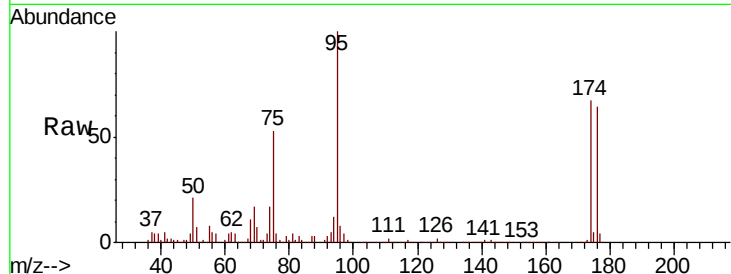

#70
 n-Butylbenzene
 Concen: 0.147 ppbv
 RT: 18.69 min Scan# 4900
 Delta R.T. -0.01 min
 Lab File: VL033952.D
 Acq: 25 Jun 2019 1:16

Tgt Ion: 91 Resp: 55456
 Ion Ratio Lower Upper
 91 100
 92 48.8 42.5 63.7
 134 31.7 17.8 26.6#

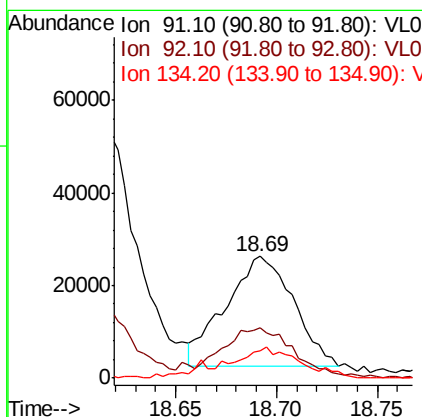

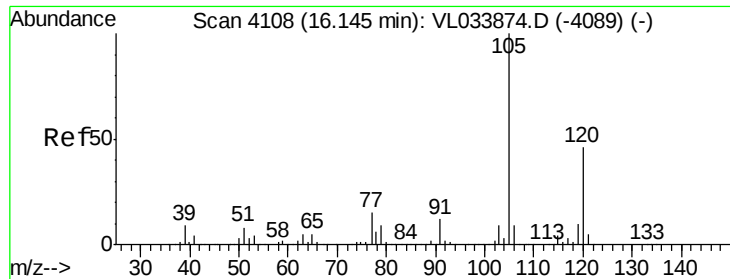

#73

1,3,5-Trimethylbenzene

Concen: 0.124 ppbv

RT: 16.14 min Scan# 4105

Delta R.T. -0.01 min

Lab File: VL033952.D

Acq: 25 Jun 2019 1:16

Instrument :

MSVOA_L

ClientSampleId :

TZC-SSDS-AREA-D-1

Tot Ion:105 Resp: 33018

Ion Ratio Lower Upper

105 100


120 33.0 37.1 55.7#

Manual Integrations

APPROVED

MMDadoda

6/26/2019 8:15:51 AM

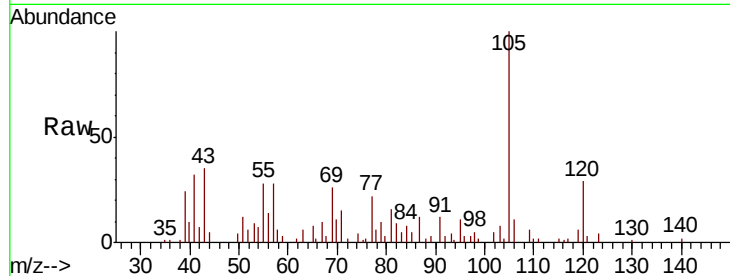

Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

16.14



15000

10000

5000

0

Time--> 16.05 16.10 16.15 16.20

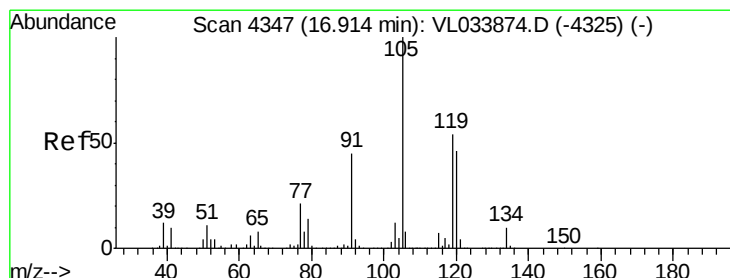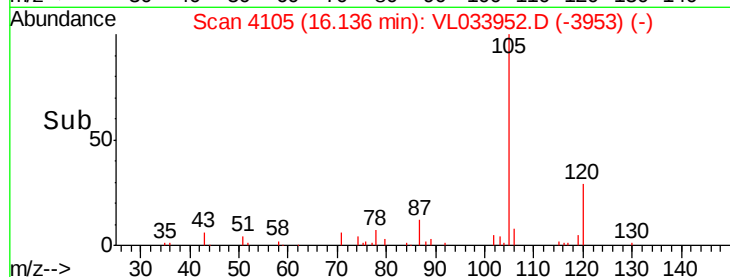

#74

1,2,4-Trimethylbenzene

Concen: 0.285 ppbv m

RT: 16.90 min Scan# 4343

Delta R.T. -0.01 min

Lab File: VL033952.D

Acq: 25 Jun 2019 1:16

Tgt Ion:105 Resp: 87425


Ion Ratio Lower Upper

105 100

120 37.6 36.7 55.1

91 15.4 35.8 53.8#

77 18.9 16.9 25.3

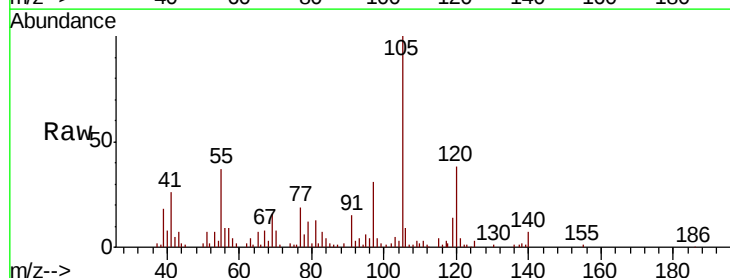

Abundance Ion 105.10 (104.80 to 105.80): V

Ion 120.20 (119.90 to 120.90): V

Ion 91.10 (90.80 to 91.80): VLO

Ion 77.10 (76.80 to 77.80): VLO

16.90

60000

50000

40000


30000


20000

10000

0

Time--> 16.80 16.85 16.90 16.95

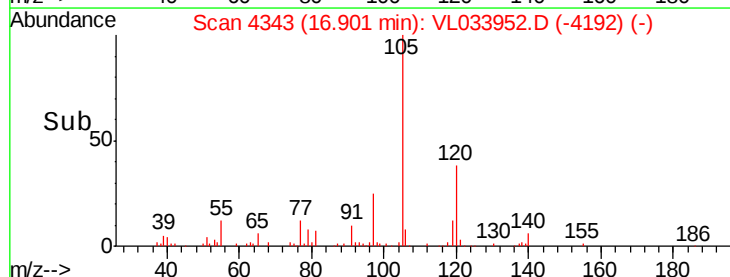

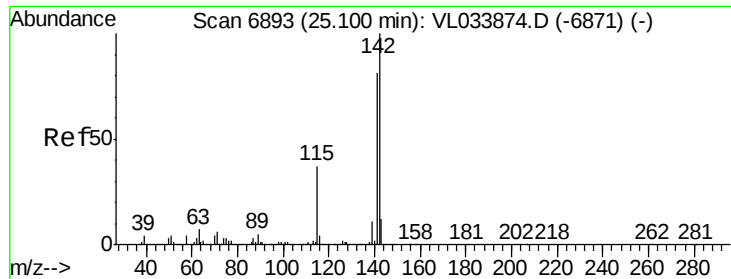

#80
Naphthalene, 2-methyl-
Concen: 0.056 ppbv
RT: 25.09 min Scan# 6889
Delta R.T. -0.01 min
Lab File: VL033952.D
Acq: 25 Jun 2019 1:16

Instrument :
MSVOA_L
ClientSampleId :
TZC-SSDS-AREA-D-1

Tot Ion	Ratio	Lower	Upper
142	100		
141	87.5	65.7	98.5
115	93.4	28.9	43.3

Manual Integrations
APPROVED

MMDadoda
6/26/2019 8:15:51 AM

