


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL062419\
 Data File : VL033929.D
 Acq On : 24 Jun 2019 8:39
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL060719AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Jun 07 08:53:27 2019
 Last Update : Fri Jun 07 08:53:27 2019

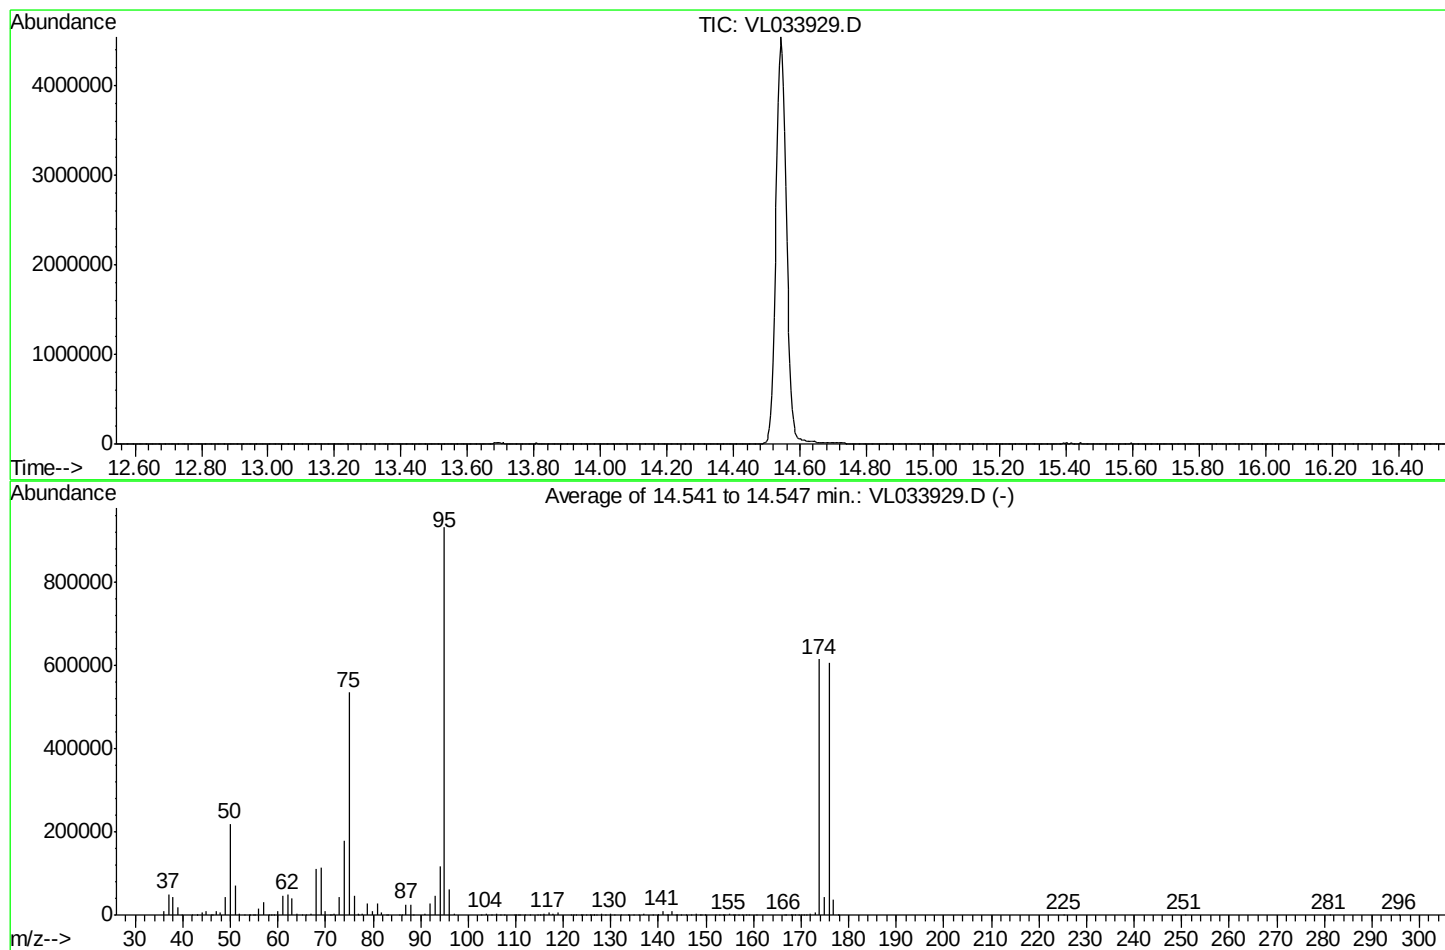

AutoFind: Scans 3609, 3610, 3611; Background Corrected with Scan 3585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.5	218901	PASS
75	95	30	66	57.3	534656	PASS
95	95	100	100	100.0	932394	PASS
96	95	5	9	6.5	61005	PASS
173	174	0.00	2	1.0	5878	PASS
174	95	50	120	66.0	615189	PASS
175	174	4	9	7.2	44213	PASS
176	174	93	101	98.6	606784	PASS
177	176	5	9	6.3	38138	PASS