
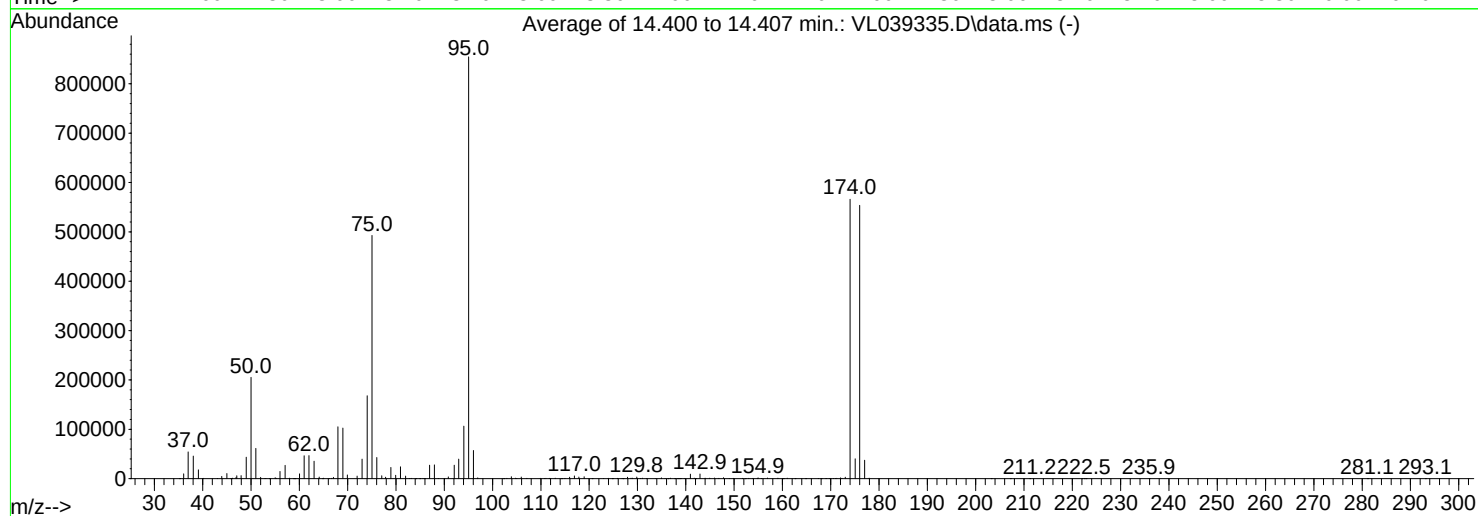


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062422\
 Data File : VL039335.D
 Acq On : 24 Jun 2022 8:43
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL053122AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jun 01 01:22:18 2022
 Last Update : Wed Jun 01 01:22:18 2022

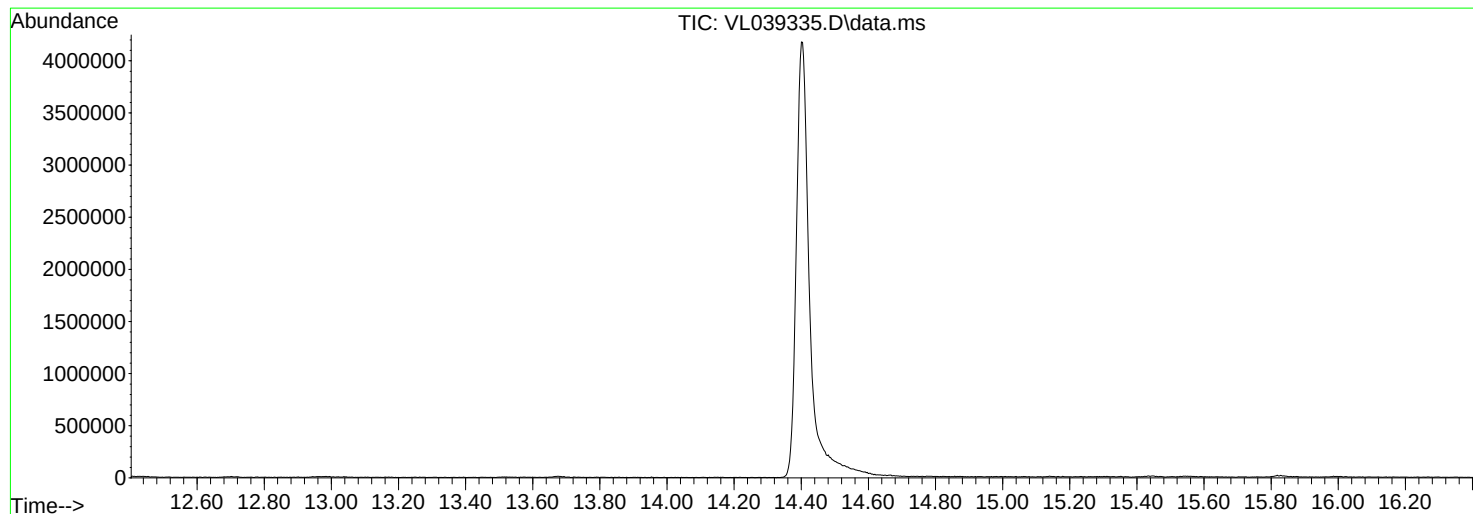

AutoFind: Scans 3612, 3613, 3614; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.0	205120	PASS
75	95	30	66	57.7	492736	PASS
95	95	100	100	100.0	854592	PASS
96	95	5	9	6.7	56952	PASS
173	174	0.00	2	0.5	2943	PASS
174	95	50	120	66.2	566101	PASS
175	174	4	9	7.1	40085	PASS
176	174	93	101	97.8	553643	PASS
177	176	5	9	6.8	37435	PASS

Average of 14.400 to 14.407 min.: VL039335.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.20	68	46.90	2360	55.20	704	64.80	10
36.05	9835	47.05	5825	56.00	14614	65.05	89
37.00	54163	47.95	6059	57.05	26923	66.20	27
38.05	45843	49.00	43403	58.00	932	66.70	68
39.10	17738	50.00	205120	58.80	91	67.05	2574
40.10	576	51.00	61373	59.10	69	68.00	105112
43.05	452	52.00	2592	60.05	9652	69.00	102488
43.95	4523	52.90	327	61.00	46216	69.95	7509
45.00	10248	53.10	250	62.00	46603	71.95	5373
45.80	188	53.80	148	63.05	35312	73.00	39445
46.15	876	55.00	1958	64.10	3220	74.05	168000

Average of 14.400 to 14.407 min.: VL039335.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.05	492736	84.90	123	94.05	106389	109.90	685
76.05	42923	85.60	295	95.05	854592	110.70	426
77.05	5748	85.90	248	96.05	56952	111.05	598
77.85	2913	86.10	385	96.95	1741	111.75	552
78.95	22688	86.95	27179	102.30	163	112.05	484
79.95	6732	87.95	27808	102.95	755	112.95	919
80.95	24011	88.80	379	103.90	3803	114.30	51
82.00	5105	90.05	258	104.80	843	115.00	548
82.80	265	90.85	3516	105.00	389	115.95	3093
83.15	624	92.05	27181	105.95	3316	116.95	5560
84.10	160	93.00	39736	107.10	657	117.85	3375

Average of 14.400 to 14.407 min.: VL039335.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.95	3766	129.00	998	138.30	90	146.85	686
120.60	53	129.85	3178	138.70	127	147.80	2069
123.00	481	130.60	253	139.05	397	149.00	360
123.95	662	131.00	1069	139.70	380	149.85	570
124.80	119	131.90	231	140.95	9052	151.75	697
124.95	264	133.80	249	141.75	882	152.30	79
125.85	556	134.95	1687	142.00	144	153.05	756
126.80	313	135.70	292	142.95	9551	153.90	666
127.00	127	136.30	69	144.00	899	154.80	347
127.95	3006	136.85	1132	144.95	950	154.95	1669
128.65	897	137.70	52	145.95	1324	155.70	233

Average of 14.400 to 14.407 min.: VL039335.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
156.90	1272	170.00	399	177.95	1099		
159.05	1043	170.60	284	203.20	69		
160.20	103	171.00	258	207.20	60		
161.00	923	171.25	712	211.20	78		
162.60	109	172.00	1701	222.00	74		
164.80	148	172.30	818	222.50	173		
167.45	247	173.00	2943	222.85	144		
168.00	79	174.00	566101	235.90	83		
169.00	360	175.05	40085	281.10	152		
169.15	255	176.00	553643	293.10	72		
169.70	279	177.00	37435				