

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_L\DATA\VL062619\  
Quantitation Report (Not Reviewed)

Data File : VL033968.D  
Acq On : 26 Jun 2019 15:20  
Operator : SY/AP  
Sample : QC062019 CAN 10267  
Misc : 400ml/MSVOA\_L  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_L  
ClientSampleId :  
QC062019 CAN 10267

Quant Time: Jun 27 01:23:12 2019  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_L\METHODS\VL060719AIR.M  
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA\_L Fri Jun 07 08:53:27 2019  
QLast Update : Fri Jun 07 08:53:27 2019  
Response via : Initial Calibration

| Internal Standards      | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|-------------------------|-------|------|----------|-------|-------|----------|
| 1) Bromochloromethane   | 5.74  | 49   | 770360   | 10.00 | ppbv  | -0.02    |
| 33) 1,4-Difluorobenzene | 7.26  | 114  | 1760469  | 10.00 | ppbv  | -0.02    |
| 55) Chlorobenzene-d5    | 12.21 | 117  | 1661487  | 10.00 | ppbv  | -0.02    |

System Monitoring Compounds

|                             |        |       |          |          |      |         |
|-----------------------------|--------|-------|----------|----------|------|---------|
| 68) 1-Bromo-4-Fluorobenzene | 14.54  | 95    | 1435078  | 10.52    | ppbv | -0.02   |
| Spiked Amount               | 10.000 | Range | 65 - 135 | Recovery | =    | 105.20% |


| Target Compounds        |      |    |        |       | Qvalue |    |
|-------------------------|------|----|--------|-------|--------|----|
| 15) Acetone             | 3.92 | 43 | 5449   | 0.048 | ppbv # | 86 |
| 19) Isopropyl Alcohol   | 4.06 | 45 | 1984   | 0.031 | ppbv # | 94 |
| 39) 1,2-Dichloropropane | 7.26 | 63 | 471523 | 9.085 | ppbv # | 25 |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VL033968.D  
Acq On : 26 Jun 2019 15:20  
Operator : SY/AP  
Sample : QC062019 CAN 10267  
Misc : 400ml/MSVOA\_L  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_L  
ClientSampleId :  
QC062019 CAN 10267

Quant Time: Jun 27 01:23:12 2019  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_L\METHODS\VL060719AIR.M  
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA\_L Fri Jun 07 08:53:27 2019  
QLast Update : Fri Jun 07 08:53:27 2019  
Response via : Initial Calibration

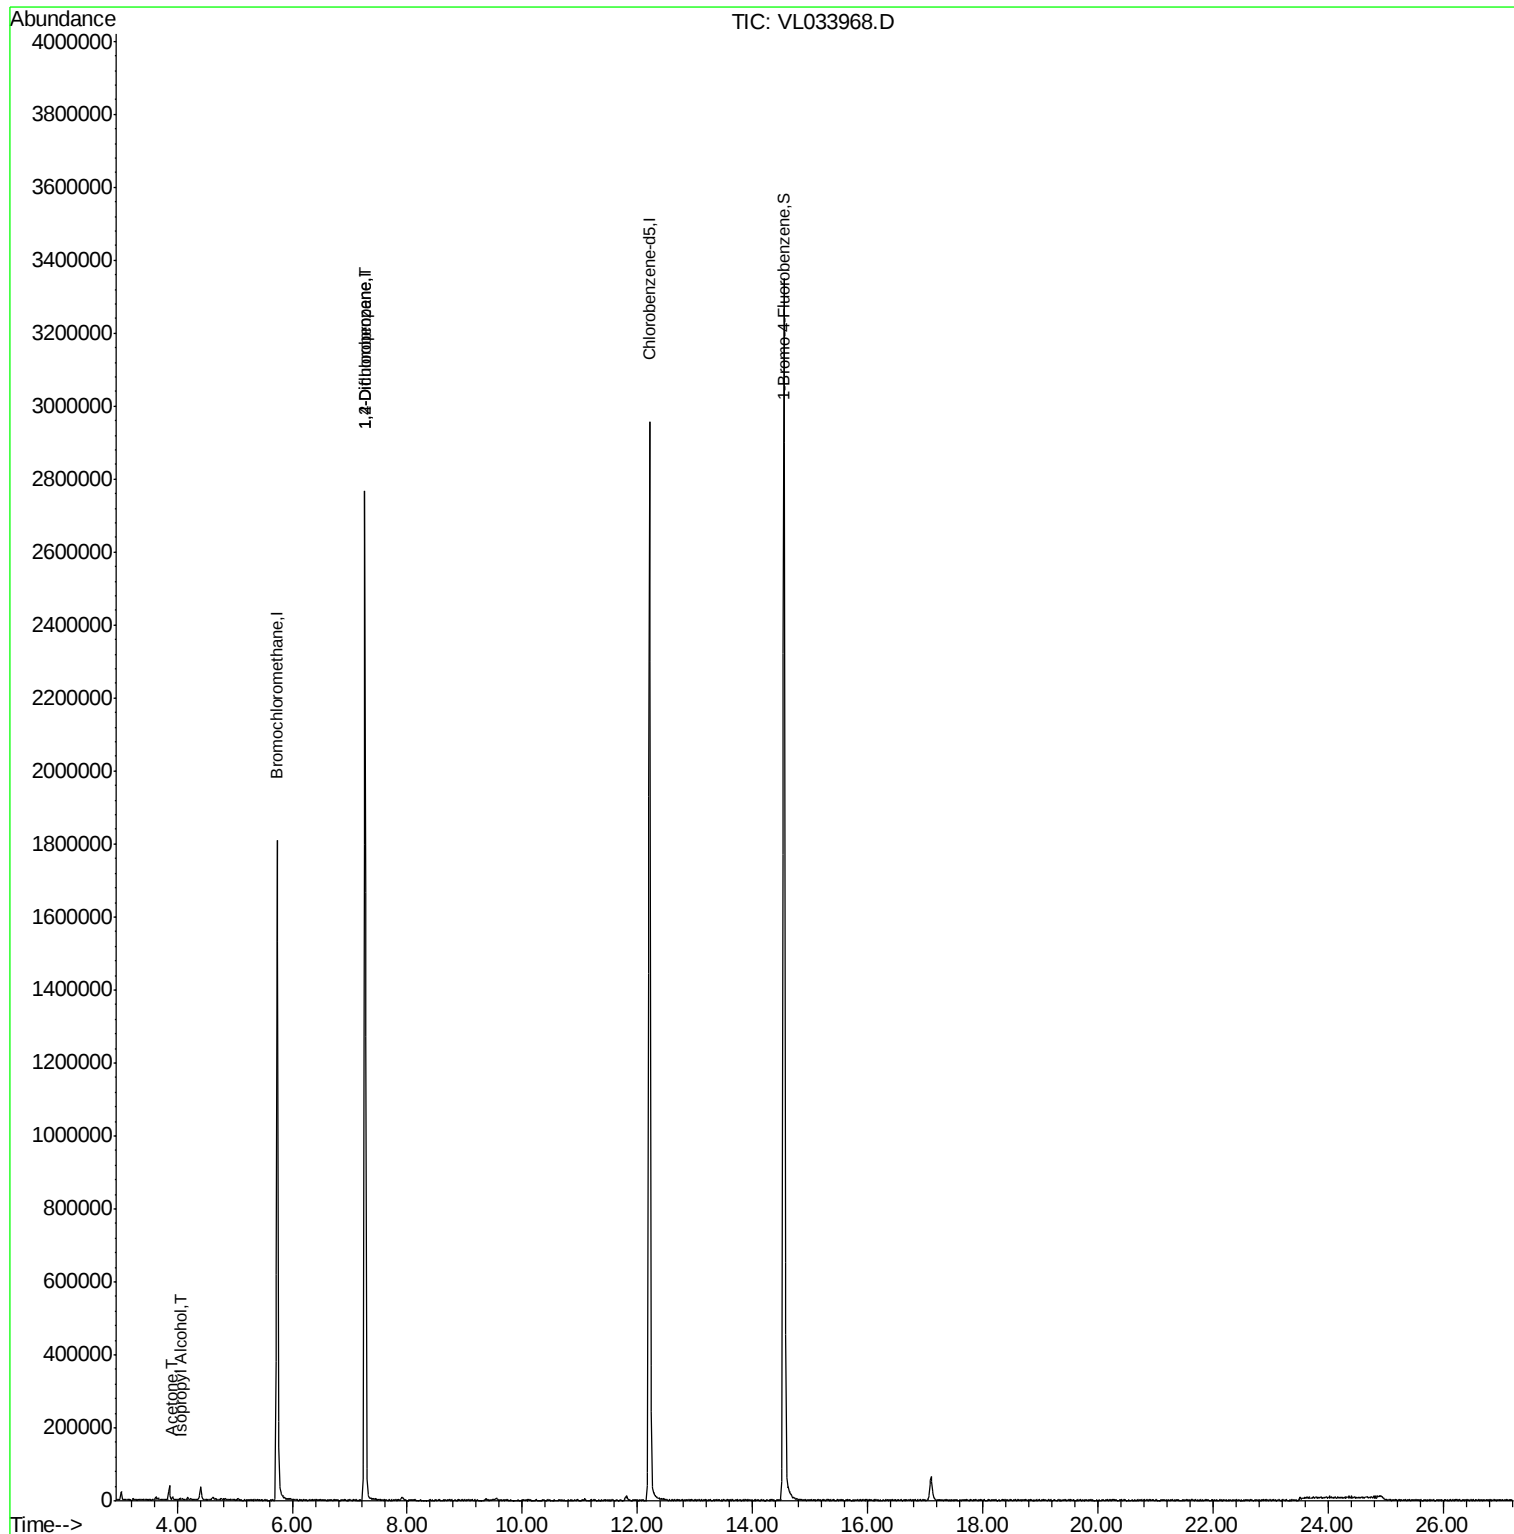

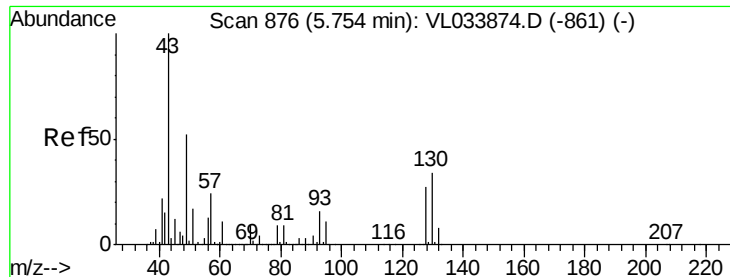

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.74 min Scan# 871

Delta R.T. -0.02 min

Lab File: VL033968.D

Acq: 26 Jun 2019 15:20

Instrument :

MSVOA\_L

ClientSampleId :

QC062019 CAN 10267


Tgt Ion: 49 Resp: 770360

Ion Ratio Lower Upper

49 100

128 51.6 25.5 76.5




130 65.2 32.5 97.4

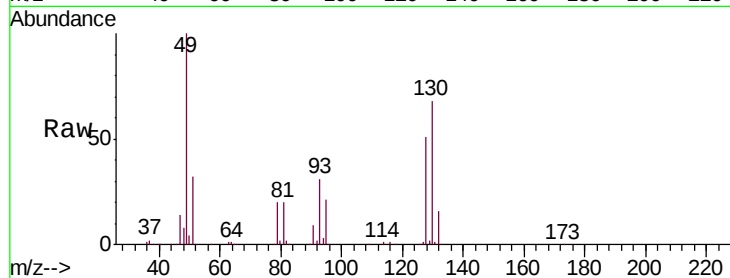

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

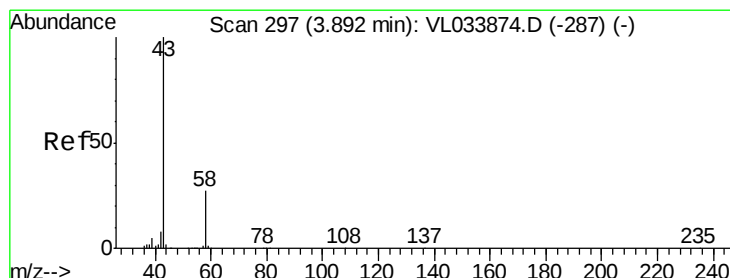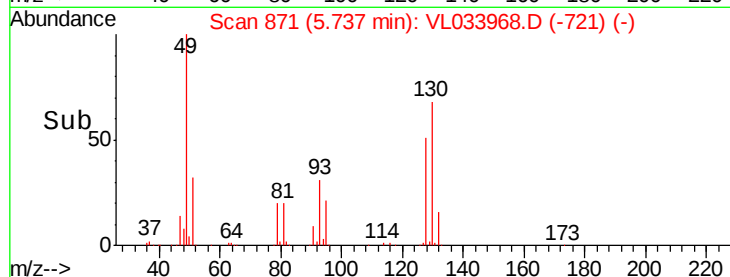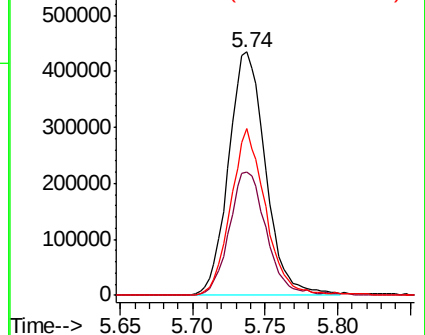

#15

Acetone

Concen: 0.048 ppbv

RT: 3.92 min Scan# 306

Delta R.T. 0.03 min

Lab File: VL033968.D


Acq: 26 Jun 2019 15:20

Tgt Ion: 43 Resp: 5449

Ion Ratio Lower Upper



43 100


58 33.9 21.3 31.9#

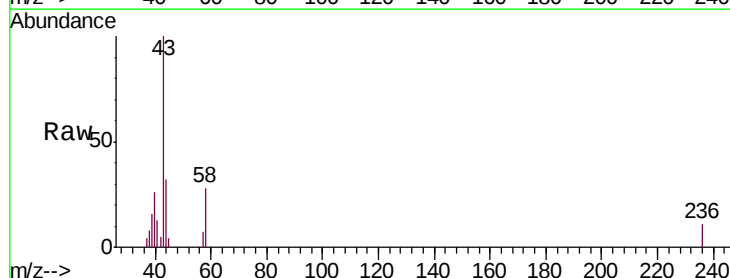

Abundance Ion 43.10 (42.80 to 43.80): VL0

Ion 58.10 (57.80 to 58.80): VL0

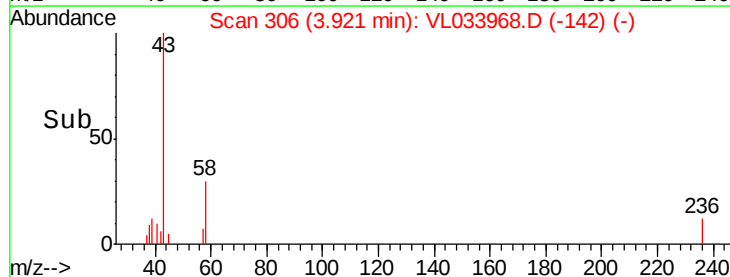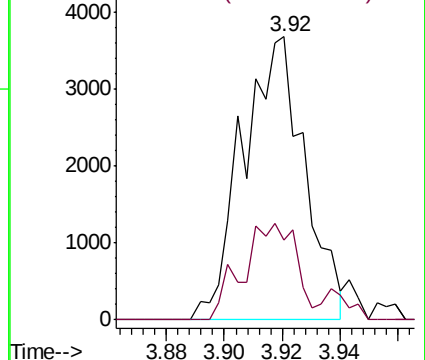

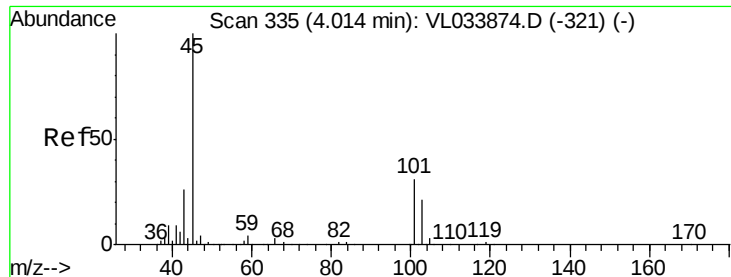

#19

Isopropyl Alcohol

Concen: 0.031 ppbv

RT: 4.06 min Scan# 349

Delta R.T. 0.04 min

Lab File: VL033968.D

Acq: 26 Jun 2019 15:20

Instrument :

MSVOA\_L

ClientSampleId :





QC062019 CAN 10267

Tgt Ion: 45 Resp: 1984

Ion Ratio Lower Upper

45 100

58 0.0 1.8 2.6#

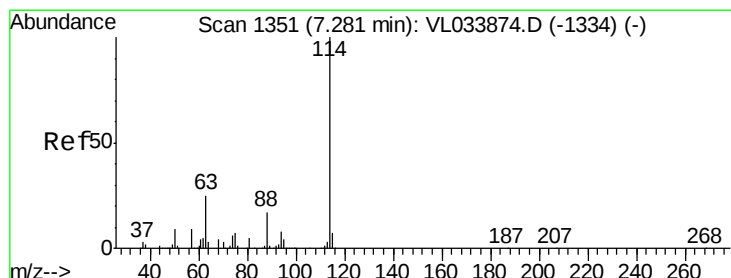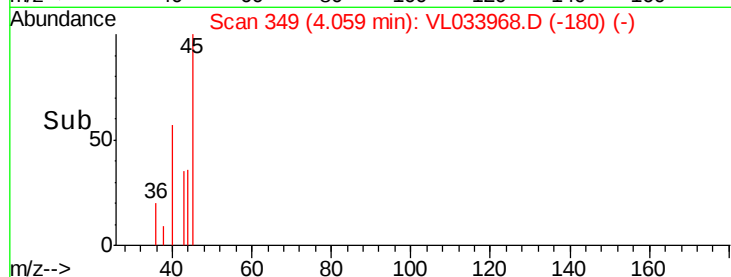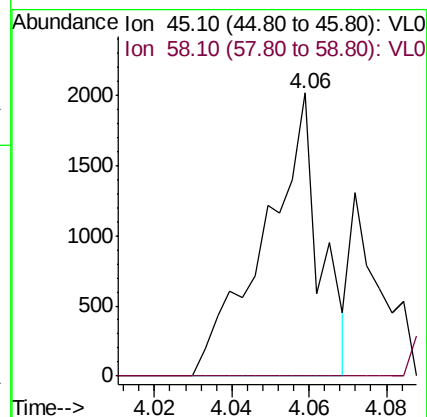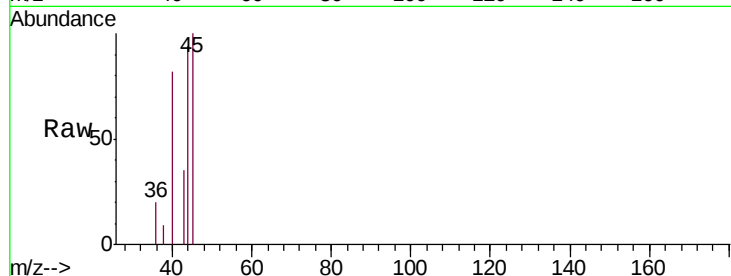

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.26 min Scan# 1345

Delta R.T. -0.02 min

Lab File: VL033968.D

Acq: 26 Jun 2019 15:20




Tgt Ion: 114 Resp: 1760469


Ion Ratio Lower Upper

114 100

63 26.9 21.1 31.7

88 18.2 14.2 21.4

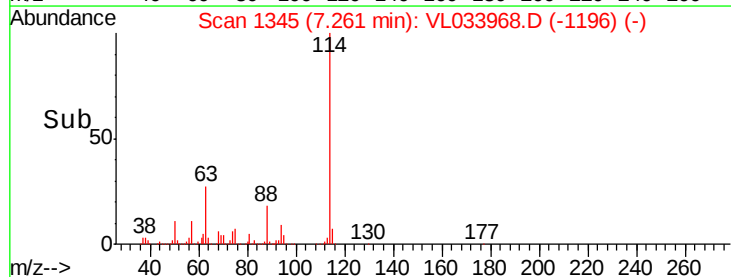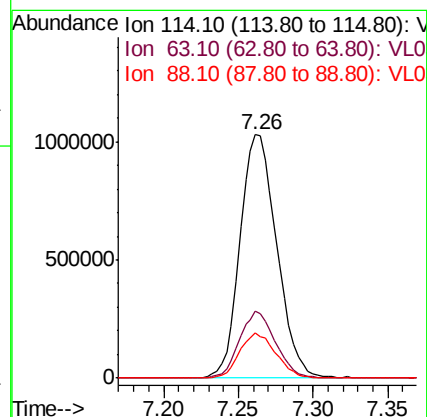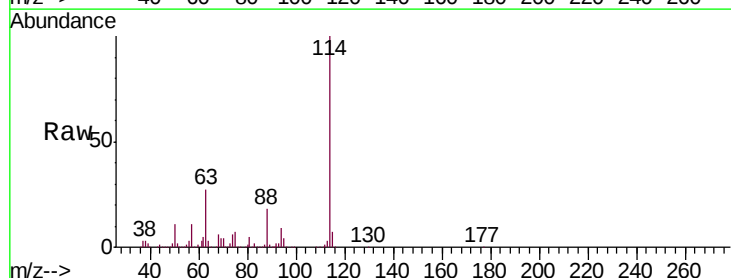

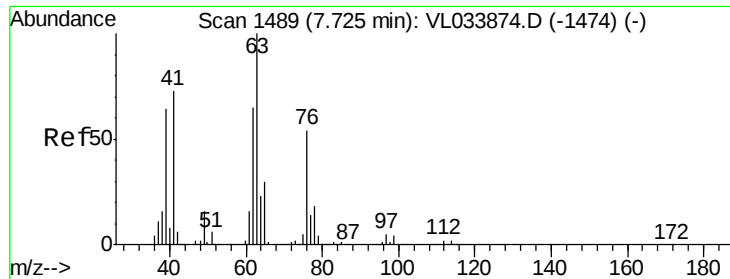

#39

1,2-Dichloropropane

Concen: 9.085 ppbv

RT: 7.26 min Scan# 1345

Delta R.T. -0.46 min

Lab File: VL033968.D

Acq: 26 Jun 2019 15:20

Instrument :

MSVOA\_L

ClientSampleId :

QC062019 CAN 10267


Tgt Ion: 63 Resp: 471523

Ion Ratio Lower Upper

63 100

41 0.0 58.7 88.1#




62 17.2 51.9 77.9#

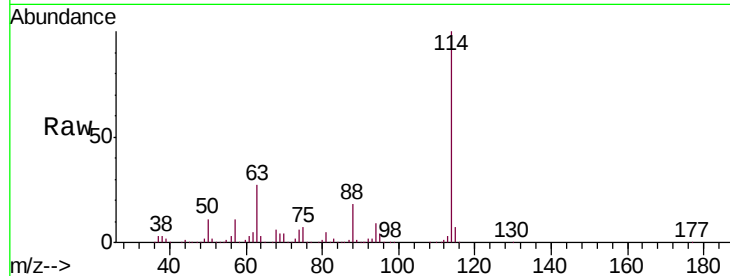

Abundance Ion 63.10 (62.80 to 63.80): VL0

Ion 41.10 (40.80 to 41.80): VL0

Ion 62.10 (61.80 to 62.80): VL0

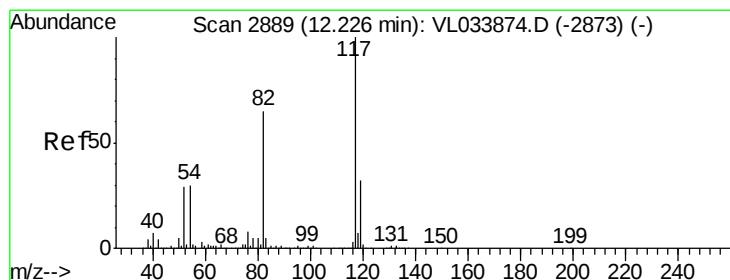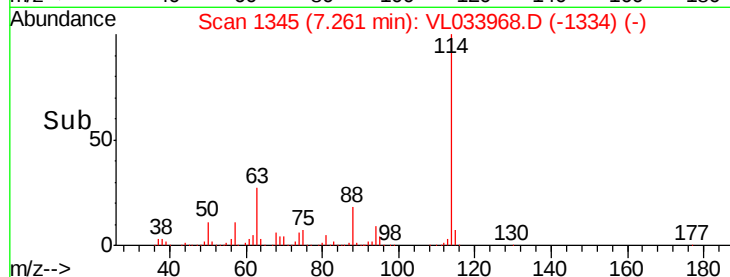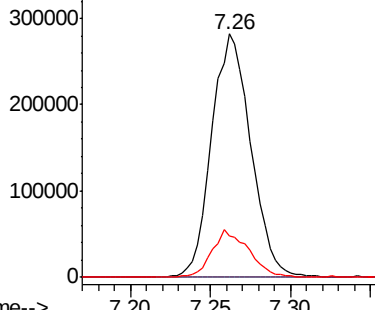

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 12.21 min Scan# 2883

Delta R.T. -0.02 min

Lab File: VL033968.D

Acq: 26 Jun 2019 15:20


Tgt Ion: 117 Resp: 1661487

Ion Ratio Lower Upper

117 100

82 69.4 50.2 75.2



119 32.9 24.8 37.2

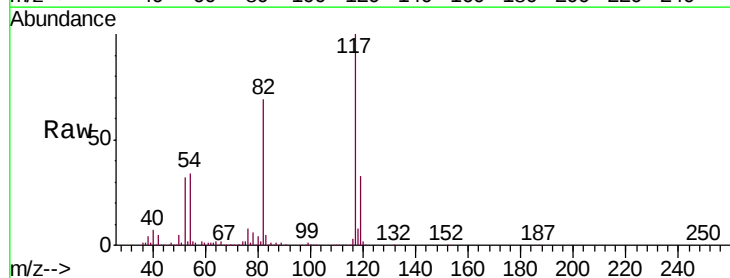


Abundance Ion 117.10 (116.80 to 117.80): V

Ion 82.10 (81.80 to 82.80): VL0

Ion 119.10 (118.80 to 119.80): V

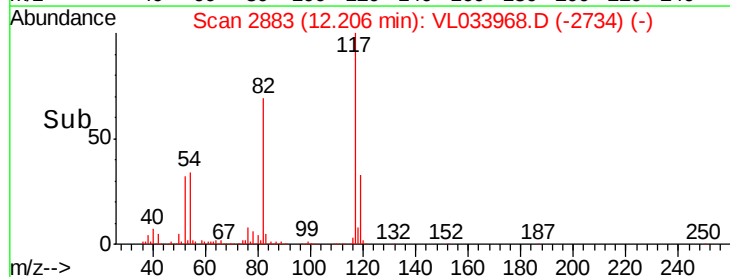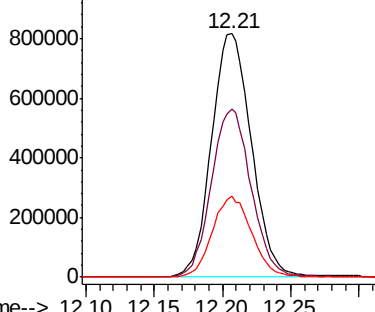

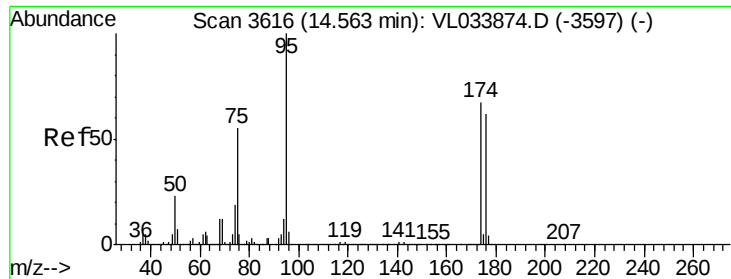

#68

1-Bromo-4-Fluorobenzene

Concen: 10.516 ppbv

RT: 14.54 min Scan# 3610

Delta R.T. -0.02 min

Lab File: VL033968.D

Acq: 26 Jun 2019 15:20

Instrument :

MSVOA\_L

ClientSampleId :

QC062019 CAN 10267

Tgt Ion: 95 Resp: 1435078

Ion Ratio Lower Upper

95 100

174 64.8 54.0 81.0

175 4.5 3.8 5.8

