

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL062619\
 Data File : VL033967.D
 Acq On : 26 Jun 2019 14:39
 Operator : SY/AP
 Sample : QC062019 CAN 10267
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC062019 CAN 10267

Quant Time: Jun 27 04:21:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL060719AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Jun 07 08:53:27 2019
 QLast Update : Fri Jun 07 08:53:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.74	49	903966	10.00	ppbv	-0.02
33) 1,4-Difluorobenzene	7.26	114	2070769	10.00	ppbv	-0.02
55) Chlorobenzene-d5	12.21	117	1904318	10.00	ppbv	-0.02

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.54	95	1603700	10.25	ppbv	-0.02
Spiked Amount	10.000	Range	65 - 135	Recovery	=	102.50%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL062619\
Data File : VL033967.D
Acq On : 26 Jun 2019 14:39
Operator : SY/AP
Sample : OC062019 CAN 10267
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC062019 CAN 10267

Quant Time: Jun 27 04:21:43 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL060719AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Jun 07 08:53:27 2019
QLast Update : Fri Jun 07 08:53:27 2019
Response via : Initial Calibration

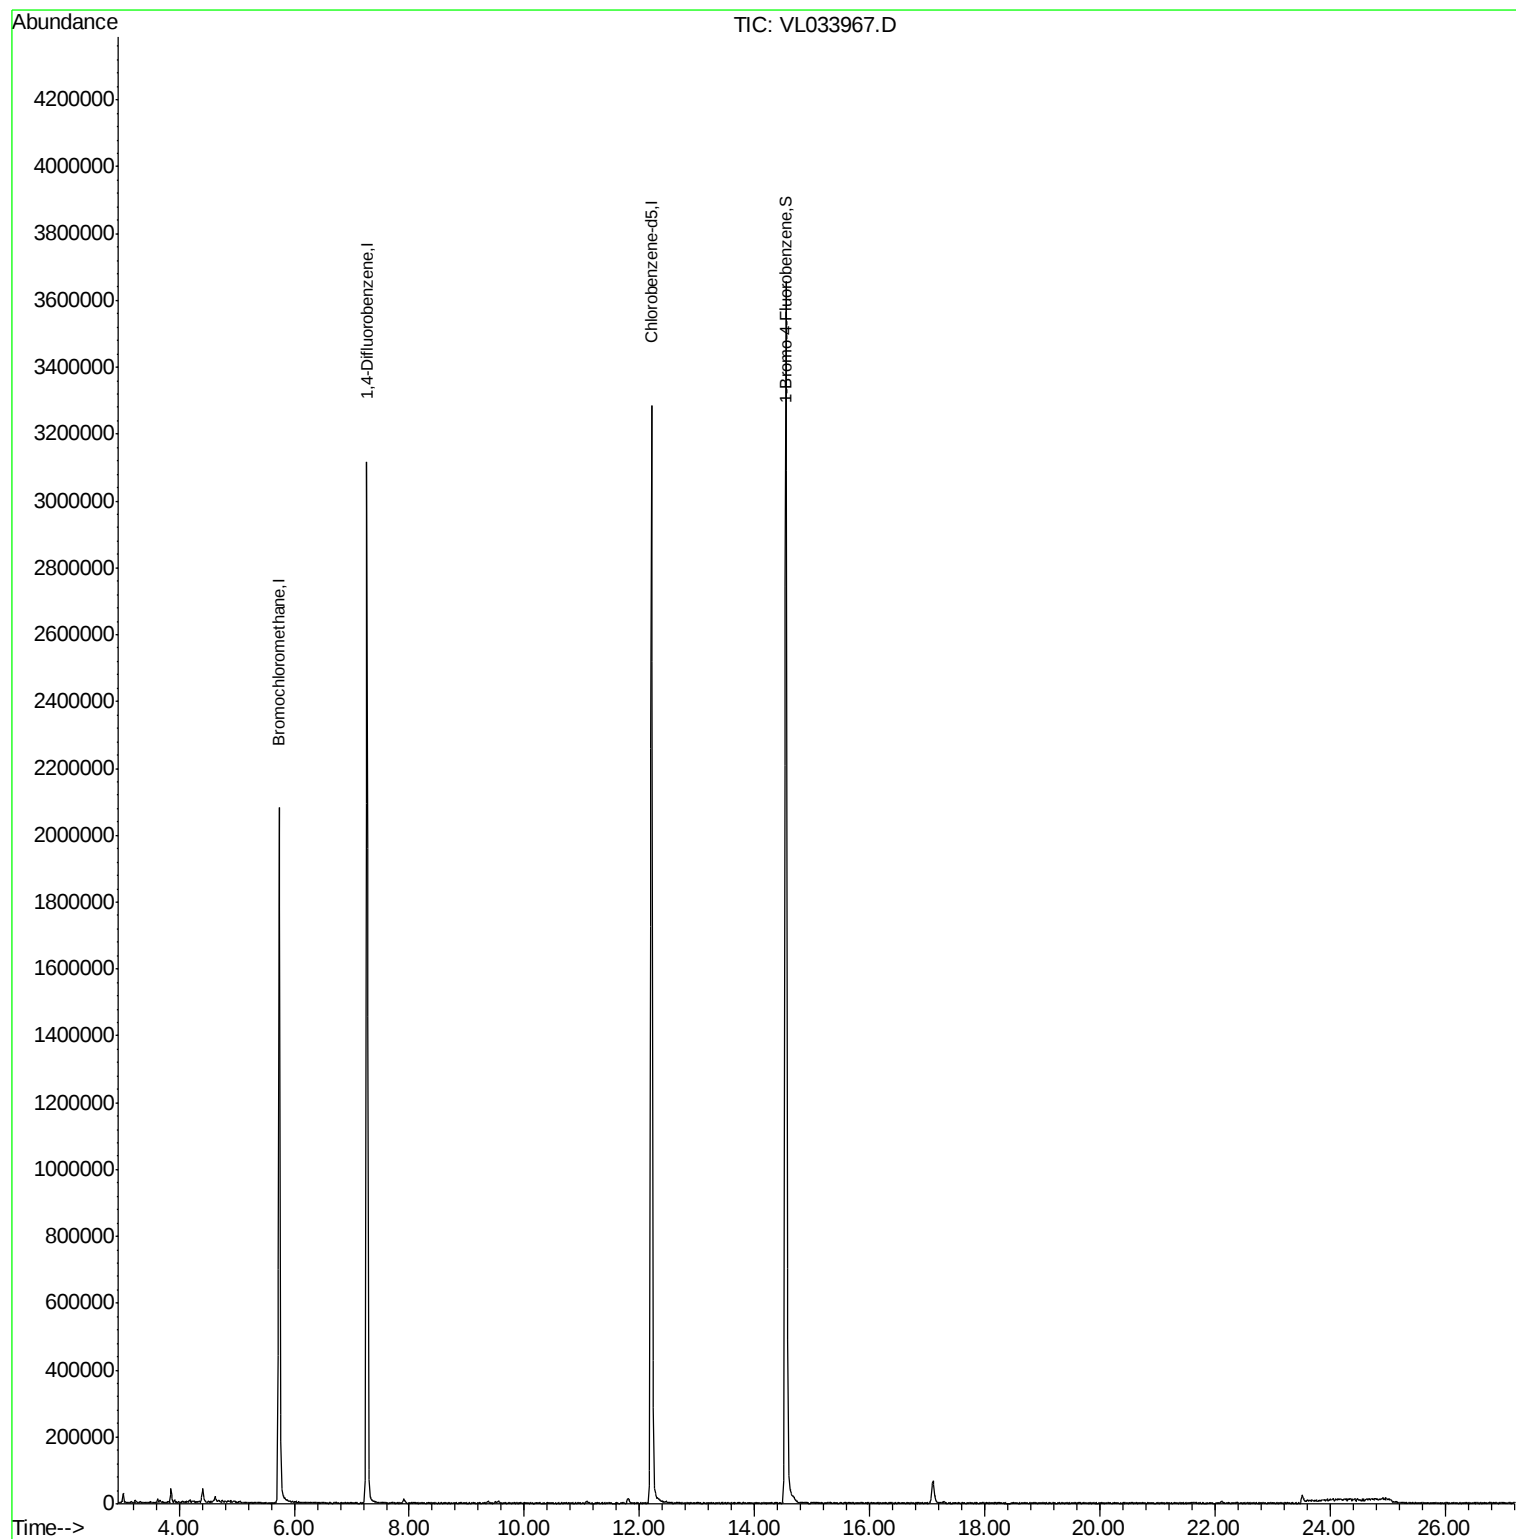

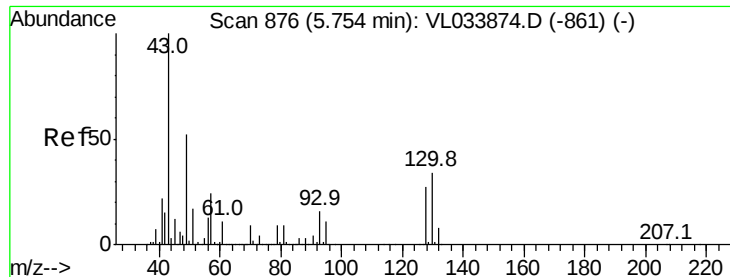

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.74 min Scan# 871

Delta R.T. -0.02 min

Lab File: VL033967.D

Acq: 26 Jun 2019 14:39

Instrument :

MSVOA_L

ClientSampleId :

QC062019 CAN 10267


Tot Ion: 49 Resp: 903966

Ion Ratio Lower Upper

49 100

128 50.3 25.5 76.5




130 66.4 32.5 97.4

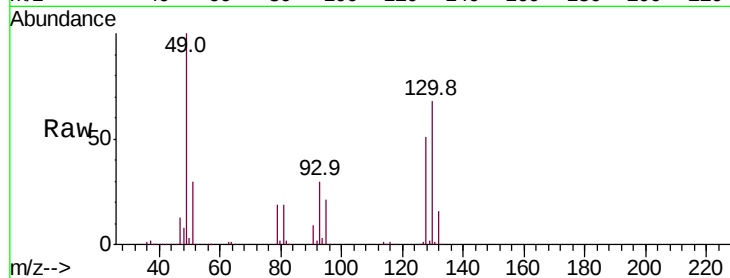

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

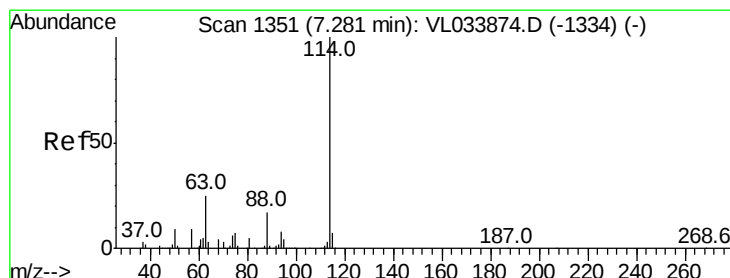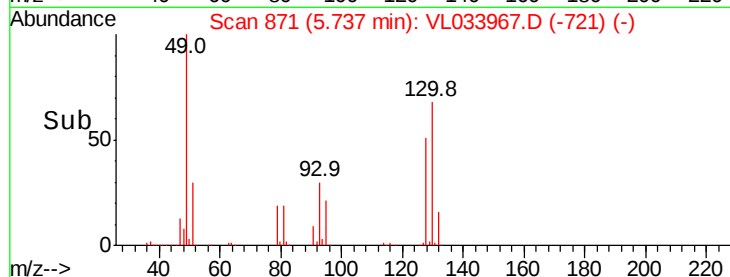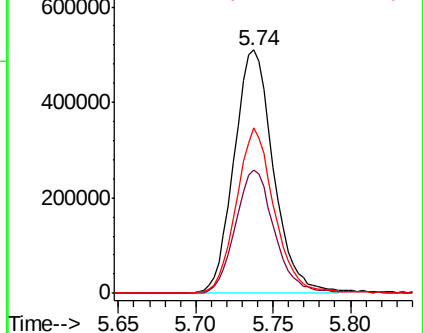

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.26 min Scan# 1346

Delta R.T. -0.02 min

Lab File: VL033967.D

Acq: 26 Jun 2019 14:39


Tgt Ion:114 Resp: 2070769

Ion Ratio Lower Upper

114 100

63 26.3 21.1 31.7



88 17.9 14.2 21.4

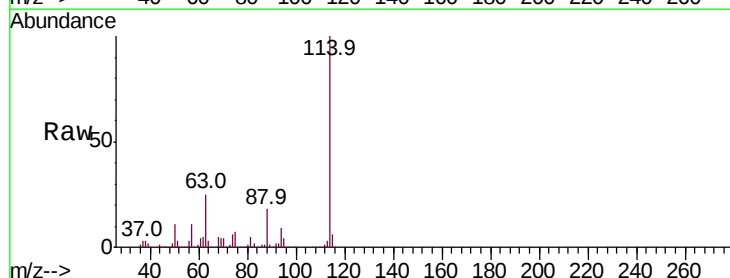


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0



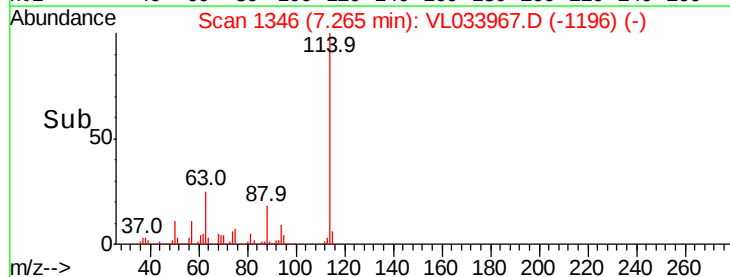
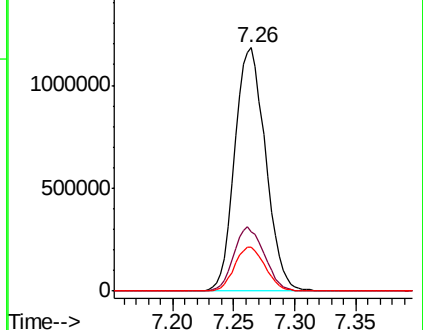


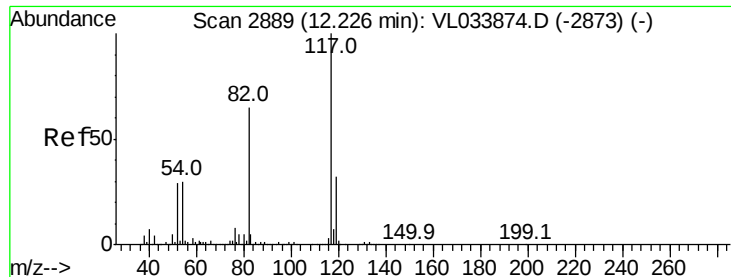

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.21 min Scan# 2883
Delta R.T. -0.02 min
Lab File: VL033967.D
Acq: 26 Jun 2019 14:39

Instrument :
MSVOA_L
ClientSampleId :
QC062019 CAN 10267

Tot Ion:117 Resp: 1904318
Ion Ratio Lower Upper
117 100
82 68.9 50.2 75.2
119 32.8 24.8 37.2

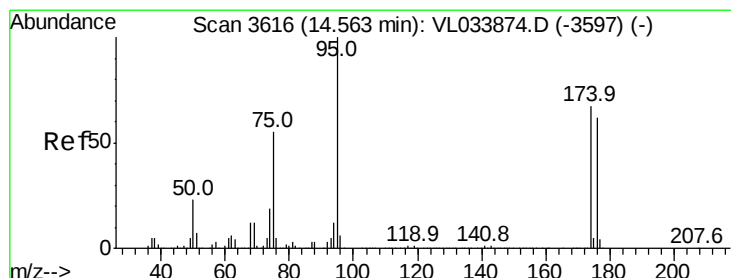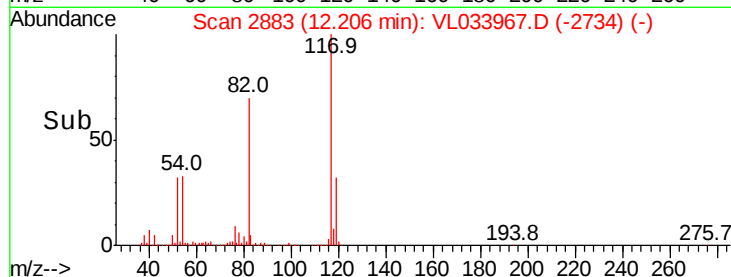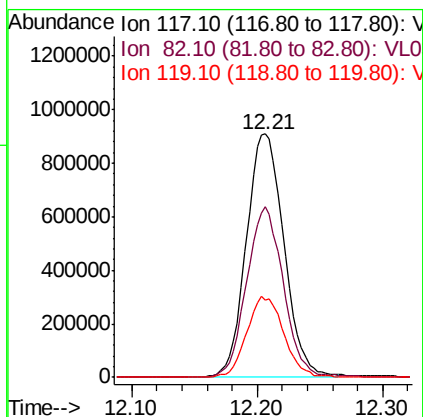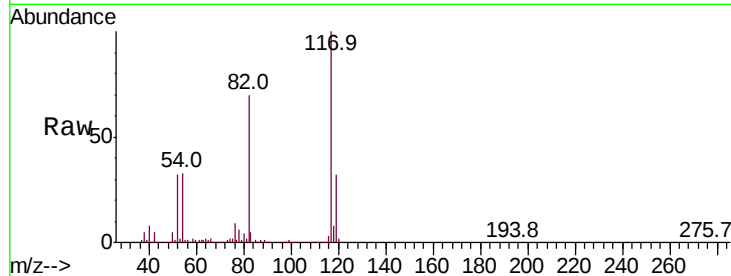

#68
1-Bromo-4-Fluorobenzene
Concen: 10.253 ppbv
RT: 14.54 min Scan# 3609
Delta R.T. -0.02 min
Lab File: VL033967.D
Acq: 26 Jun 2019 14:39

Tgt Ion: 95 Resp: 1603700
Ion Ratio Lower Upper
95 100
174 66.1 54.0 81.0
175 4.8 3.8 5.8

