
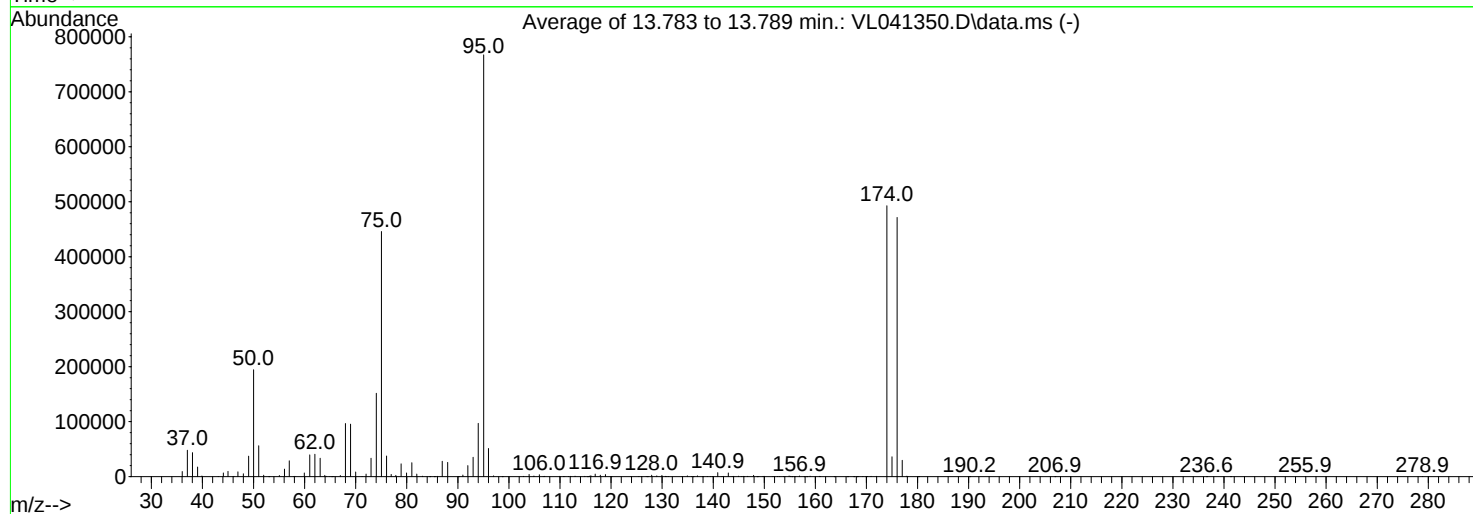


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL062624\
 Data File : VL041350.D
 Acq On : 26 Jun 2024 7:32
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL062624AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Thu Jun 27 09:18:04 2024

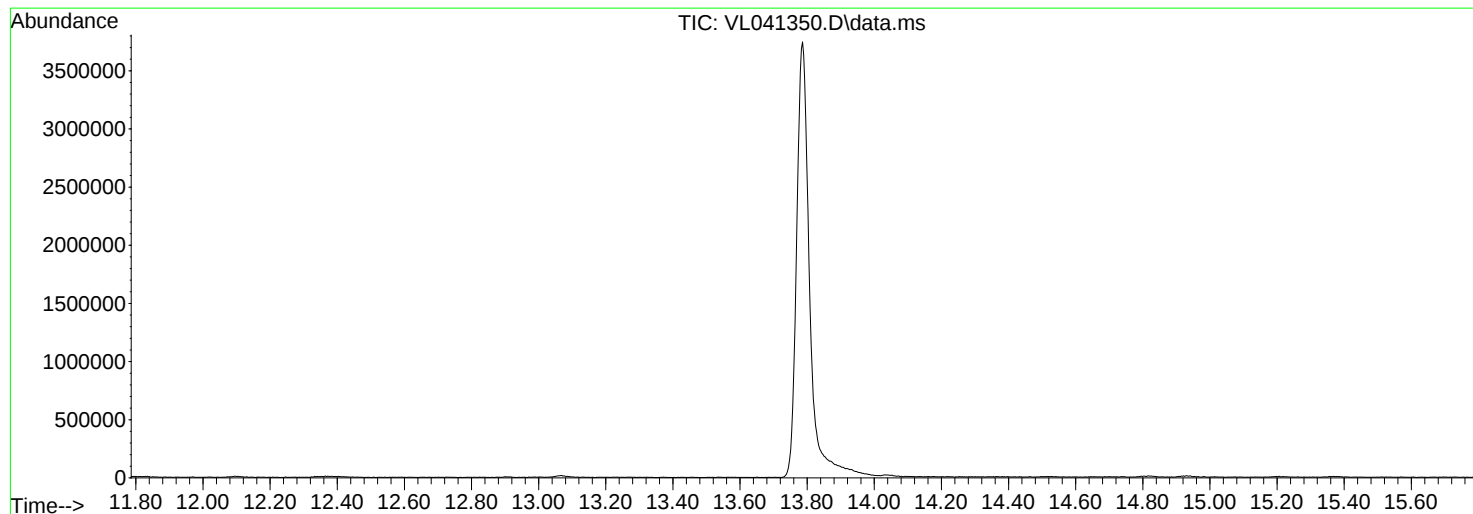

AutoFind: Scans 3477, 3478, 3479; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.4	194581	PASS
75	95	30	66	58.1	445781	PASS
95	95	100	100	100.0	767211	PASS
96	95	5	9	6.7	51192	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	64.2	492587	PASS
175	174	4	9	7.3	36147	PASS
176	174	93	101	95.7	471573	PASS
177	176	5	9	6.3	29571	PASS

Average of 13.783 to 13.789 min.: VL041350.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	9346	48.00	5353	59.95	6652	69.00	9558
37.05	48139	49.05	37237	61.00	39691	70.00	8471
38.05	43592	50.00	194581	62.00	40677	71.25	25
39.05	17376	51.00	56288	63.05	33488	72.05	479
39.90	1159	52.00	2740	63.95	2246	73.00	33381
43.10	239	53.00	79	64.20	656	74.05	151659
44.10	6693	55.05	2154	64.95	212	75.05	445781
45.00	9547	56.05	13617	65.30	62	76.05	37571
46.00	326	57.00	28725	65.70	400	76.95	4219
46.15	473	57.90	360	67.00	2155	77.85	2437
46.95	8700	58.10	474	68.00	96763	78.90	23304

Instrument :

MSVOA_L

ClientSampleId :

BFB

Average of 13.783 to 13.789 min.: VL041350.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.95	6774	91.95	20160	106.70	312	116.05	1825
81.00	25400	93.00	35221	107.00	455	116.90	4783
81.95	4744	94.00	96965	109.95	538	117.90	2670
83.10	862	95.05	767211	110.70	293	118.90	3843
84.50	108	96.00	51192	110.95	439	120.00	63
85.40	58	97.00	1511	111.65	264	123.90	347
86.00	636	98.70	60	112.10	495	125.45	349
86.95	27864	102.85	530	112.95	920	126.00	272
88.00	26040	103.95	4221	114.85	693	126.90	276
90.10	68	104.90	1095	115.40	108	127.10	132
91.00	3000	105.95	3475	115.80	1004	127.95	2514

Average of 13.783 to 13.789 min.: VL041350.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
128.95	1379	138.85	231	145.90	687	153.00	296
129.95	2390	139.50	180	146.10	322	153.80	162
130.65	646	139.90	209	146.75	595	154.05	433
130.90	408	140.90	7296	147.90	2224	154.85	1157
131.20	210	141.70	349	148.60	124	155.10	524
133.90	297	141.95	499	148.95	295	155.40	134
134.95	1358	142.95	6877	149.75	568	155.90	106
135.75	248	143.70	187	150.00	565	156.90	1225
136.05	134	144.00	685	151.70	306	157.80	60
136.90	1440	144.95	886	152.00	348	158.30	59
137.90	65	145.60	224	152.60	171	158.95	892

Average of 13.783 to 13.789 min.: VL041350.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
160.80	459	171.95	614	241.30	64		
161.00	254	174.00	492587	255.90	219		
163.70	58	175.00	36147	278.90	167		
166.30	82	176.00	471573				
167.50	65	177.00	29571				
168.10	56	177.90	893				
168.50	229	178.10	380				
169.30	397	180.20	53				
169.90	107	190.20	123				
170.20	193	206.90	110				
170.90	616	236.60	65				