

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL070124\
 Data File : VL041369.D
 Acq On : 1 Jul 2024 15:39
 Operator : SY/MD
 Sample : VL0701ABL01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0701ABL01

Quant Time: Jul 01 23:31:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL062624AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Mon Jul 01 23:27:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.211	49	1055107	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.664	114	2824710	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.471	117	2475108	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.777	95	1786758	9.632	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	96.300%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL070124\
Data File : VL041369.D
Acq On : 1 Jul 2024 15:39
Operator : SY/MD
Sample : VL0701ABL01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0701ABL01

Quant Time: Jul 01 23:31:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL062624AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Mon Jul 01 23:27:24 2024
Response via : Initial Calibration




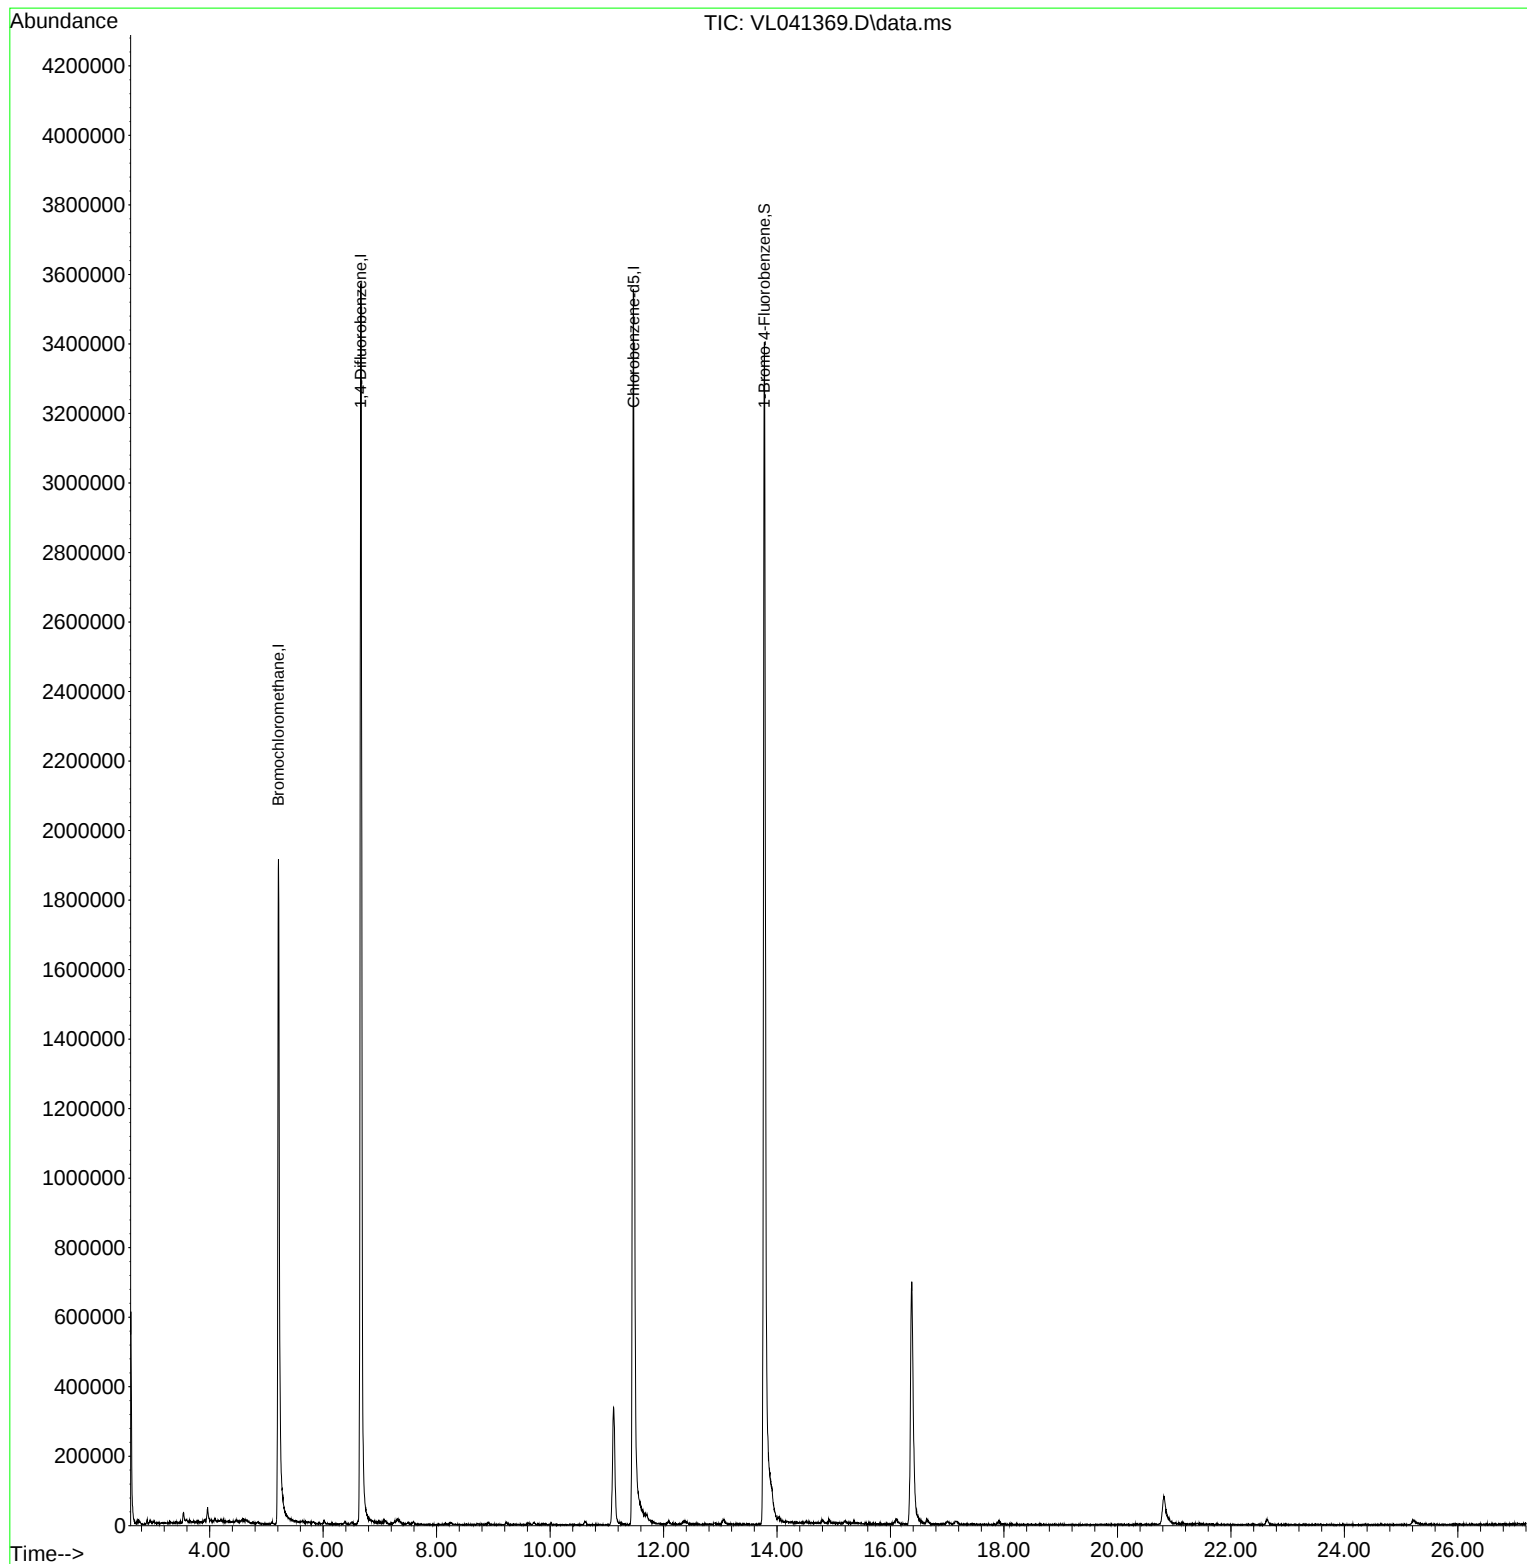


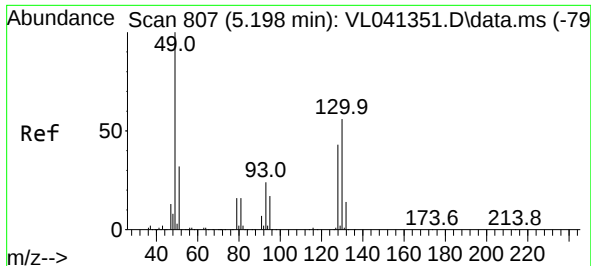

#1
Bromochloromethane
Concen: 10.000 ppbv
RT: 5.211 min Scan# 811
Delta R.T. -0.007 min
Lab File: VL041369.D
Acq: 1 Jul 2024 15:39




Instrument :
MSVOA_L
ClientSampleId :
VL0701ABL01


Tgt Ion: 49 Resp: 1055107
Ion Ratio Lower Upper
49 100
128 46.8 22.8 68.3
130 59.8 28.9 86.7

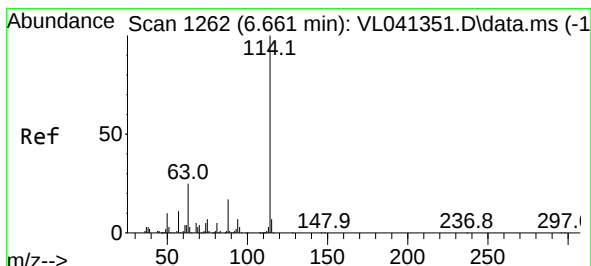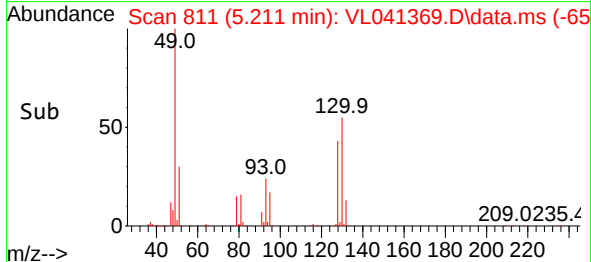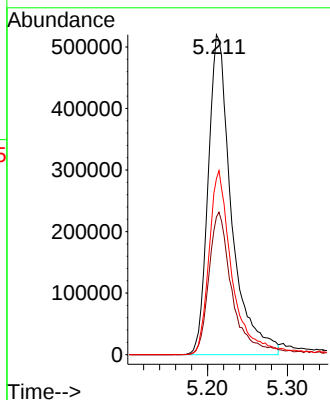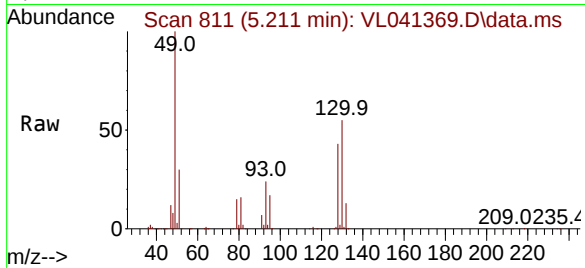

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.664 min Scan# 1263
Delta R.T. -0.006 min
Lab File: VL041369.D
Acq: 1 Jul 2024 15:39

Tgt Ion: 114 Resp: 2824710
Ion Ratio Lower Upper
114 100
63 25.0 20.6 31.0
88 17.7 14.6 21.8


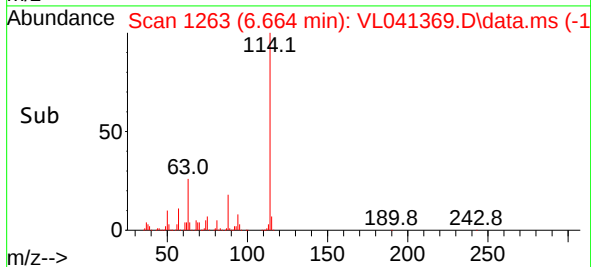
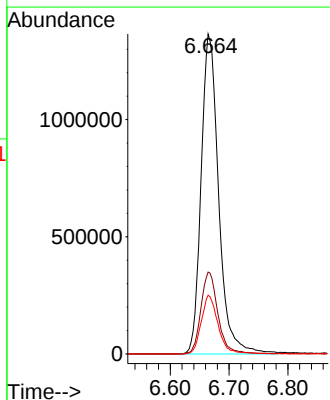
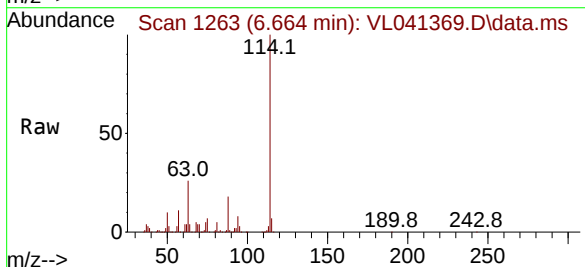


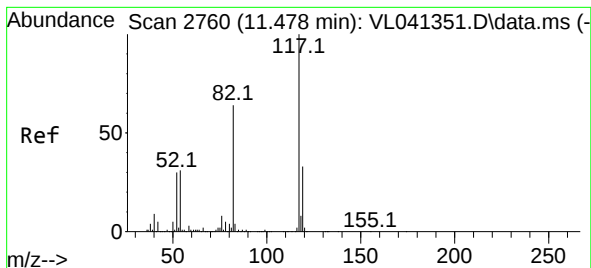

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.471 min Scan# 21
Delta R.T. 0.000 min
Lab File: VL041369.D
Acq: 1 Jul 2024 15:39

Instrument :
MSVOA_1
ClientSampleId :
VL0701ABL01

Tgt Ion:117 Resp: 2475108
Ion Ratio Lower Upper
117 100
82 65.2 50.6 75.8
119 33.5 24.7 37.1

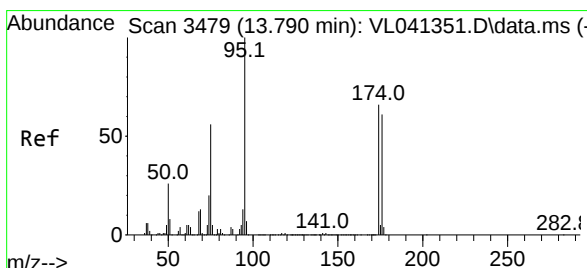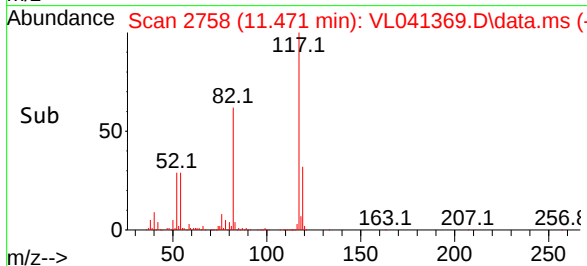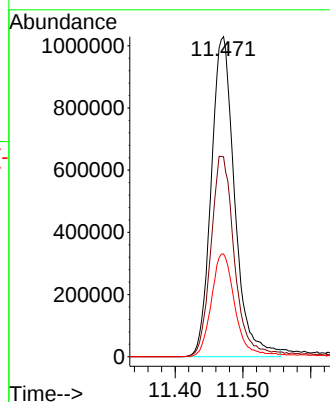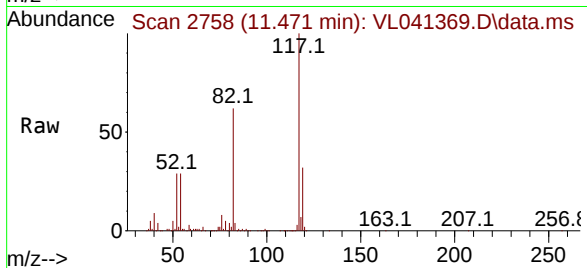

#68
1-Bromo-4-Fluorobenzene
Concen: 9.632 ppbv
RT: 13.777 min Scan# 3475
Delta R.T. 0.000 min
Lab File: VL041369.D
Acq: 1 Jul 2024 15:39

Tgt Ion: 95 Resp: 1786758
Ion Ratio Lower Upper
95 100
174 69.3 53.1 79.7
175 4.9 4.0 6.0

