
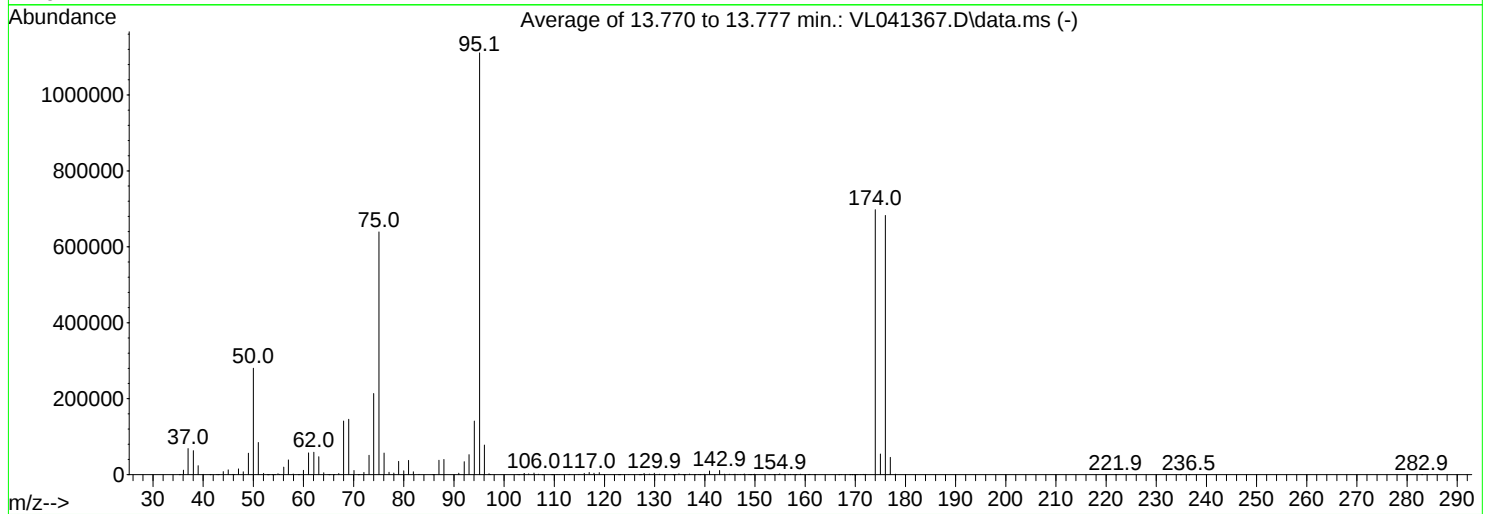


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL070124\
Data File : VL041367.D
Acq On : 1 Jul 2024 14:13
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL062624AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Mon Jul 01 23:27:24 2024

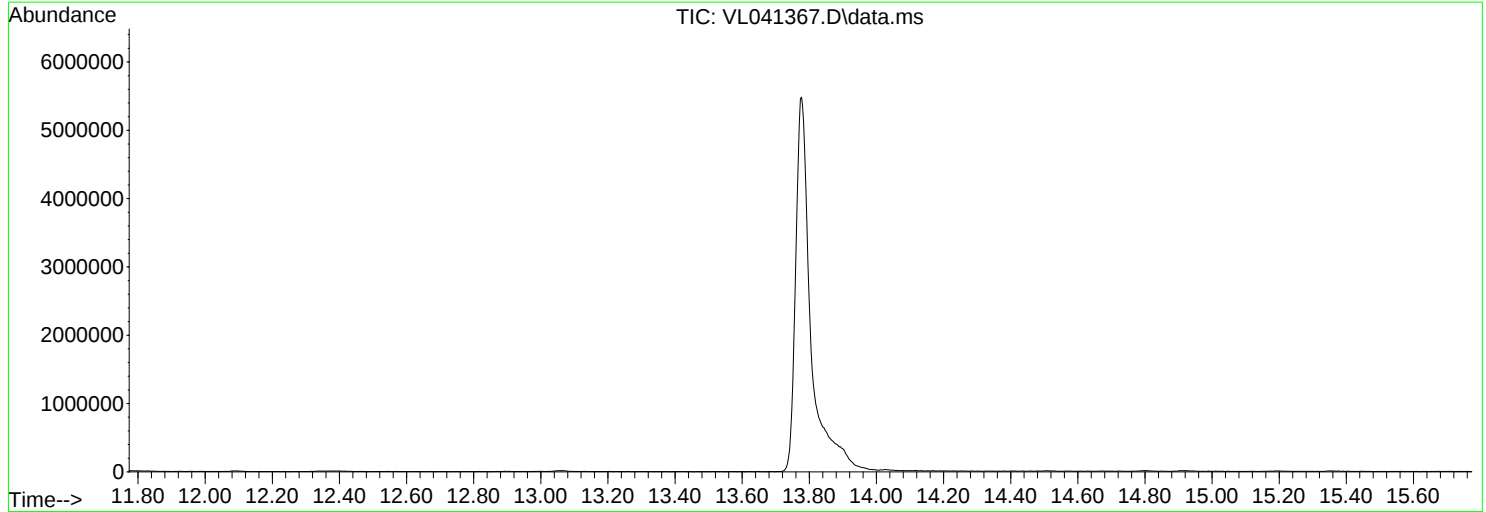

AutoFind: Scans 3473, 3474, 3475; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.2	280235	PASS
75	95	30	66	57.6	639317	PASS
95	95	100	100	100.0	1110869	PASS
96	95	5	9	7.0	78125	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	62.8	698027	PASS
175	174	4	9	7.8	54408	PASS
176	174	93	101	97.8	682624	PASS
177	176	5	9	6.7	45437	PASS

Average of 13.770 to 13.777 min.: VL041367.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.25	246	45.00	12887	53.75	196	63.05	4714
36.05	11928	45.95	838	54.20	59	64.05	518
37.00	68624	46.20	625	54.90	2421	64.90	53
38.05	63363	47.05	15126	55.20	860	65.10	21
39.00	23529	48.00	7522	56.05	19811	66.00	95
40.00	880	49.00	56381	57.00	38771	67.05	3162
41.40	91	50.00	280235	57.95	1700	68.00	141397
42.70	275	51.00	84781	59.00	162	69.00	145835
42.90	213	52.05	3638	60.00	11215	70.05	11110
43.20	273	52.80	52	61.00	57443	70.90	168
44.00	7956	53.00	62	62.05	58827	71.15	410

Average of 13.770 to 13.777 min.: VL041367.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
72.05	5983	83.00	946	97.00	2436	109.85	620
73.05	51120	85.80	221	97.30	554	110.55	447
74.00	213803	86.05	520	102.60	267	110.95	635
75.05	639317	87.00	38197	102.90	156	111.95	517
76.05	57035	88.00	39960	103.90	1850	112.90	328
77.05	6353	90.95	3960	104.05	2984	113.05	811
78.00	4056	92.05	34277	104.90	1998	114.90	776
78.95	34963	93.00	52848	105.95	4436	115.95	3323
80.00	10023	94.05	141099	106.85	1150	116.95	5773
80.95	37549	95.10	1.11087e+006	107.65	115	117.90	3728
81.90	7660	96.05	78125	109.50	126	118.95	5368

Average of 13.770 to 13.777 min.: VL041367.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.85	335	129.95	3953	139.00	203	147.70	717
121.90	564	130.95	1283	139.90	1145	147.90	1806
122.80	145	132.00	211	140.95	9749	148.75	616
123.05	223	133.70	120	142.00	402	148.90	400
123.95	532	134.00	66	142.95	11009	149.10	97
124.85	469	134.85	2101	143.95	1098	149.70	315
125.90	443	135.70	90	144.90	1168	149.95	1123
126.95	159	136.00	178	145.80	492	151.95	371
127.20	146	136.95	1907	146.00	1206	152.80	298
127.90	3529	138.00	56	146.60	376	152.95	593
128.95	1849	138.75	374	147.05	631	153.80	247

Average of 13.770 to 13.777 min.: VL041367.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
153.95	320	160.95	831	171.55	915	282.90	73
154.70	381	161.90	60	171.80	504		
154.95	2171	166.70	115	172.10	1071		
155.80	253	167.20	294	174.00	698027		
155.95	276	168.10	280	175.00	54408		
156.70	370	168.90	117	176.00	682624		
157.05	1019	169.35	250	177.00	45437		
157.75	277	169.80	71	178.00	1311		
158.10	122	170.00	139	221.90	60		
159.05	1109	170.50	587	234.80	58		
160.70	368	171.10	305	236.50	66		