


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL070219\
 Data File : VL033988.D
 Acq On : 2 Jul 2019 13:02
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL070219AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Jul 02 19:31:31 2019
 Last Update : Tue Jul 02 19:31:31 2019

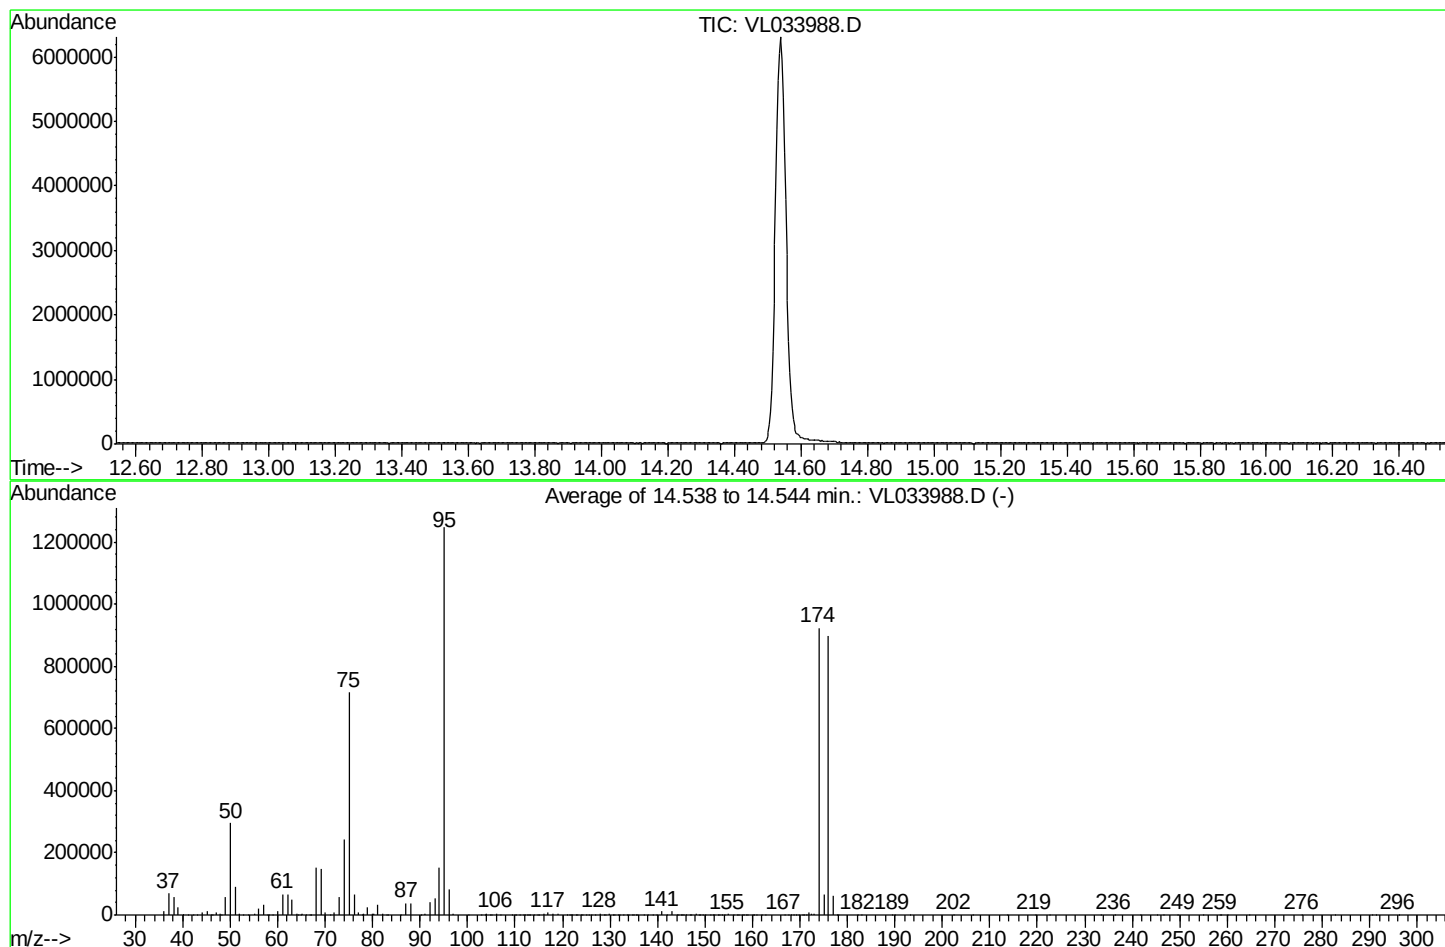

AutoFind: Scans 3608, 3609, 3610; Background Corrected with Scan 3585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.7	295253	PASS
75	95	30	66	57.4	716740	PASS
95	95	100	100	100.0	1247744	PASS
96	95	5	9	6.7	82984	PASS
173	174	0.00	2	0.4	4059	PASS
174	95	50	120	74.1	924608	PASS
175	174	4	9	7.2	66338	PASS
176	174	93	101	97.2	898325	PASS
177	176	5	9	6.8	61336	PASS