


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL070221\
 Data File : VL037266.D
 Acq On : 2 Jul 2021 8:30
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL061621AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Jun 16 14:06:32 2021
 Last Update : Wed Jun 16 14:06:32 2021

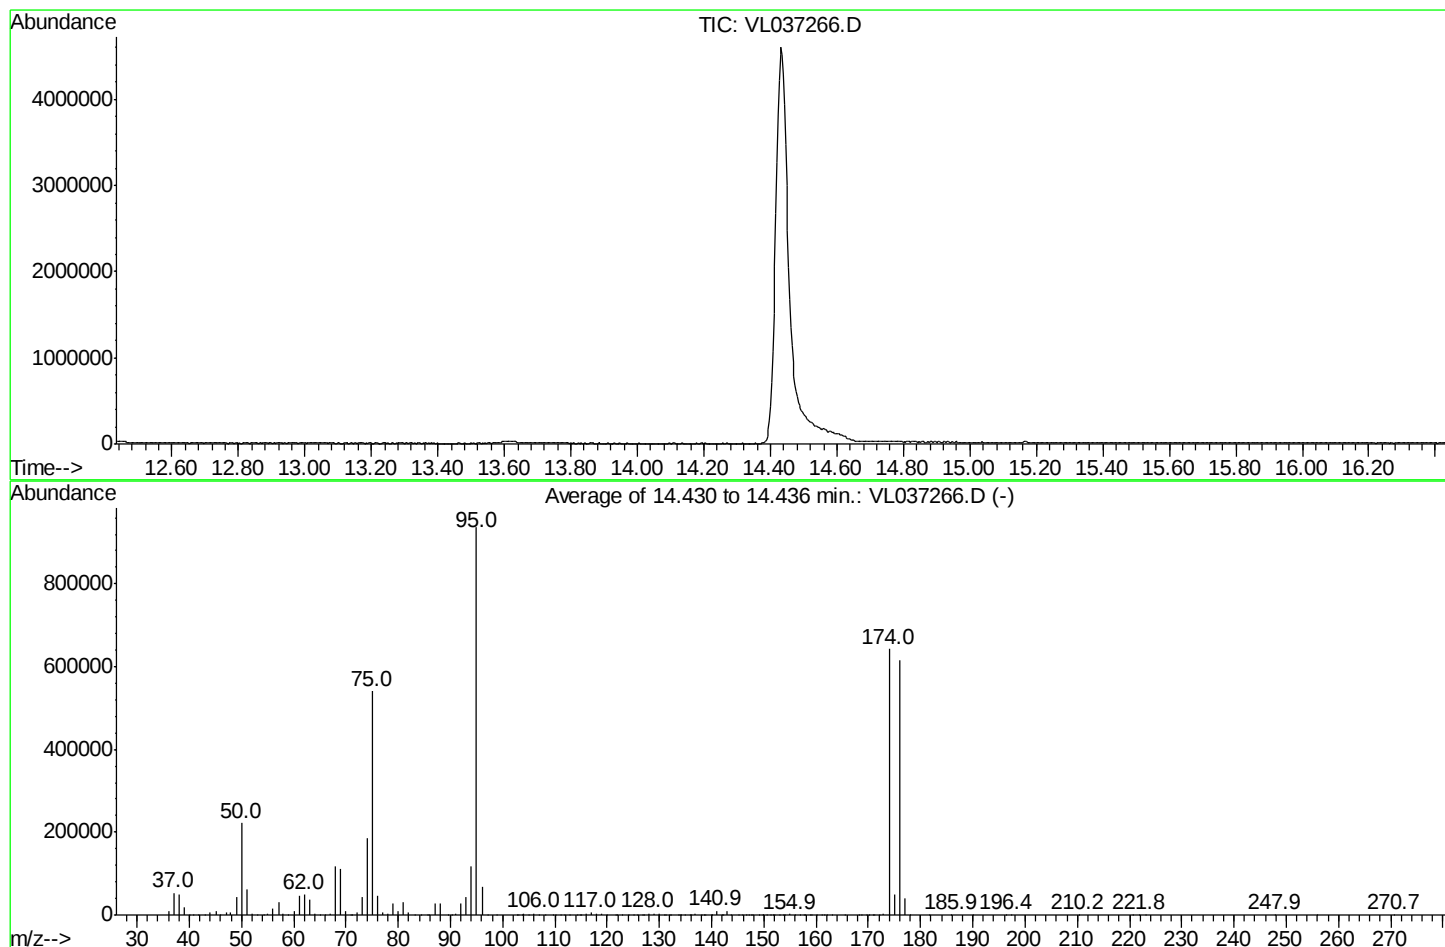

AutoFind: Scans 3621, 3622, 3623; Background Corrected with Scan 3597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.8	222528	PASS
75	95	30	66	57.6	539861	PASS
95	95	100	100	100.0	936640	PASS
96	95	5	9	7.3	68077	PASS
173	174	0.00	2	0.4	2650	PASS
174	95	50	120	68.5	641962	PASS
175	174	4	9	7.6	48570	PASS
176	174	93	101	95.8	614912	PASS
177	176	5	9	6.6	40677	PASS