


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL070522\
Data File : VL039418.D
Acq On : 5 Jul 2022 12:18
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL062922AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jul 06 02:15:38 2022
Last Update : Wed Jul 06 02:15:38 2022

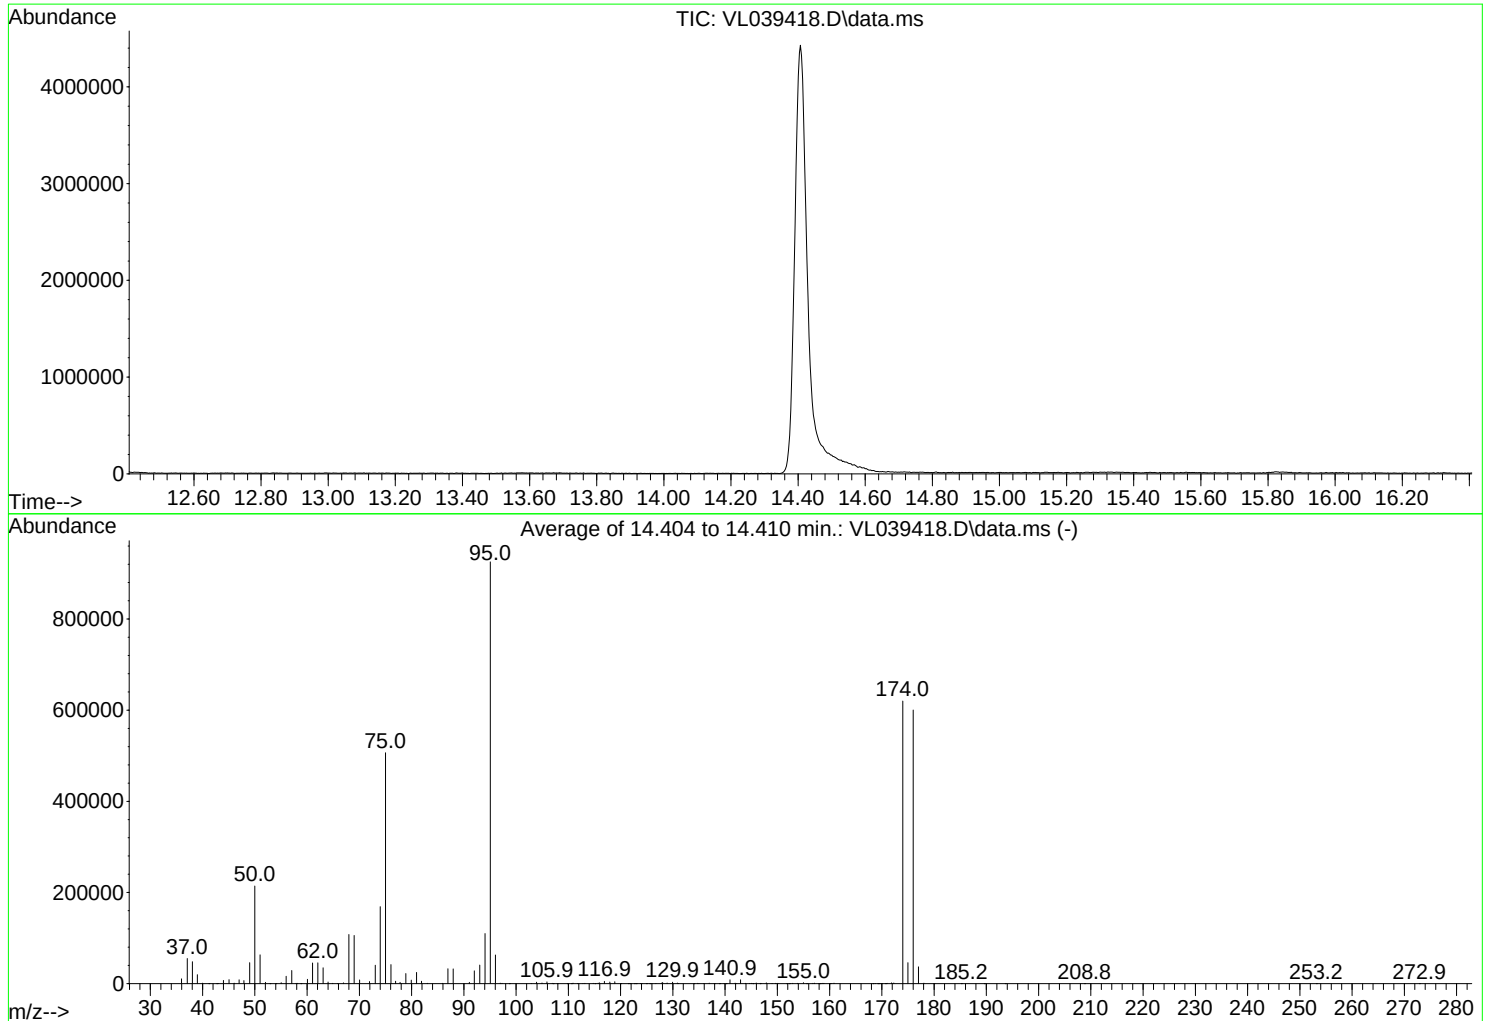

AutoFind: Scans 3613, 3614, 3615; Background Corrected with Scan 3588

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	23.1	214229	PASS
75	95	30	66	54.8	506688	PASS
95	95	100	100	100.0	925440	PASS
96	95	5	9	6.8	62853	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.0	619815	PASS
175	174	4	9	7.4	46013	PASS
176	174	93	101	96.9	600299	PASS
177	176	5	9	6.1	36768	PASS

Average of 14.404 to 14.410 min.: VL039418.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	10384	47.00	8359	57.90	776	68.00	10787
37.05	55253	47.90	6811	58.20	800	69.00	10584
38.05	48005	49.00	46016	58.80	54	70.05	794
39.00	19752	50.00	214229	60.05	9594	71.95	446
40.00	1067	51.00	63229	61.05	45475	73.05	40293
41.20	74	52.05	2908	62.05	45717	74.00	168917
42.70	77	52.90	118	63.05	34667	75.00	506688
43.00	242	54.00	44	64.00	3601	76.05	41893
44.00	7212	55.05	2231	64.90	845	76.95	5431
45.05	8707	56.00	16084	65.85	334	77.80	2814
46.05	1022	57.05	28800	66.95	1846	78.90	22264

Average of 14.404 to 14.410 min.: VL039418.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.95	7667	95.05	925440	107.85	117	115.95	1610
80.95	24581	96.05	62853	109.80	153	116.90	5000
81.90	5195	96.95	1212	110.60	124	117.95	3509
83.00	630	97.30	694	110.90	928	118.90	4225
85.90	848	98.70	110	111.75	442	120.00	59
86.95	32715	102.90	229	112.00	217	121.50	119
87.95	32267	103.90	3275	112.80	447	121.85	152
91.05	2663	104.95	1376	113.15	551	122.65	186
92.00	27976	105.90	3783	114.75	554	123.00	163
93.05	40867	106.90	799	115.10	154	123.80	241
94.05	109883	107.10	119	115.70	935	124.10	509

Average of 14.404 to 14.410 min.: VL039418.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
124.95	175	134.75	570	142.10	342	149.70	582
125.60	62	135.00	472	142.95	8303	150.10	570
126.00	342	135.95	445	143.90	699	151.80	158
126.75	295	136.95	1180	144.70	238	152.00	499
127.90	1428	137.90	169	145.00	862	152.30	175
128.05	2370	138.90	100	145.30	157	152.95	748
128.90	1312	139.05	542	145.95	1481	153.85	893
129.95	3021	139.80	213	146.70	120	155.00	1974
130.85	1413	140.20	176	146.85	577	155.60	98
131.10	317	140.95	8586	147.90	1948	156.80	708
134.00	165	141.90	1061	149.00	474	157.10	1043

Average of 14.404 to 14.410 min.: VL039418.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
157.90	103	169.80	176	179.95	154		
158.20	97	170.10	452	185.20	83		
158.70	573	170.70	185	189.60	75		
158.90	875	171.00	564	193.60	52		
160.00	103	171.85	1664	208.80	98		
160.40	253	172.30	1328	253.15	126		
160.85	1029	174.00	619815	272.90	104		
168.30	98	175.00	46013				
168.80	205	176.00	600299				
169.20	135	177.00	36768				
169.40	68	178.05	1033				