

Data Path : W:\HPCHEM1\MSVOA_L\DATA\VL070715\
 Data File : VL025612.D
 Acq On : 7 Jul 2015 17:16
 Operator : SY/MD
 Sample : VL0707ABL01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0707ABL01

Quant Time: Jul 08 06:53:20 2015
 Quant Method : W:\HPCHEM1\MSVOA_L\METHODS\VL070715AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Jul 08 02:22:55 2015
 QLast Update : Wed Jul 08 02:22:55 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	6.66	49	542637	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	8.33	114	1448659	10.00	ppbv	0.00
55) Chlorobenzene-d5	13.75	117	1975781	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	16.29	95	1678830	10.07	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	100.70%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chlorodifluoromethane	3.57	51	651	0.01	ppbv #	51
4) Chloromethane	3.58	50	267	0.01	ppbv #	42
9) Propene	3.61	41	821	0.03	ppbv #	46
15) Acetone	4.65	43	21073	0.22	ppbv #	42
16) 1,3-Butadiene	3.95	39	2625	0.07	ppbv #	12
20) Methylene Chloride	5.15	84	2095	0.05	ppbv #	77
23) Vinyl Acetate	6.01	43	2186	0.02	ppbv #	77
25) Ethyl Acetate	6.26	43	1075	0.01	ppbv #	76
30) Cyclohexane	8.31	84	7295	0.11	ppbv #	1
34) 2-Butanone	6.18	43	123	0.00	ppbv #	52
42) Bromodichloromethane	8.72	83	147	0.00	ppbv #	24
43) Methyl Methacrylate	8.79	69	113	0.00	ppbv #	1
44) 2,2,4-Trimethylpentane	8.76	57	309	0.00	ppbv #	39
51) 2-Hexanone	11.94	43	23867	0.22	ppbv #	46
52) Tetrachloroethene	13.22	164	3011	0.04	ppbv #	27
58) Ethyl Benzene	14.41	91	129	0.00	ppbv #	44
59) m/p-Xylene	14.73	91	250	0.00	ppbv #	29
60) o-Xylene	15.49	91	626	0.00	ppbv #	32
62) Isopropylbenzene	16.30	105	722	0.00	ppbv #	49
63) 1,1,2,2-Tetrachloroethane	15.39	83	243	0.00	ppbv #	25
65) tert-Butylbenzene	18.92	119	63469	0.16	ppbv #	21
66) Benzyl Chloride	18.94	91	396	0.00	ppbv #	1
67) sec-Butylbenzene	18.97	105	163	0.00	ppbv #	1
74) 1,2,4-Trimethylbenzene	18.85	105	455	0.00	ppbv #	31
75) 1,3-Dichlorobenzene	18.94	146	239	0.00	ppbv #	24
76) 1,4-Dichlorobenzene	18.94	146	239	0.00	ppbv #	24
79) Naphthalene	23.96	128	908	0.00	ppbv #	68
80) Naphthalene,2-methyl-	26.11	142	162	0.00	ppbv #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA_L\DATA\VL070715\
Data File : VL025612.D
Acq On : 7 Jul 2015 17:16
Operator : SY/MD
Sample : VL0707ABL01
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0707ABL01

Quant Time: Jul 08 06:53:20 2015
Quant Method : W:\HPCHEM1\MSVOA_L\METHODS\VL070715AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Jul 08 02:22:55 2015
QLast Update : Wed Jul 08 02:22:55 2015
Response via : Initial Calibration

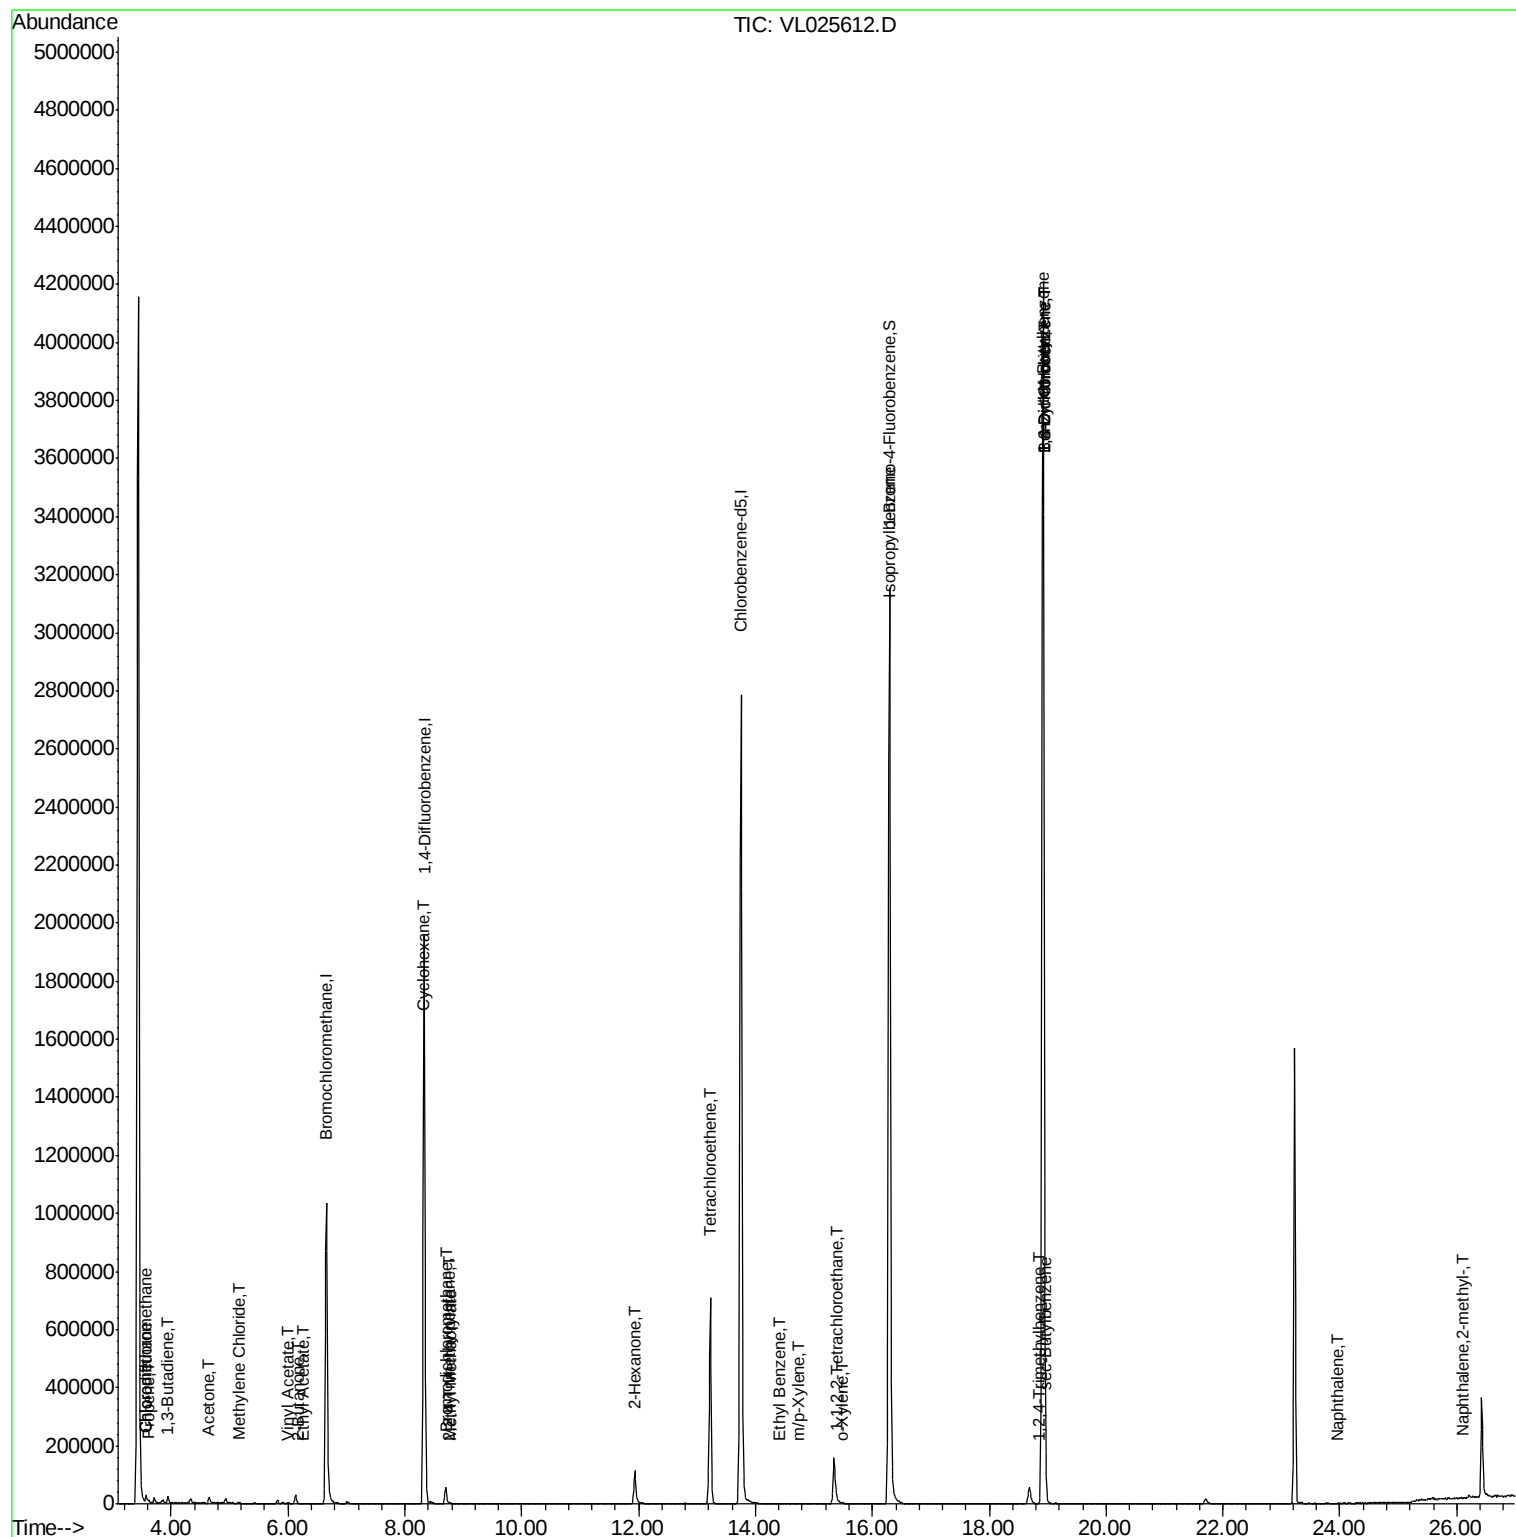



#1

Bromochloromethane

Concen: 10.00 ppbv

RT: 6.66 min Scan# 586

Delta R.T. 0.01 min

Lab File: VL025612.D

Acq: 7 Jul 2015 17:16

Instrument :

MSVOA_L

ClientSampleId :

VL0707ABL01


Tgt Ion: 49 Resp: 542637

Ion Ratio Lower Upper

49 100

128 53.5 25.4 76.0




130 67.6 31.9 95.9

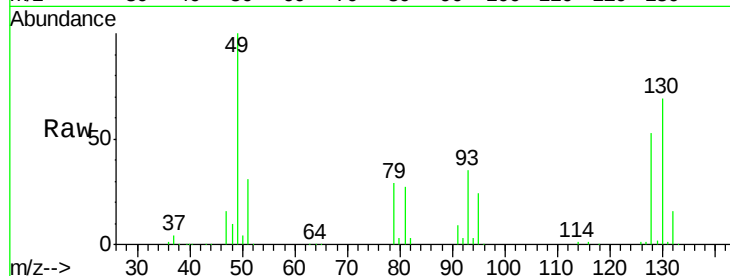

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

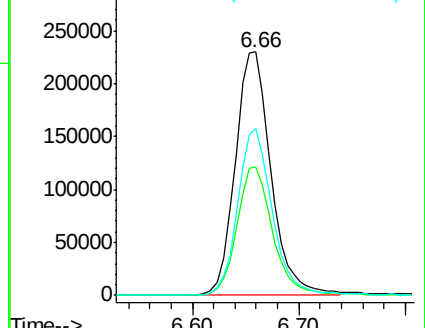

#3

Chlorodifluoromethane

Concen: 0.01 ppbv

RT: 3.57 min Scan# 79

Delta R.T. 0.00 min

Lab File: VL025612.D


Acq: 7 Jul 2015 17:16

Tgt Ion: 51 Resp: 651

Ion Ratio Lower Upper



51 100


67 0.0 19.5 29.3#



Abundance Ion 51.00 (50.70 to 51.70): VL0

Ion 67.00 (66.70 to 67.70): VL0

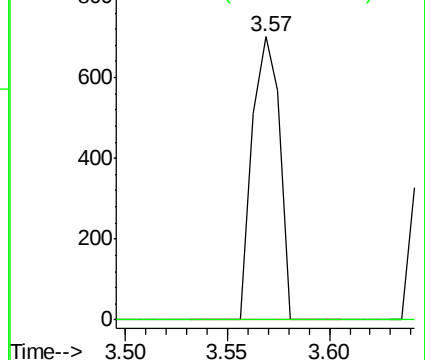

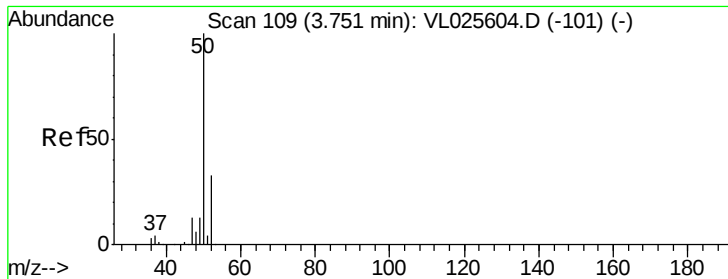

#4

Chloromethane

Concen: 0.01 ppbv

RT: 3.58 min Scan# 81

Delta R.T. -0.17 min

Lab File: VL025612.D

Acq: 7 Jul 2015 17:16

Instrument :

MSVOA_L

ClientSampleId :


VL0707ABL01

Tgt Ion: 50 Resp: 267

Ion Ratio Lower Upper




50 100

52 0.0 26.2 39.2#

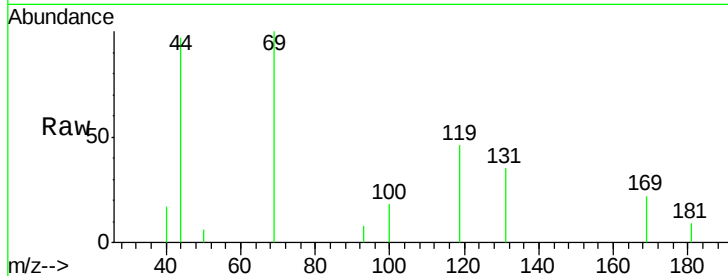

Abundance Ion 50.10 (49.80 to 50.80): VL0

Ion 52.10 (51.80 to 52.80): VL0

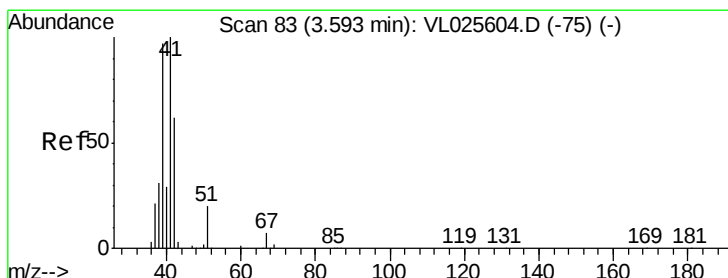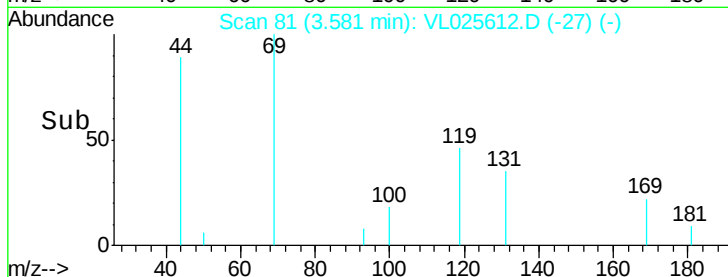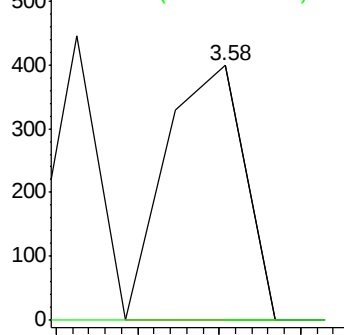

#9

Propene

Concen: 0.03 ppbv

RT: 3.61 min Scan# 85

Delta R.T. 0.01 min

Lab File: VL025612.D


Acq: 7 Jul 2015 17:16

Tgt Ion: 41 Resp: 821

Ion Ratio Lower Upper



41 100


42 23.0 52.4 78.6#

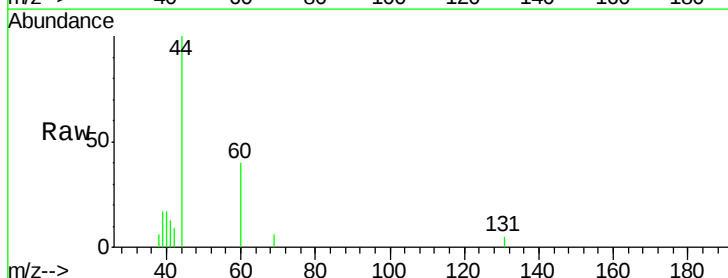

Abundance Ion 41.10 (40.80 to 41.80): VL0

Ion 42.10 (41.80 to 42.80): VL0

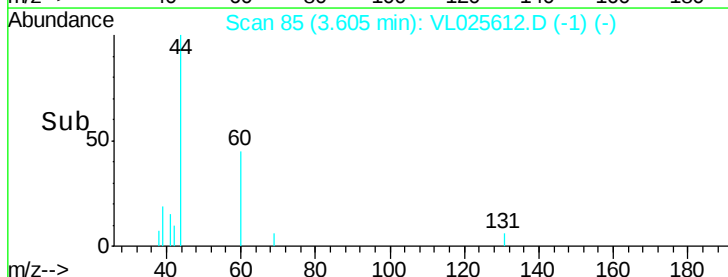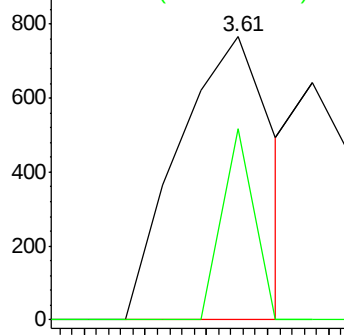



#15

Acetone

Concen: 0.22 ppbv

RT: 4.65 min Scan# 257

Delta R.T. 0.05 min

Lab File: VL025612.D

Acq: 7 Jul 2015 17:16

Instrument :

MSVOA_L

ClientSampleId :


VL0707ABL01

Tgt Ion: 43 Resp: 21073

Ion Ratio Lower Upper




43 100

58 48.8 17.2 25.8#

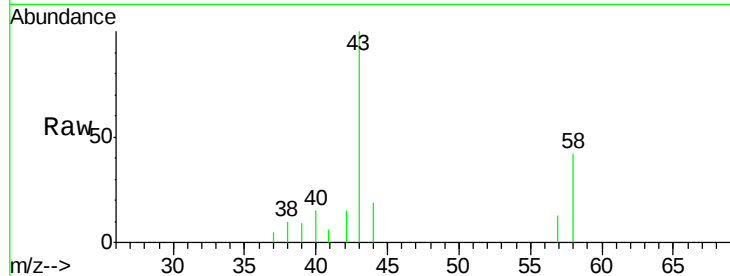

Abundance Ion 43.10 (42.80 to 43.80): VL0

Ion 58.10 (57.80 to 58.80): VL0

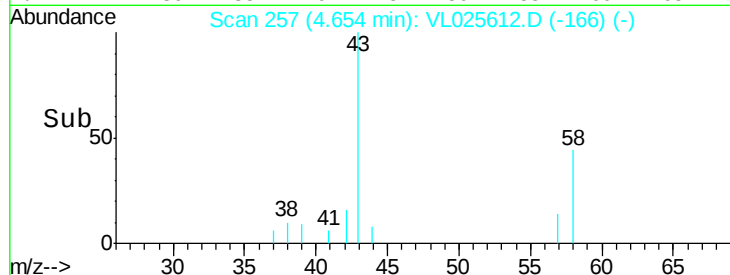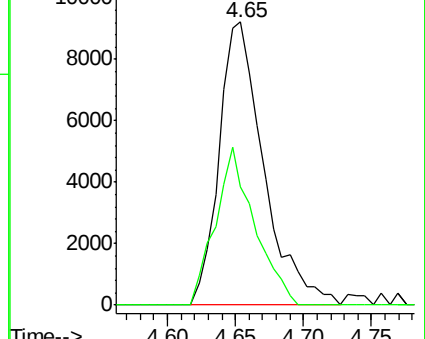

#16

1,3-Butadiene

Concen: 0.07 ppbv

RT: 3.95 min Scan# 142

Delta R.T. -0.02 min

Lab File: VL025612.D


Acq: 7 Jul 2015 17:16

Tgt Ion: 39 Resp: 2625

Ion Ratio Lower Upper



39 100


54 0.0 59.3 88.9#

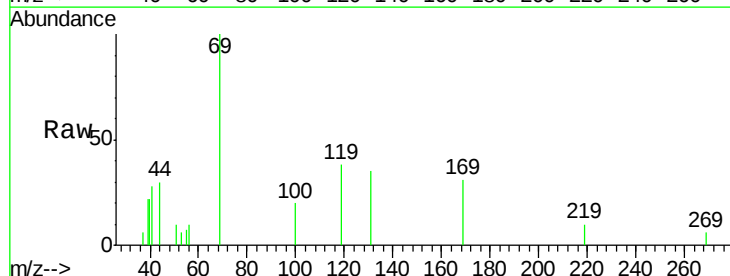

Abundance Ion 39.10 (38.80 to 39.80): VL0

Ion 54.10 (53.80 to 54.80): VL0




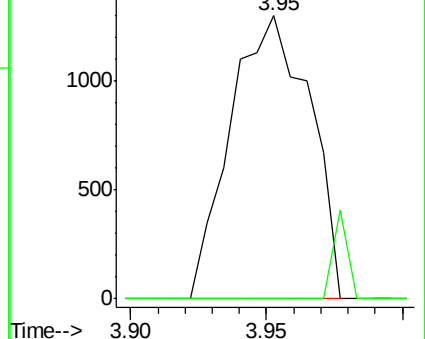


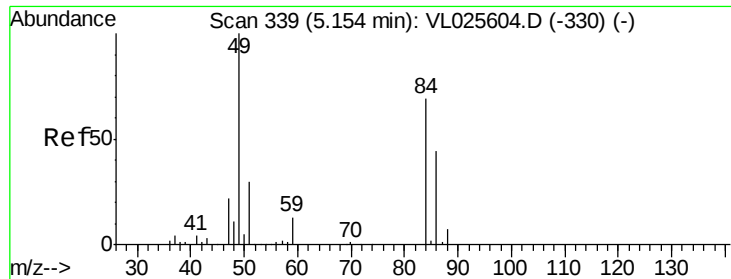

#20
Methylene Chloride
Concen: 0.05 ppbv
RT: 5.15 min Scan# 339
Delta R.T. 0.00 min
Lab File: VL025612.D
Acq: 7 Jul 2015 17:16




Instrument :
MSVOA_L
ClientSampleId :
VL0707ABL01


Tgt Ion:	84	Resp:	2095
Ion	Ratio	Lower	Upper
84	100		
49	101.3	115.2	172.8#
51	53.8	35.0	52.6#
86	62.0	50.6	76.0

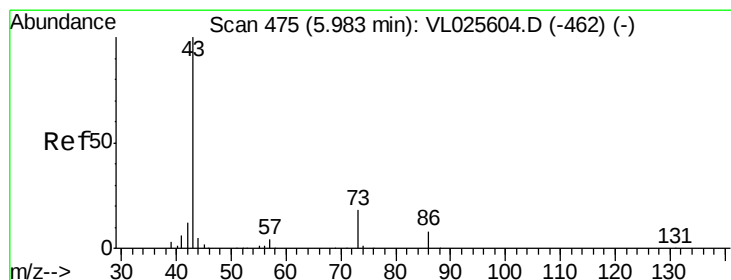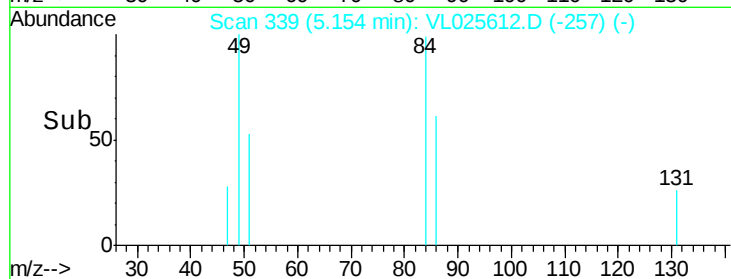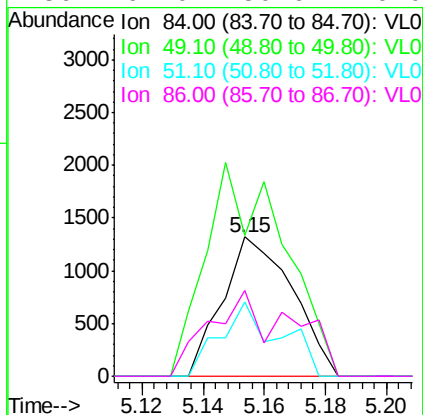

#23
Vinyl Acetate
Concen: 0.02 ppbv
RT: 6.01 min Scan# 479
Delta R.T. 0.02 min
Lab File: VL025612.D
Acq: 7 Jul 2015 17:16

Tgt Ion:	43	Resp:	2186
Ion	Ratio	Lower	Upper
43	100		
86	0.0	6.7	10.1#
42	0.0	9.8	14.6#
44	5.4	4.1	6.1


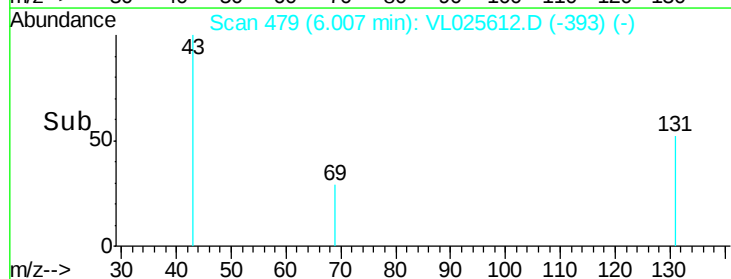
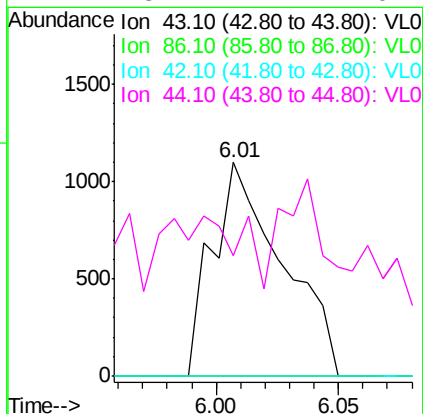
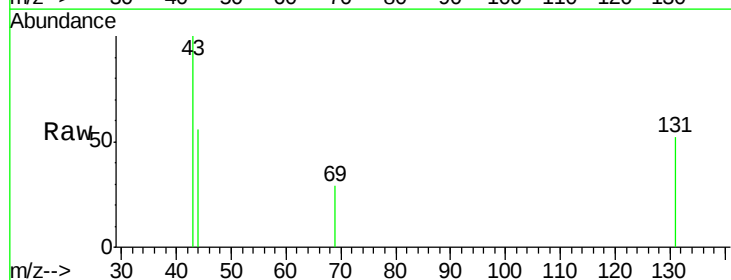




#25
Ethyl Acetate
Concen: 0.01 ppbv
RT: 6.26 min Scan# 521
Delta R.T. -0.41 min
Lab File: VL025612.D
Acq: 7 Jul 2015 17:16




Instrument :
MSVOA_L
ClientSampleId :
VL0707ABL01


Tgt Ion:	43	Resp:	1075
Ion	Ratio	Lower	Upper
43	100		
45	0.0	7.5	11.3#
61	0.0	6.6	10.0#
70	0.0	6.0	9.0#

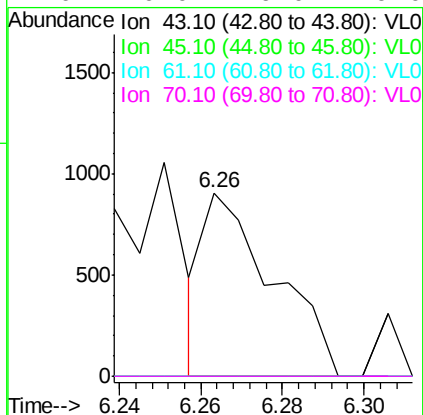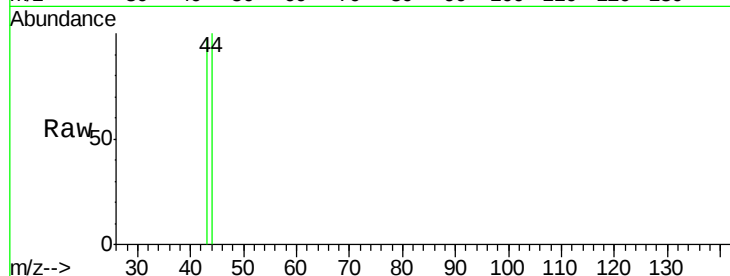

#30
Cyclohexane
Concen: 0.11 ppbv
RT: 8.31 min Scan# 857
Delta R.T. 0.02 min
Lab File: VL025612.D
Acq: 7 Jul 2015 17:16

Tgt Ion:	84	Resp:	7295
Ion	Ratio	Lower	Upper
84	100		
56	694.4	97.5	146.3#
41	0.0	65.4	98.2#

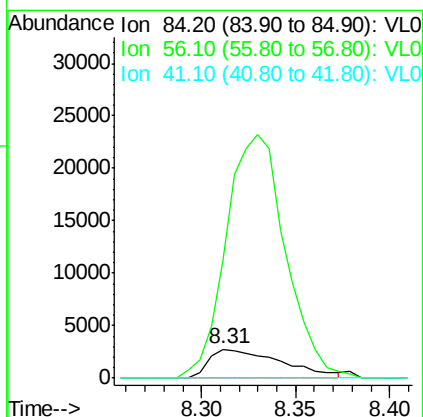


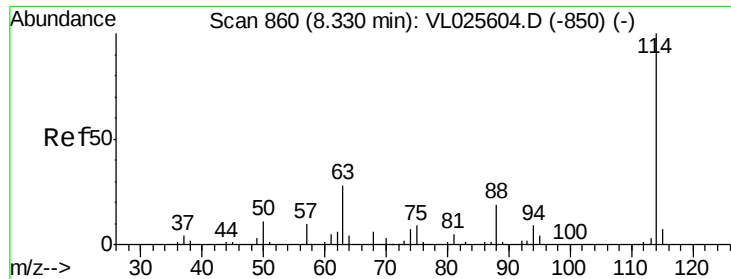




#33
 1,4-Difluorobenzene
 Concen: 10.00 ppbv
 RT: 8.33 min Scan# 860
 Delta R.T. 0.00 min
 Lab File: VL025612.D
 Acq: 7 Jul 2015 17:16

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0707ABL01

Tgt Ion:114 Resp: 1448659
 Ion Ratio Lower Upper
 114 100
 63 28.1 22.4 33.6
 88 18.7 15.0 22.4

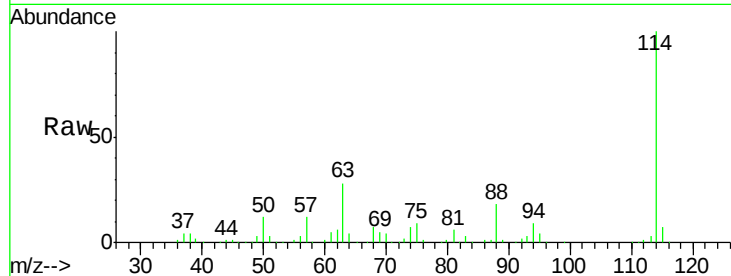


Abundance Ion 114.10 (113.80 to 114.80): VL0
 Ion 63.10 (62.80 to 63.80): VL0
 Ion 88.10 (87.80 to 88.80): VL0

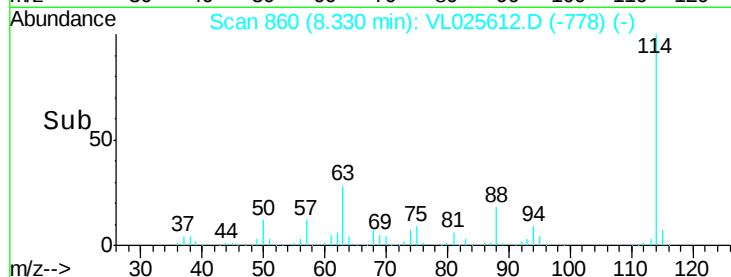
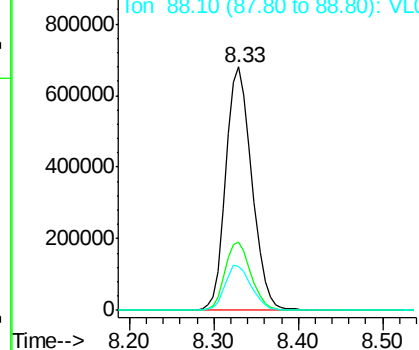



#34
 2-Butanone
 Concen: 0.00 ppbv
 RT: 6.18 min Scan# 508
 Delta R.T. -0.01 min
 Lab File: VL025612.D
 Acq: 7 Jul 2015 17:16

Tgt Ion: 43 Resp: 123
 Ion Ratio Lower Upper
 43 100
 72 0.0 18.6 28.0#



Abundance Ion 43.10 (42.80 to 43.80): VL0
 Ion 72.10 (71.80 to 72.80): VL0

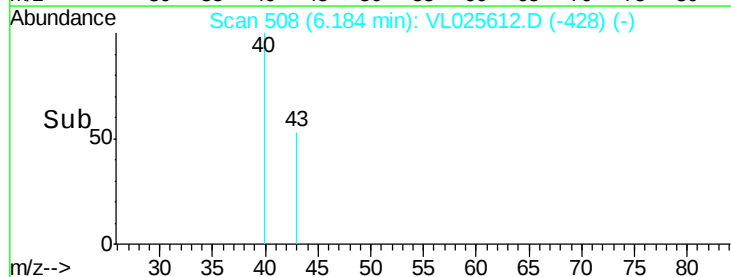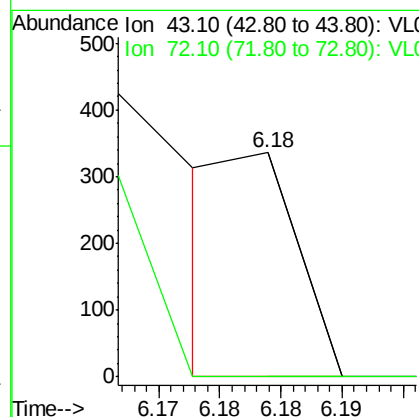

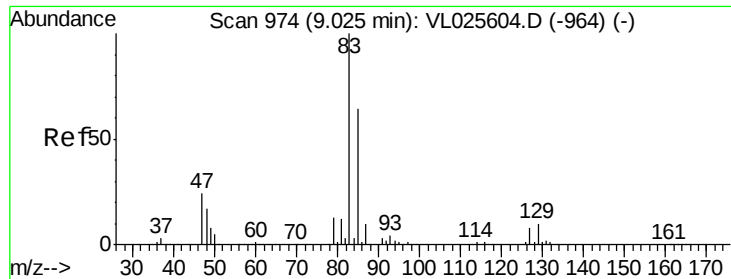

#42

Bromodichloromethane

Concen: 0.00 ppbv

RT: 8.72 min Scan# 924

Delta R.T. -0.30 min

Lab File: VL025612.D

Acq: 7 Jul 2015 17:16

Instrument :

MSVOA_L

ClientSampleId :

VL0707ABL01


Tgt Ion: 83 Resp: 147

Ion Ratio Lower Upper

83 100

85 0.0 51.3 76.9#




127 0.0 6.0 9.0#

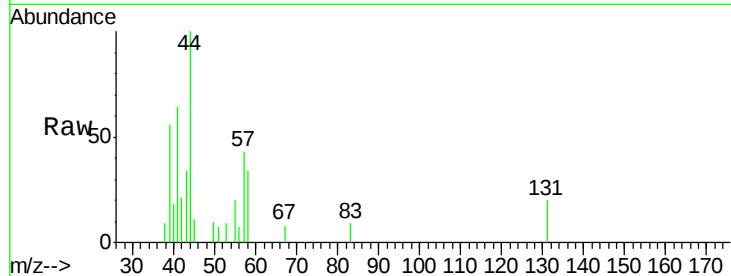

Abundance Ion 83.00 (82.70 to 83.70): VL0

Ion 85.00 (84.70 to 85.70): VL0

Ion 126.90 (126.60 to 127.60): VL0

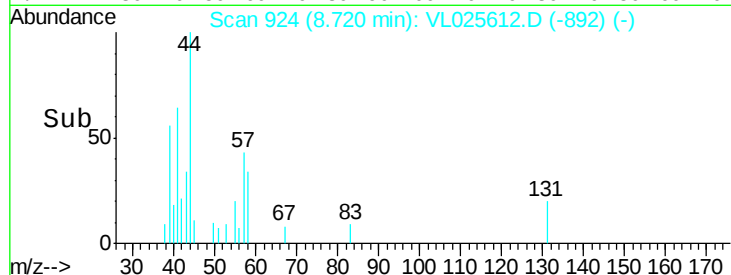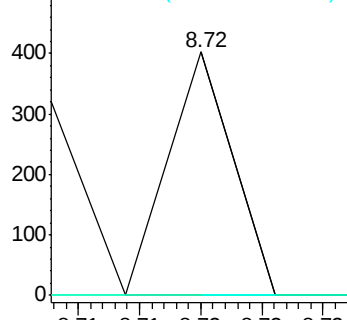

#43

Methyl Methacrylate

Concen: 0.00 ppbv

RT: 8.79 min Scan# 935

Delta R.T. -0.48 min

Lab File: VL025612.D

Acq: 7 Jul 2015 17:16


Tgt Ion: 69 Resp: 113

Ion Ratio Lower Upper

69 100

41 0.0 117.3 175.9#



100 0.0 29.0 43.6#




Abundance Ion 69.10 (68.80 to 69.80): VL0

Ion 41.10 (40.80 to 41.80): VL0

Ion 100.10 (99.80 to 100.80): VL0



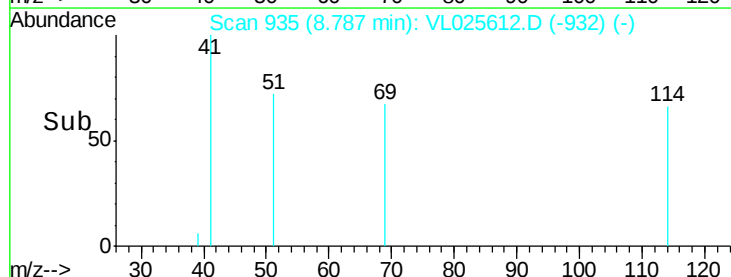
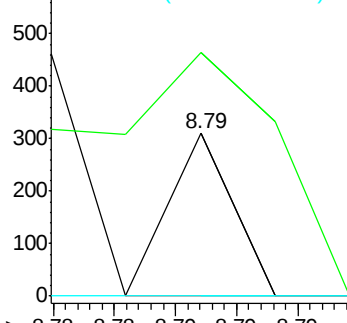


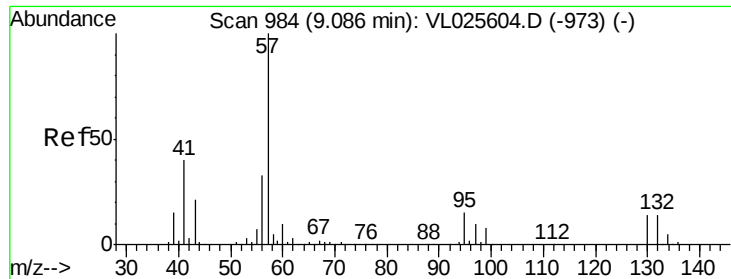

#44
2,2,4-Trimethylpentane
Concen: 0.00 ppbv
RT: 8.76 min Scan# 931
Delta R.T. -0.32 min
Lab File: VL025612.D
Acq: 7 Jul 2015 17:16




Instrument :
MSVOA_L
ClientSampleId :
VL0707ABL01


Tgt Ion: 57 Resp: 309
Ion Ratio Lower Upper
57 100
41 0.0 31.2 46.8#
56 0.0 25.4 38.2#

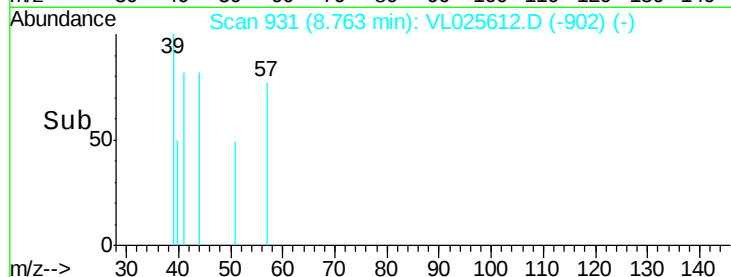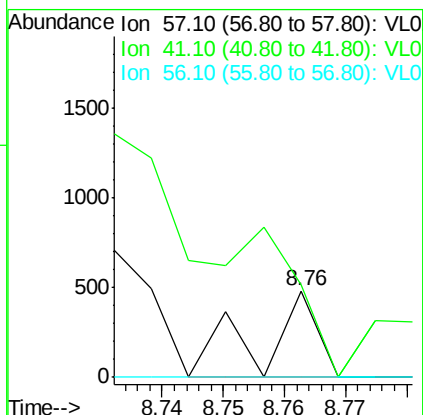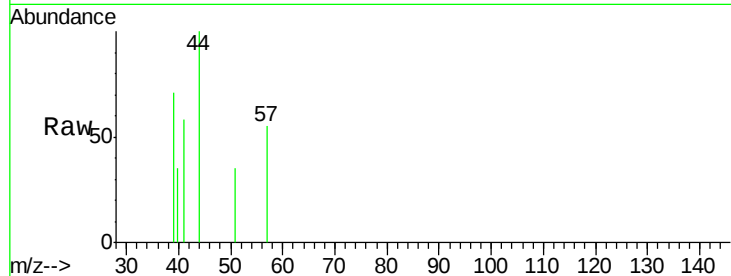

#51
2-Hexanone
Concen: 0.22 ppbv
RT: 11.94 min Scan# 1452
Delta R.T. 0.32 min
Lab File: VL025612.D
Acq: 7 Jul 2015 17:16

Tgt Ion: 43 Resp: 23867
Ion Ratio Lower Upper
43 100
58 11.8 39.0 58.6#
98 5.9 0.2 0.4#

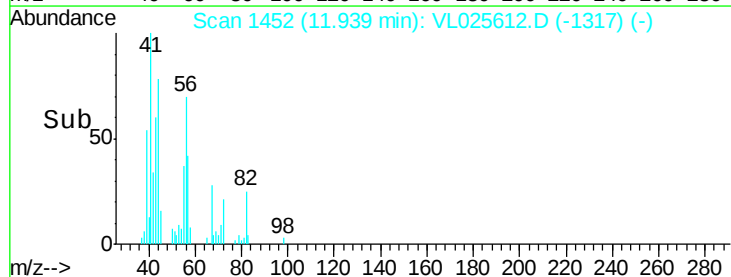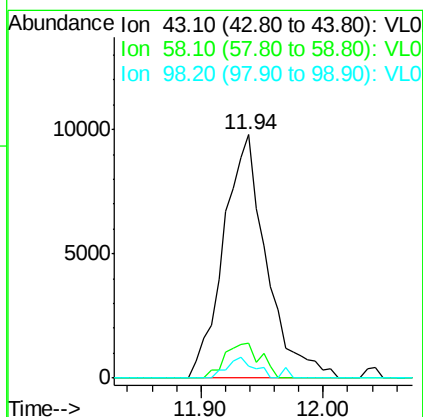



#52

Tetrachloroethene

Concen: 0.04 ppbv

RT: 13.22 min Scan# 1662

Delta R.T. 0.43 min

Lab File: VL025612.D

Acq: 7 Jul 2015 17:16

Instrument :

MSVOA_L

ClientSampleId :

VL0707ABL01

Tgt Ion:164 Resp: 3011


Ion Ratio Lower Upper

164 100

166 23.1 102.3 153.5#

129 21.2 86.2 129.4#

131 60.8 80.3 120.5#






Abundance Ion 163.90 (163.60 to 164.60): V

Ion 165.90 (165.60 to 166.60): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

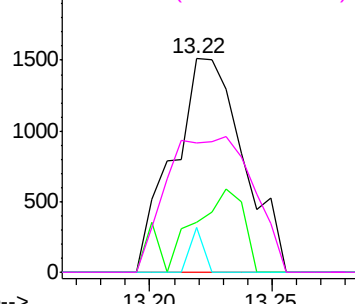

#55

Chlorobenzene-d5

Concen: 10.00 ppbv

RT: 13.75 min Scan# 1749

Delta R.T. 0.00 min

Lab File: VL025612.D

Acq: 7 Jul 2015 17:16


Tgt Ion:117 Resp: 1975781

Ion Ratio Lower Upper

117 100

82 65.9 50.5 75.7



119 33.0 45.1 67.7#




Abundance Ion 117.10 (116.80 to 117.80): V

Ion 82.10 (81.80 to 82.80): V

Ion 119.10 (118.80 to 119.80): V

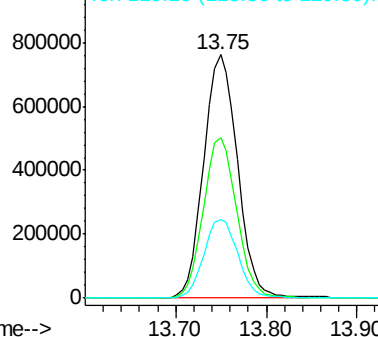

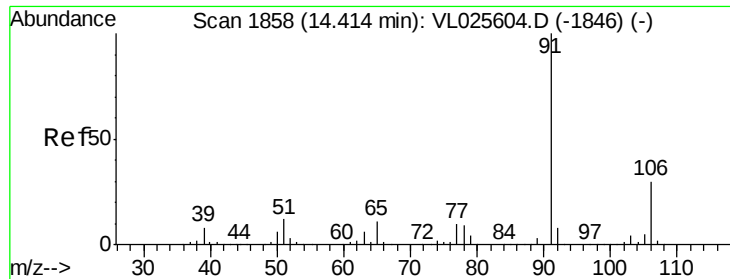

#58

Ethyl Benzene

Concen: 0.00 ppbv

RT: 14.41 min Scan# 1858

Delta R.T. 0.00 min

Lab File: VL025612.D

Acq: 7 Jul 2015 17:16

Instrument :

MSVOA_L

ClientSampleId :


VL0707ABL01

Tgt Ion: 91 Resp: 129

Ion Ratio Lower Upper

91 100

106 0.0 24.2 36.2#



Abundance Ion 91.10 (90.80 to 91.80): VL0

Ion 106.10 (105.80 to 106.80): V

14.41

300

200



100

0

14.41

14.42

Time-->



#59

m/p-Xylene

Concen: 0.00 ppbv

RT: 14.73 min Scan# 1910

Delta R.T. 0.01 min

Lab File: VL025612.D


Acq: 7 Jul 2015 17:16

Tgt Ion: 91 Resp: 250

Ion Ratio Lower Upper

91 100

106 0.0 37.9 56.9#



Abundance Ion 91.10 (90.80 to 91.80): VL0

Ion 106.10 (105.80 to 106.80): V

14.73

800

600

400

200


0


14.72

14.73

14.74

Time-->









#60
o-Xylene
Concen: 0.00 ppbv
RT: 15.49 min Scan# 2034
Delta R.T. -0.01 min
Lab File: VL025612.D
Acq: 7 Jul 2015 17:16




Instrument :
MSVOA_L
ClientSampleId :
VL0707ABL01


Tgt Ion: 91 Resp: 626
Ion Ratio Lower Upper
91 100
106 0.0 22.1 66.1#

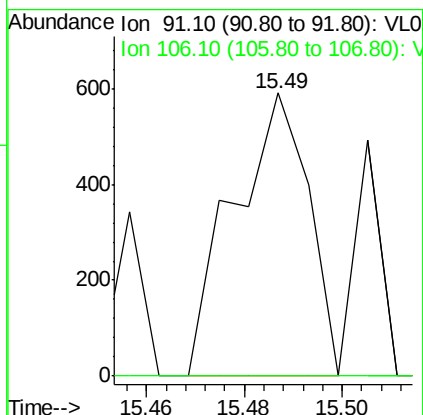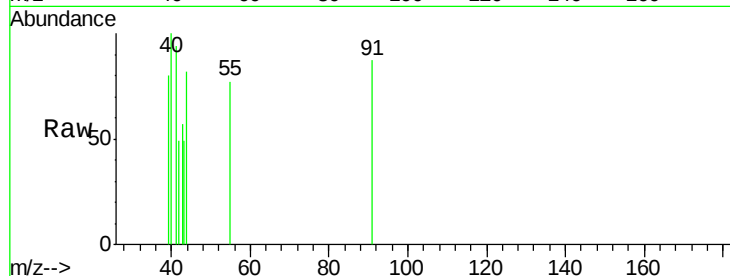

#62
Isopropylbenzene
Concen: 0.00 ppbv
RT: 16.30 min Scan# 2168
Delta R.T. -0.24 min
Lab File: VL025612.D
Acq: 7 Jul 2015 17:16

Tgt Ion: 105 Resp: 722
Ion Ratio Lower Upper
105 100
120 0.0 20.6 31.0#



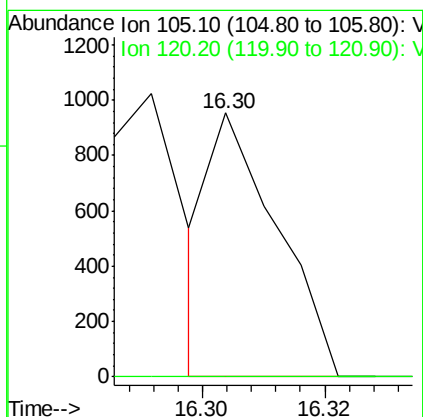



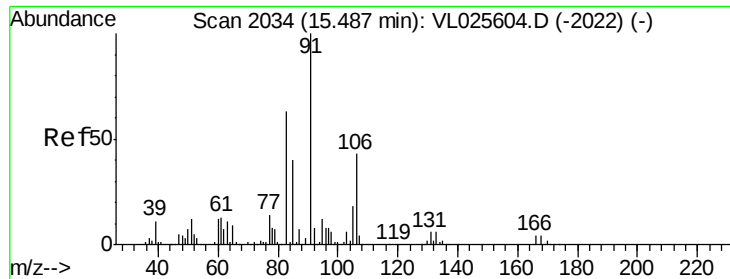

#63
 1,1,2,2-Tetrachloroethane
 Concen: 0.00 ppbv
 RT: 15.39 min Scan# 2018
 Delta R.T. -0.10 min
 Lab File: VL025612.D
 Acq: 7 Jul 2015 17:16




Instrument :
 MSVOA_L
 ClientSampleId :
 VL0707ABL01


Tgt Ion: 83 Resp: 243
 Ion Ratio Lower Upper
 83 100
 131 0.0 4.8 14.4#
 85 0.0 32.4 97.2#

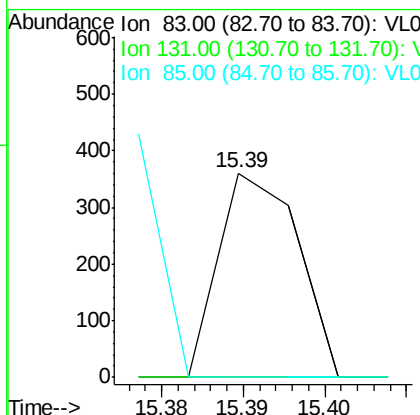

#65
 tert-Butylbenzene
 Concen: 0.16 ppbv
 RT: 18.92 min Scan# 2597
 Delta R.T. 0.10 min
 Lab File: VL025612.D
 Acq: 7 Jul 2015 17:16

Tgt Ion: 119 Resp: 63469
 Ion Ratio Lower Upper
 119 100
 91 3.6 64.5 96.7#
 134 46.1 17.4 26.0#

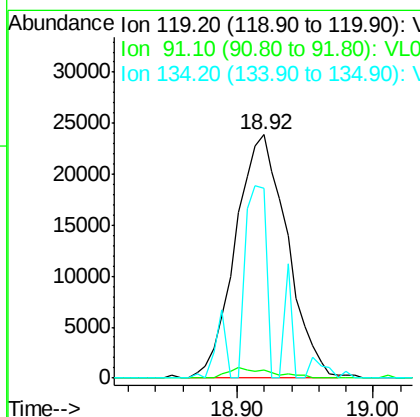


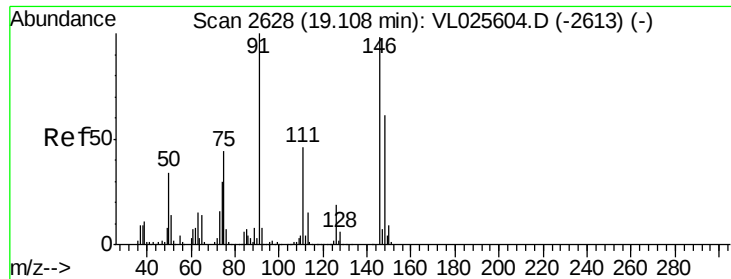




#66
Benzyl Chloride
Concen: 0.00 ppbv
RT: 18.94 min Scan# 2600
Delta R.T. -0.17 min
Lab File: VL025612.D
Acq: 7 Jul 2015 17:16

Instrument :
MSVOA_L
ClientSampleId :
VL0707ABL01

Tgt Ion: 91 Resp: 396
Ion Ratio Lower Upper
91 100
126 278.5 14.5 21.7#
128 0.0 4.6 7.0#

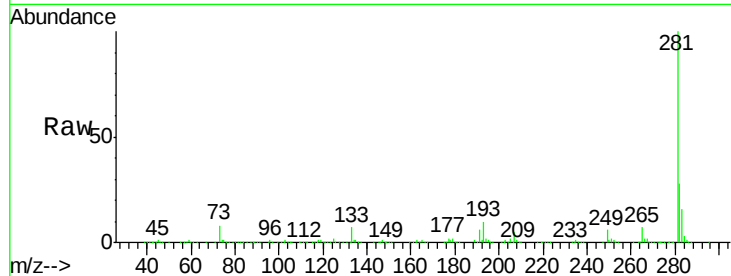


Abundance Ion 91.10 (90.80 to 91.80): VL0
Ion 126.10 (125.80 to 126.80): V
Ion 128.10 (127.80 to 128.80): V

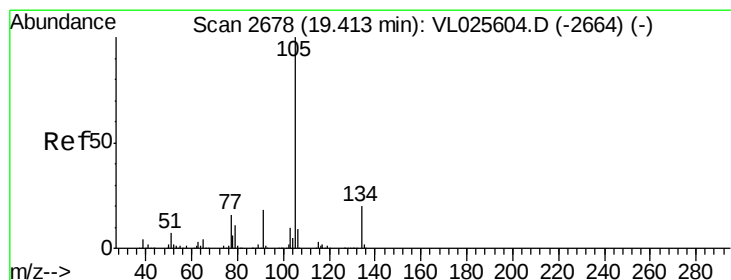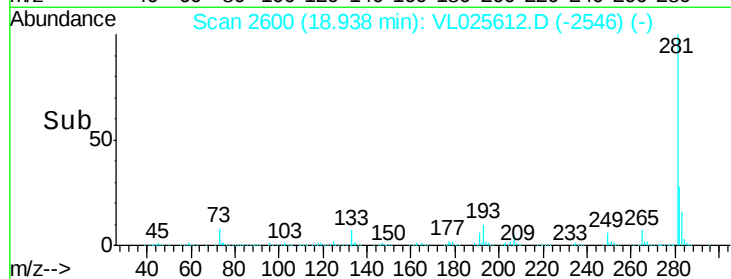
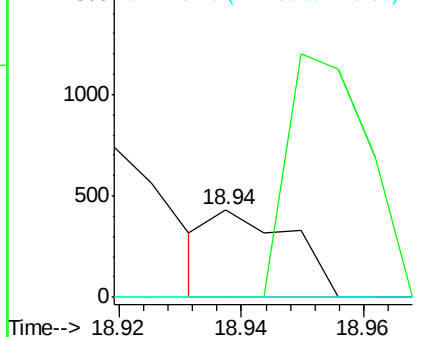



#67
sec-Butylbenzene
Concen: 0.00 ppbv
RT: 18.97 min Scan# 2606
Delta R.T. -0.44 min
Lab File: VL025612.D
Acq: 7 Jul 2015 17:16

Tgt Ion: 105 Resp: 163
Ion Ratio Lower Upper
105 100
134 1129.4 15.4 23.2#



Abundance Ion 105.10 (104.80 to 105.80): V
Ion 134.20 (133.90 to 134.90): V

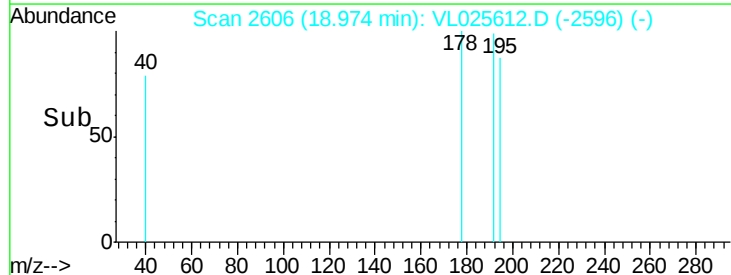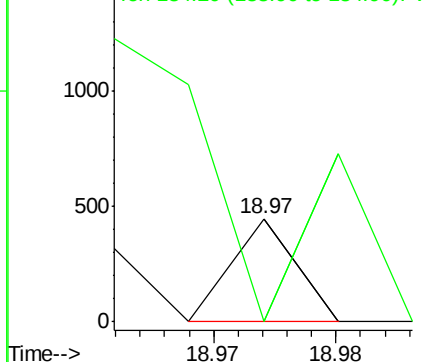


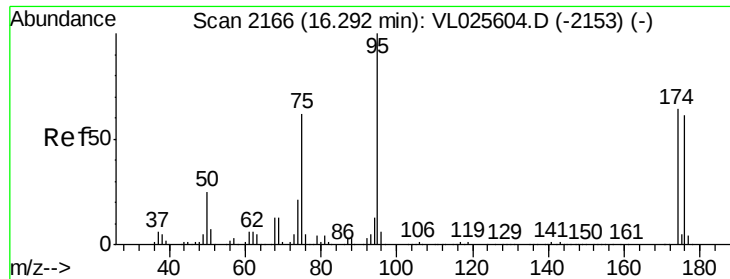




#68
 1-Bromo-4-Fluorobenzene
 Concen: 10.07 ppbv
 RT: 16.29 min Scan# 2166
 Delta R.T. 0.00 min
 Lab File: VL025612.D
 Acq: 7 Jul 2015 17:16

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0707ABL01

Tgt Ion: 95 Resp: 1678830
 Ion Ratio Lower Upper
 95 100
 174 64.6 52.0 78.0
 175 4.7 3.9 5.9

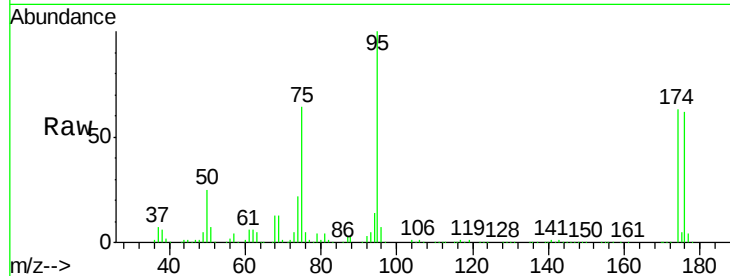


Abundance Ion 95.10 (94.80 to 95.80): VL0
 Ion 174.00 (173.70 to 174.70): V
 Ion 175.00 (174.70 to 175.70): V

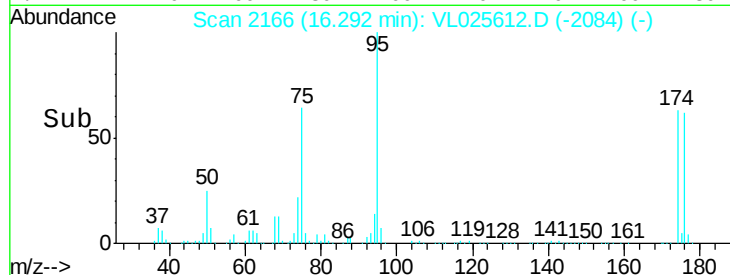
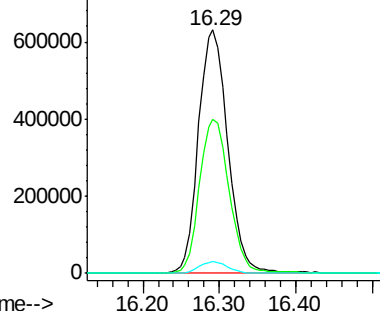



#74
 1,2,4-Trimethylbenzene
 Concen: 0.00 ppbv
 RT: 18.85 min Scan# 2585
 Delta R.T. 0.01 min
 Lab File: VL025612.D
 Acq: 7 Jul 2015 17:16

Tgt Ion: 105 Resp: 455
 Ion Ratio Lower Upper
 105 100
 120 0.0 39.3 58.9#
 91 0.0 43.8 65.6#
 77 0.0 18.3 27.5#



Abundance Ion 105.10 (104.80 to 105.80): V
 Ion 120.20 (119.90 to 120.90): V
 Ion 91.10 (90.80 to 91.80): VL0
 Ion 77.10 (76.80 to 77.80): VL0

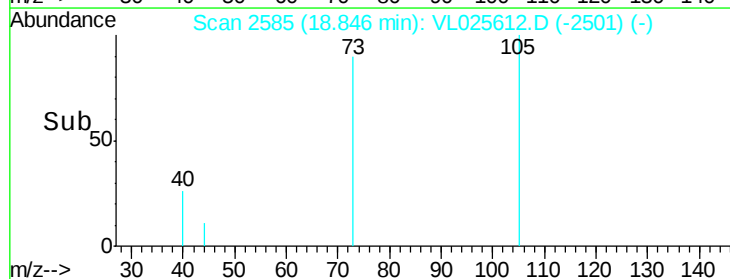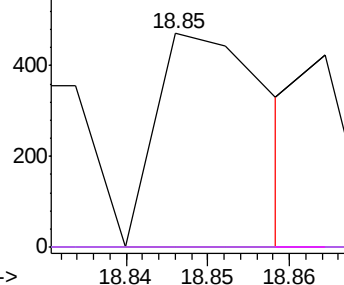


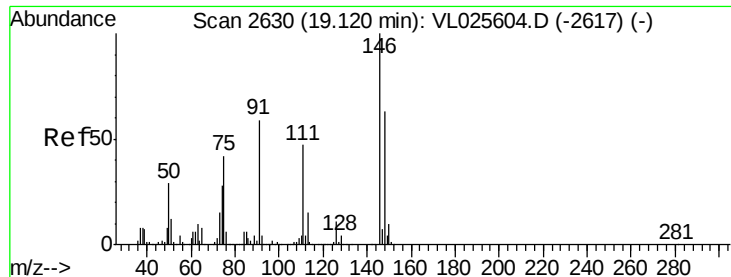




#75
 1,3-Dichlorobenzene
 Concen: 0.00 ppbv
 RT: 18.94 min Scan# 2600
 Delta R.T. -0.18 min
 Lab File: VL025612.D
 Acq: 7 Jul 2015 17:16

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0707ABL01

Tgt Ion:146 Resp: 239
 Ion Ratio Lower Upper
 146 100
 111 0.0 22.7 68.1#
 148 0.0 31.8 95.3#




Abundance Ion 146.00 (145.70 to 146.70): V
 Ion 111.10 (110.80 to 111.80): V
 Ion 148.00 (147.70 to 148.70): V

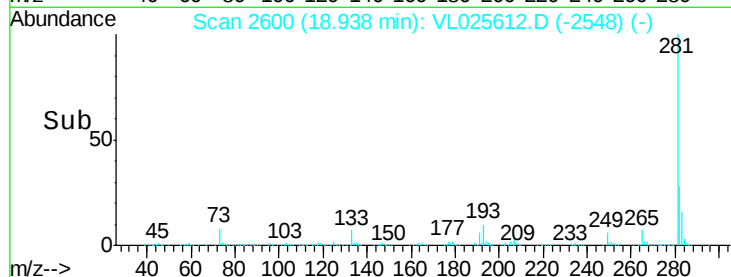
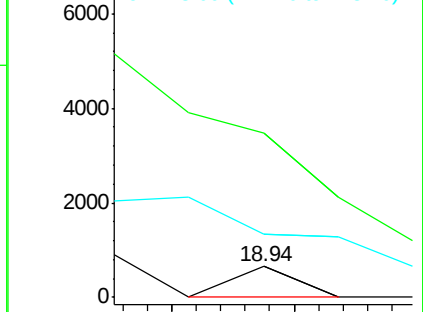



#76
 1,4-Dichlorobenzene
 Concen: 0.00 ppbv
 RT: 18.94 min Scan# 2600
 Delta R.T. -0.34 min
 Lab File: VL025612.D
 Acq: 7 Jul 2015 17:16

Tgt Ion:146 Resp: 239
 Ion Ratio Lower Upper
 146 100
 111 0.0 22.1 66.1#
 148 0.0 31.9 95.9#



Abundance Ion 146.00 (145.70 to 146.70): V
 Ion 111.10 (110.80 to 111.80): V
 Ion 148.00 (147.70 to 148.70): V

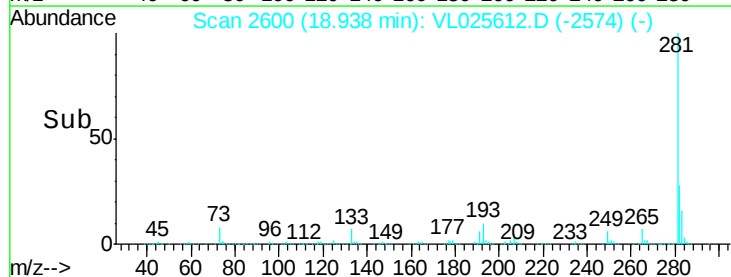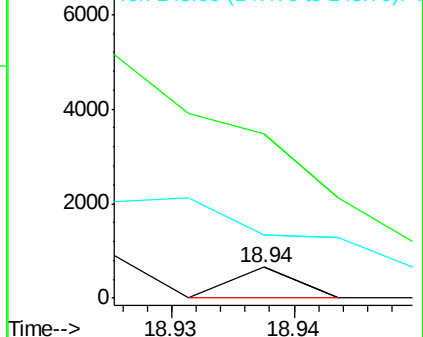



#79

Naphthalene

Concen: 0.00 ppbv

RT: 23.96 min Scan# 3424

Delta R.T. 0.04 min

Lab File: VL025612.D

Acq: 7 Jul 2015 17:16

Instrument :

MSVOA_L

ClientSampleId :

VL0707ABL01


Tgt Ion:128 Resp: 908

Ion Ratio Lower Upper

128 100

127 0.0 10.8 16.2#




129 0.0 9.0 13.4#



Abundance Ion 128.10 (127.80 to 128.80): V

Ion 127.10 (126.80 to 127.80): V

Ion 129.10 (128.80 to 129.80): V

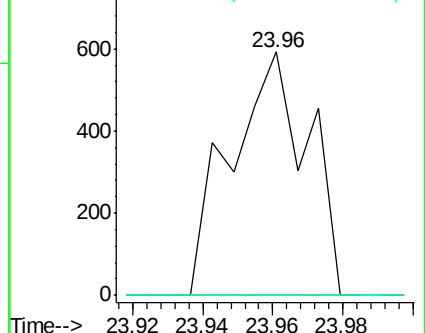

#80

Naphthalene, 2-methyl-

Concen: 0.00 ppbv

RT: 26.11 min Scan# 3776

Delta R.T. 0.07 min

Lab File: VL025612.D

Acq: 7 Jul 2015 17:16


Tgt Ion:142 Resp: 162

Ion Ratio Lower Upper

142 100

141 0.0 67.1 100.7#

115 227.2 33.9 50.9#



Abundance Ion 142.00 (141.70 to 142.70): V

Ion 141.00 (140.70 to 141.70): V

Ion 115.00 (114.70 to 115.70): V

