


Data Path : W:\HPCHEM1\MSVOA_L\Data\VL070715\
Data File : VL025603.D
Acq On : 7 Jul 2015 9:53
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL070715AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Jun 03 16:25:57 2015
Last Update : Wed Jun 03 16:25:57 2015

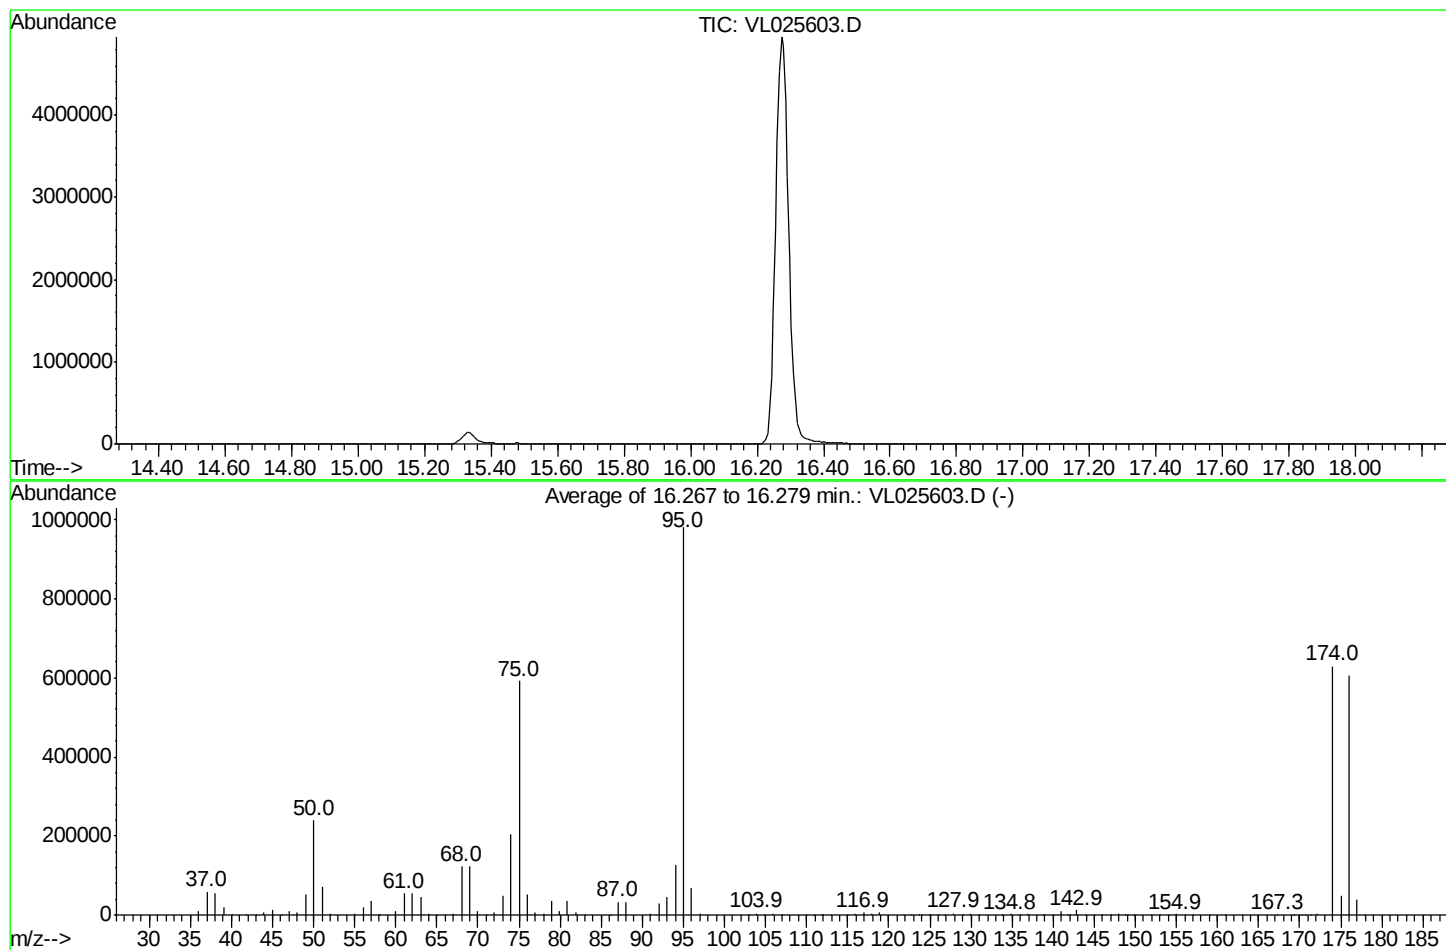

AutoFind: Scans 2162, 2163, 2164; Background Corrected with Scan 2145

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.3	238720	PASS
75	95	30	66	60.4	592085	PASS
95	95	100	100	100.0	980928	PASS
96	95	5	9	6.8	66538	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	64.1	628586	PASS
175	174	4	9	7.7	48184	PASS
176	174	93	101	96.3	605056	PASS
177	176	5	9	6.5	39386	PASS