


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL070819\
Data File : VL034007.D
Acq On : 8 Jul 2019 10:26
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL070219AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Jul 02 19:31:31 2019
Last Update : Tue Jul 02 19:31:31 2019

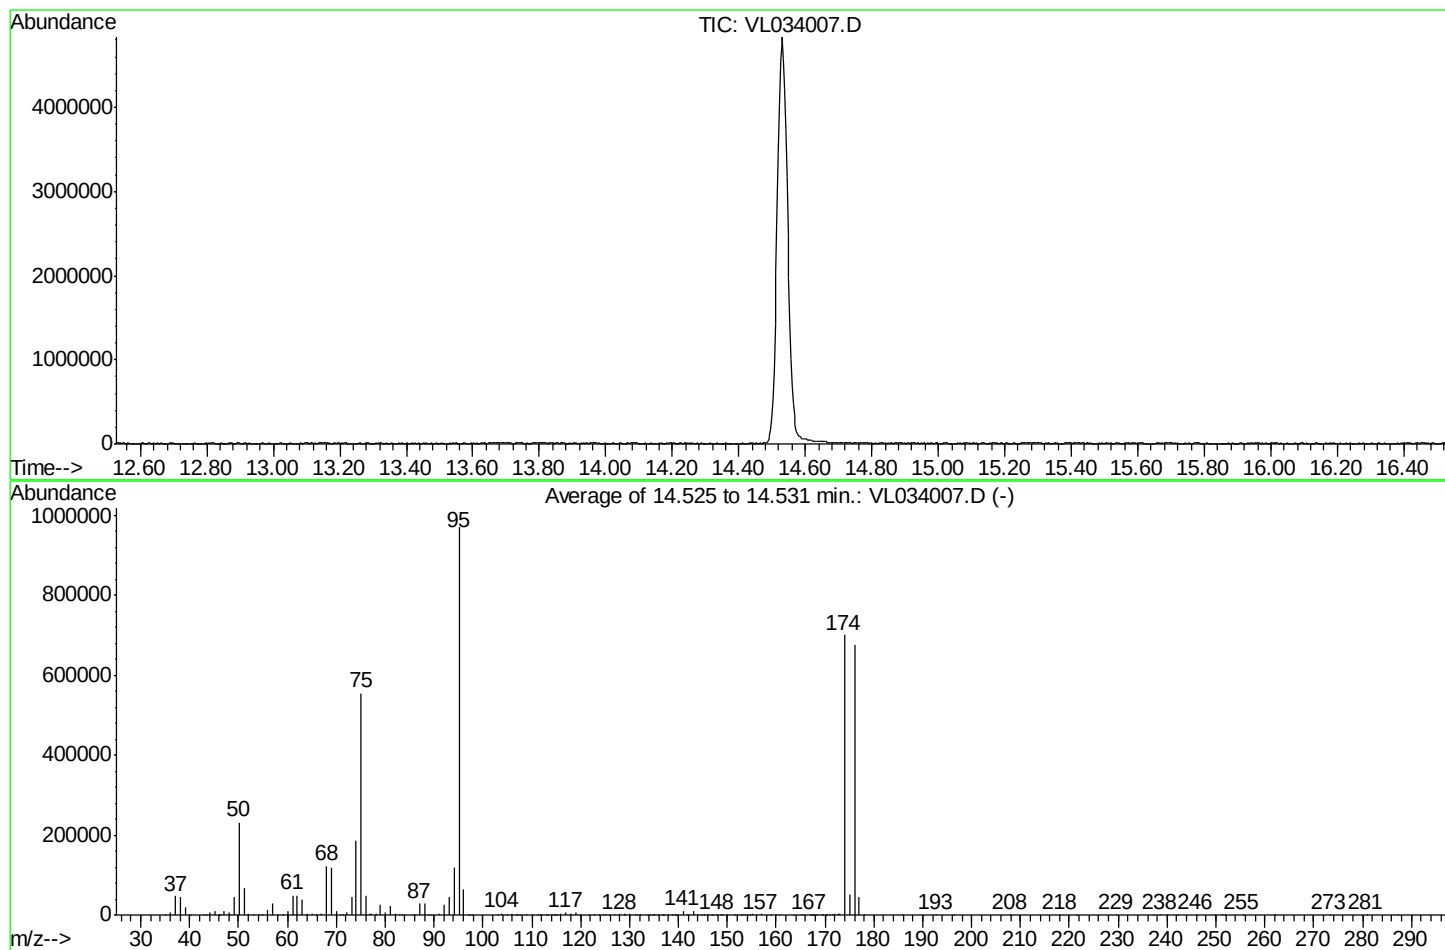

AutoFind: Scans 3604, 3605, 3606; Background Corrected with Scan 3579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	231658	PASS
75	95	30	66	57.2	553941	PASS
95	95	100	100	100.0	969258	PASS
96	95	5	9	6.7	64850	PASS
173	174	0.00	2	0.5	3779	PASS
174	95	50	120	72.3	700629	PASS
175	174	4	9	7.3	51496	PASS
176	174	93	101	96.2	674048	PASS
177	176	5	9	6.9	46450	PASS