


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL071119\
 Data File : VL034016.D
 Acq On : 11 Jul 2019 12:22
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL070219AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Jul 02 19:31:31 2019
 Last Update : Tue Jul 02 19:31:31 2019

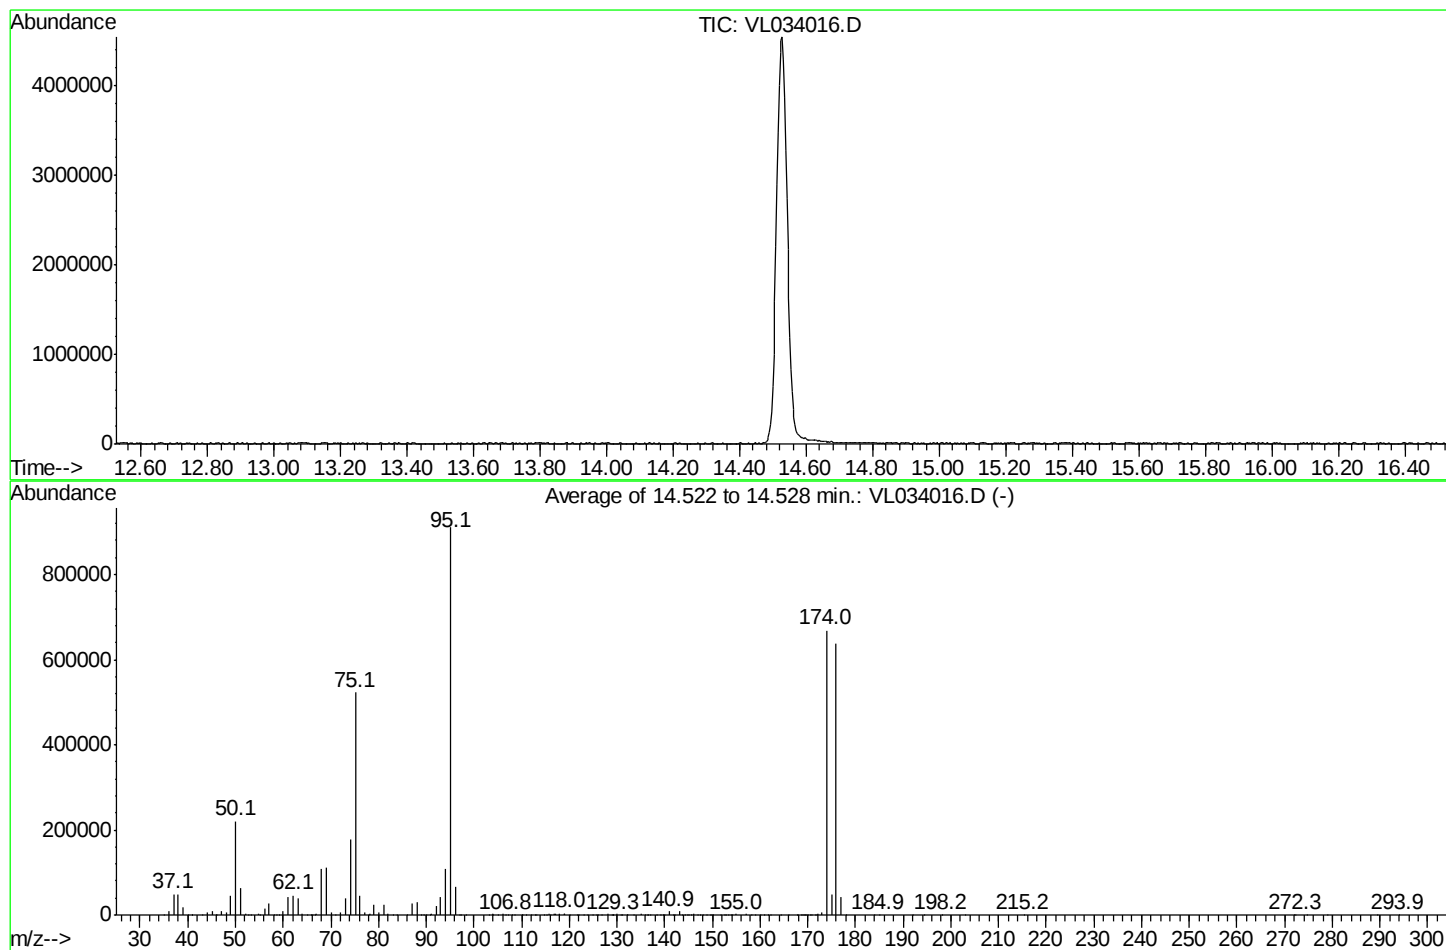

AutoFind: Scans 3603, 3604, 3605; Background Corrected with Scan 3576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.3	220949	PASS
75	95	30	66	57.4	522560	PASS
95	95	100	100	100.0	910976	PASS
96	95	5	9	7.2	65602	PASS
173	174	0.00	2	0.8	5201	PASS
174	95	50	120	73.5	669226	PASS
175	174	4	9	7.1	47816	PASS
176	174	93	101	95.4	638549	PASS
177	176	5	9	6.5	41754	PASS