


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL071218\
 Data File : VL032227.D
 Acq On : 12 Jul 2018 17:23
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL071218AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Jul 13 04:25:14 2018
 Last Update : Fri Jul 13 04:25:14 2018

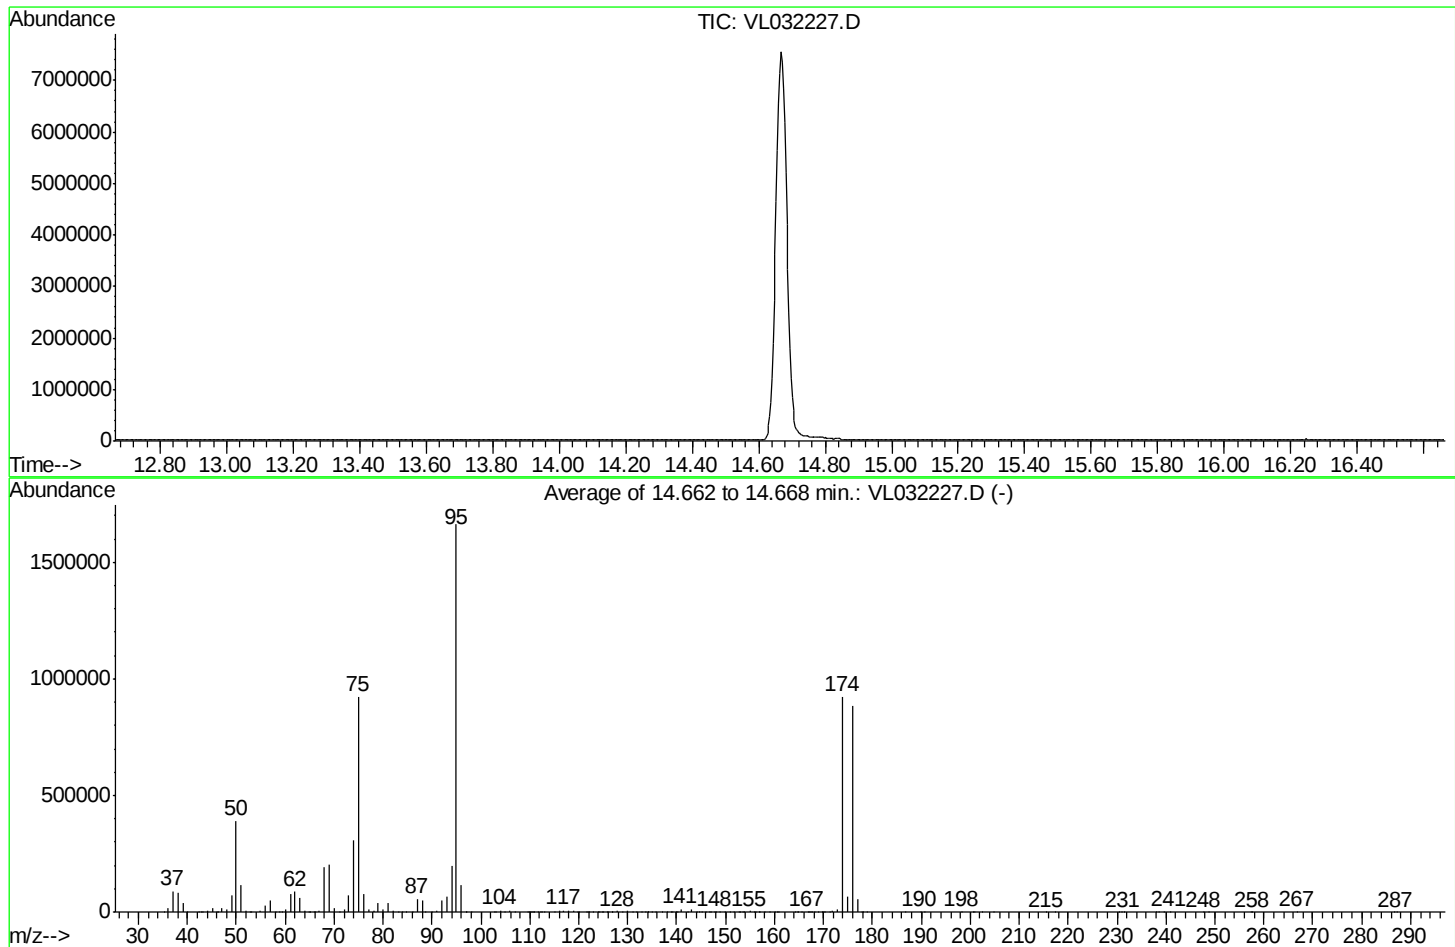

AutoFind: Scans 4222, 4223, 4224; Background Corrected with Scan 4197

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.5	390101	PASS
75	95	30	66	55.5	922666	PASS
95	95	100	100	100.0	1662805	PASS
96	95	5	9	6.8	113861	PASS
173	174	0.00	2	1.1	10136	PASS
174	95	50	120	55.6	924906	PASS
175	174	4	9	7.2	66208	PASS
176	174	93	101	95.5	882986	PASS
177	176	5	9	6.2	55013	PASS