


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL071318\
 Data File : VL032244.D
 Acq On : 13 Jul 2018 11:57
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL071218AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Jul 13 04:25:14 2018
 Last Update : Fri Jul 13 04:25:14 2018

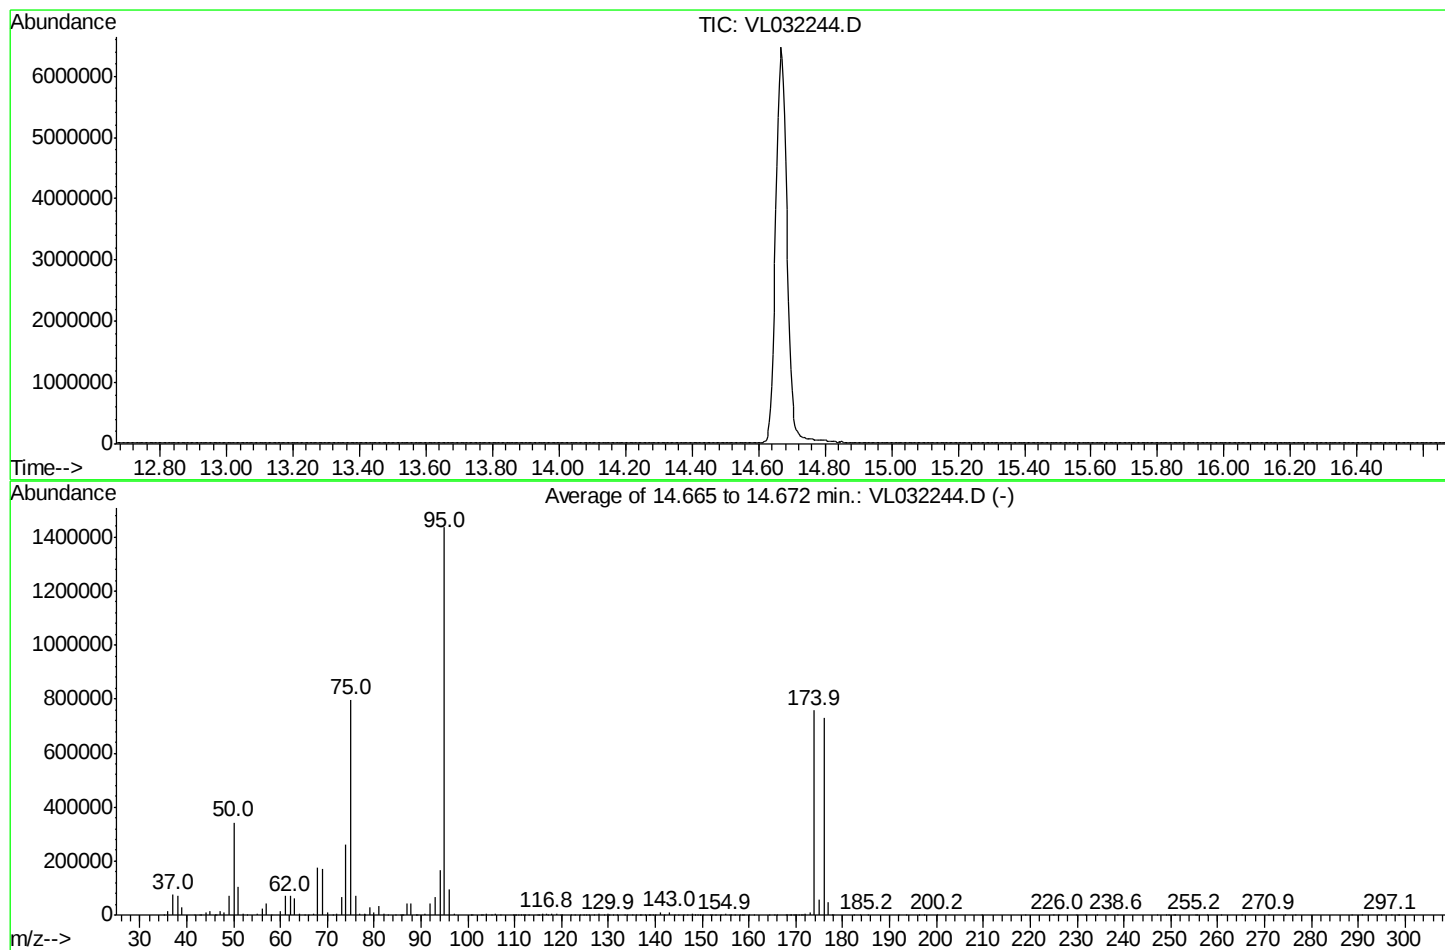

AutoFind: Scans 4223, 4224, 4225; Background Corrected with Scan 4200

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	343594	PASS
75	95	30	66	55.5	797461	PASS
95	95	100	100	100.0	1436330	PASS
96	95	5	9	6.5	93184	PASS
173	174	0.00	2	1.0	7593	PASS
174	95	50	120	52.7	757333	PASS
175	174	4	9	7.3	55226	PASS
176	174	93	101	96.6	731904	PASS
177	176	5	9	6.8	49568	PASS