


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL071322\
 Data File : VL039468.D
 Acq On : 13 Jul 2022 14:34
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL062922AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Jul 06 02:15:38 2022
 Last Update : Wed Jul 06 02:15:38 2022

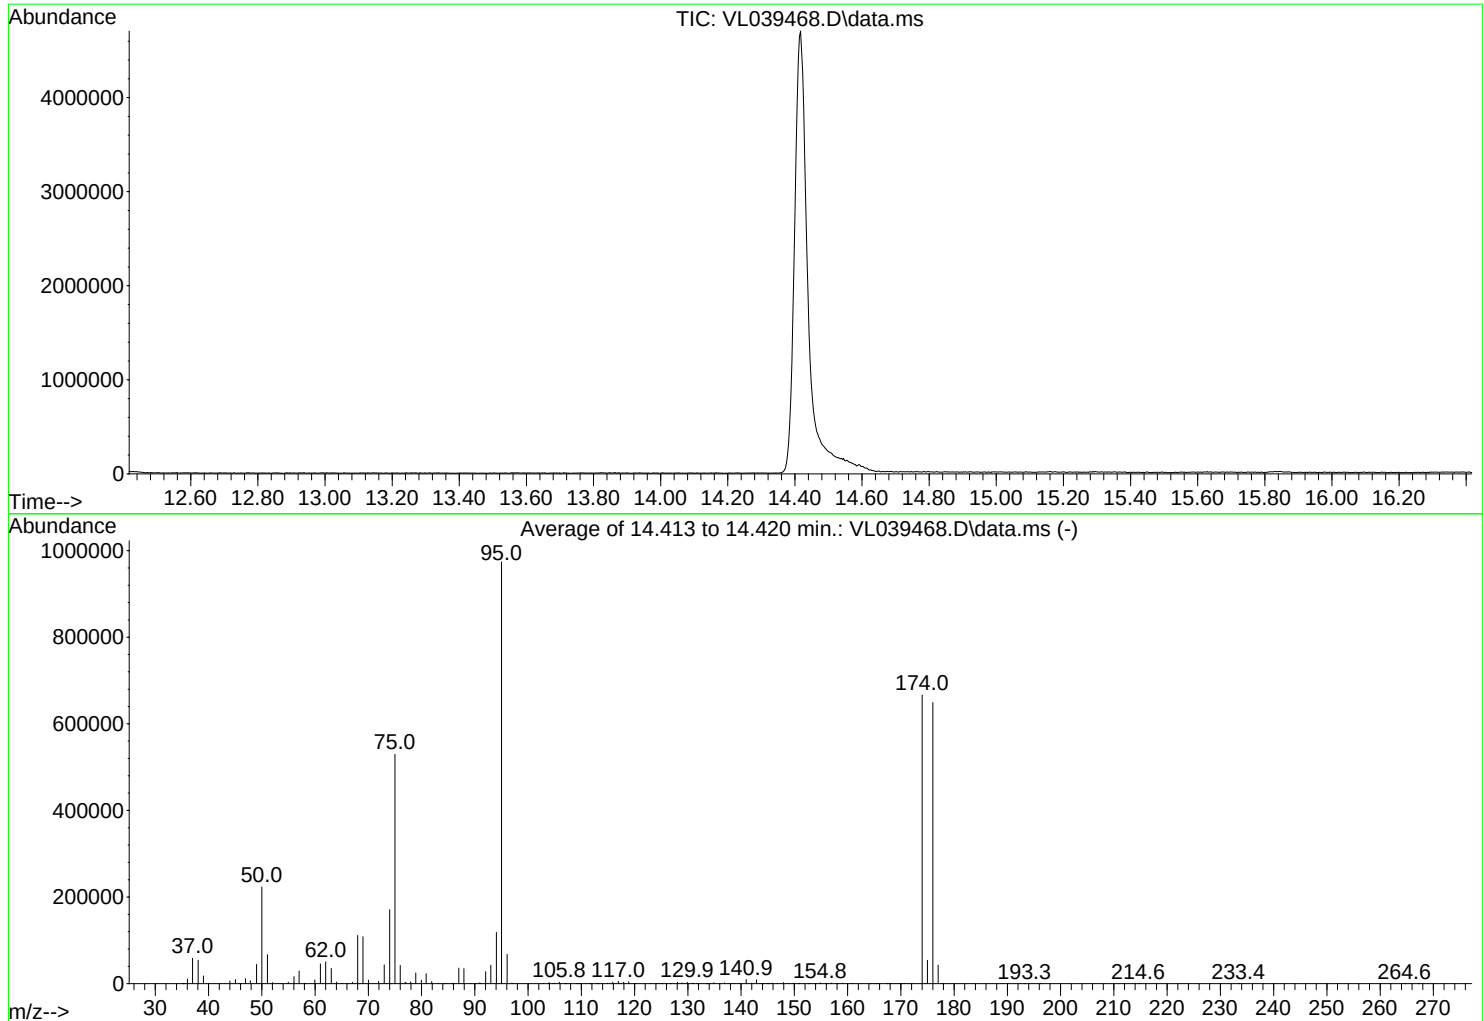

AutoFind: Scans 3616, 3617, 3618; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.9	223168	PASS
75	95	30	66	54.4	529984	PASS
95	95	100	100	100.0	974080	PASS
96	95	5	9	7.0	67749	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.5	666773	PASS
175	174	4	9	8.1	53904	PASS
176	174	93	101	97.4	649131	PASS
177	176	5	9	6.6	42881	PASS

Average of 14.413 to 14.420 min.: VL039468.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.10	61	45.05	9692	54.95	3544	64.90	340
35.30	201	45.90	289	56.05	16344	65.15	33
36.05	10693	46.15	754	57.00	29171	66.00	9
37.00	58971	46.95	11418	58.00	825	67.05	306
38.05	54075	47.85	6573	58.20	586	68.00	111312
39.05	17796	49.00	44459	59.15	301	69.00	108256
40.05	634	50.00	223168	59.95	8555	70.05	8166
41.10	444	51.05	66998	61.00	45499	71.05	250
42.20	387	52.05	2635	62.00	50216	71.95	5251
43.05	409	53.10	375	63.05	35176	73.00	43319
44.00	5786	53.70	265	64.05	3801	74.00	170624

Average of 14.413 to 14.420 min.: VL039468.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.00	529984	84.90	284	94.05	118101	106.90	705
76.00	42333	85.60	173	95.00	974080	107.10	212
76.90	2089	86.05	1131	96.05	67749	109.20	155
77.05	3258	87.00	36011	96.95	1248	109.70	133
77.95	4024	87.95	34899	97.15	600	110.10	382
78.90	24813	89.20	249	102.90	795	110.85	576
79.95	8071	90.00	133	103.80	1022	111.60	171
80.85	22849	90.85	1792	103.95	2068	111.85	523
81.90	4908	91.10	1168	104.60	416	112.80	617
83.10	909	92.05	27651	104.95	1186	113.10	78
84.20	77	93.00	42637	105.85	3243	114.90	1082

Average of 14.413 to 14.420 min.: VL039468.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
115.90	3353	126.75	215	136.90	1759	145.20	90
116.95	5066	128.05	2956	137.65	277	145.85	1595
117.95	3472	128.90	1780	138.30	230	146.85	480
118.90	4319	129.90	3453	138.75	383	147.95	2482
119.90	82	130.90	1208	139.60	691	148.80	304
120.15	240	131.10	587	140.95	9562	149.00	243
122.90	586	131.65	248	142.00	1232	149.80	1037
124.05	731	133.50	111	142.90	8879	150.80	53
124.75	402	133.95	204	143.75	306	151.85	563
125.10	169	134.90	2085	144.20	214	152.60	122
125.95	492	135.90	334	144.95	779	153.05	695

Average of 14.413 to 14.420 min.: VL039468.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
153.80	123	164.90	138	171.20	689	214.60	97
154.05	744	165.40	68	171.70	659	233.40	80
154.85	1887	165.90	163	172.10	628	264.60	116
155.80	280	167.40	55	174.00	666773	267.20	67
156.00	173	167.80	141	175.00	53904		
156.90	1605	168.00	115	176.00	649131		
158.00	96	168.90	305	177.00	42881		
159.05	1091	169.50	449	177.85	908		
160.75	569	170.00	60	178.10	303		
161.00	242	170.20	274	193.25	162		
164.20	109	170.65	634	196.30	90		