
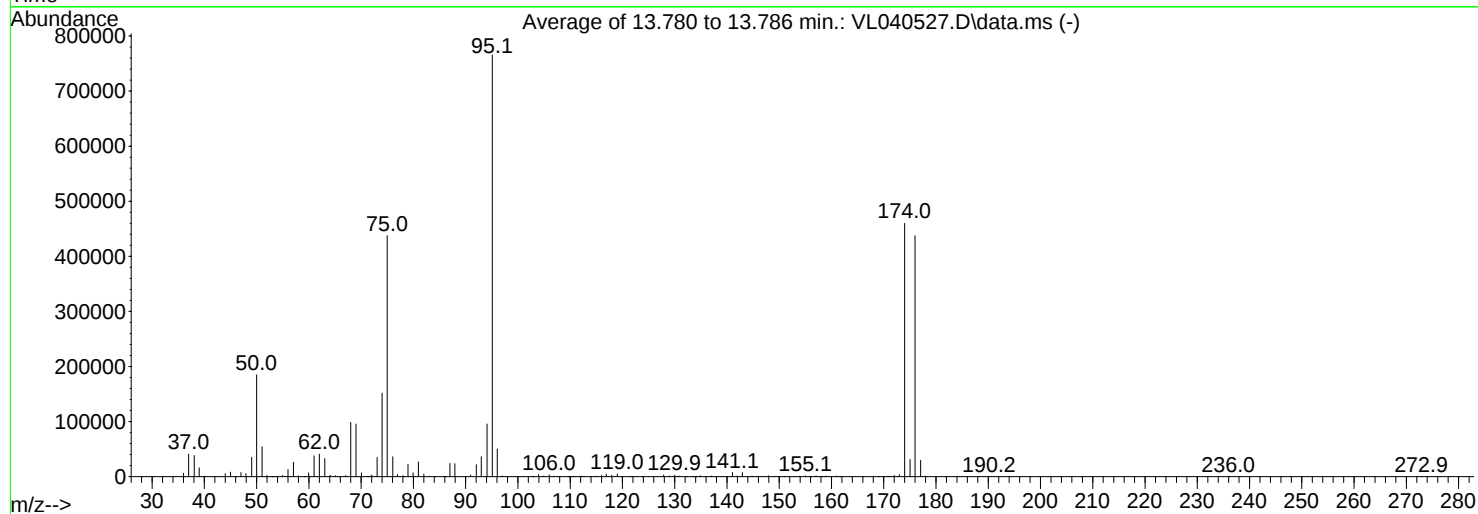


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL071423\
 Data File : VL040527.D
 Acq On : 14 Jul 2023 14:23
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL071023AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Mon Jul 10 16:32:00 2023

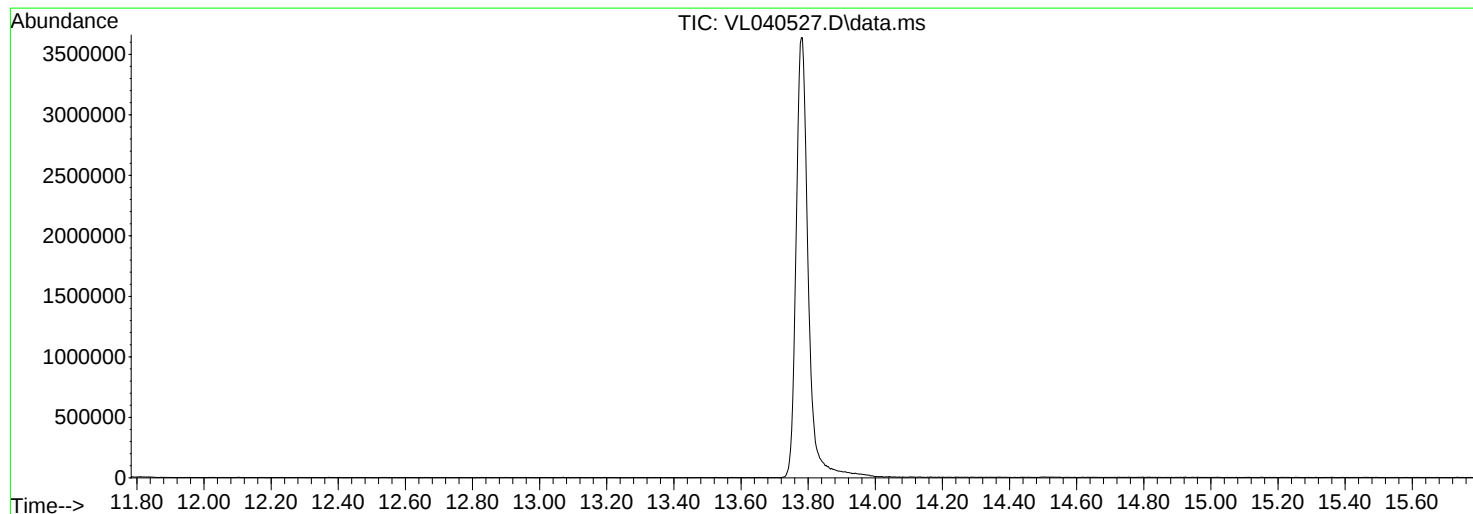

AutoFind: Scans 3476, 3477, 3478; Background Corrected with Scan 3453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.1	184747	PASS
75	95	30	66	57.1	437611	PASS
95	95	100	100	100.0	765845	PASS
96	95	5	9	6.6	50392	PASS
173	174	0.00	2	0.8	3701	PASS
174	95	50	120	60.1	460011	PASS
175	174	4	9	6.8	31480	PASS
176	174	93	101	95.1	437504	PASS
177	176	5	9	6.8	29640	PASS

Average of 13.780 to 13.786 min.: VL040527.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	6191	47.95	5430	58.00	1390	69.00	9557
37.00	40923	49.05	35197	59.10	112	70.05	702
38.05	38371	50.00	184747	59.95	6926	71.30	15
39.00	15977	51.05	54213	61.00	37944	71.90	184
40.10	891	51.95	2055	62.00	40928	72.05	2606
43.10	285	52.90	65	63.05	32744	73.05	34928
44.00	5477	53.20	64	64.05	2644	74.00	151659
45.00	8134	53.80	59	65.05	1833	75.00	437611
45.85	280	55.00	1975	66.05	225	76.05	36035
46.15	443	56.00	13099	67.05	1935	76.95	3806
47.00	7513	57.05	26123	68.00	98437	78.05	1774

Average of 13.780 to 13.786 min.: VL040527.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	22368	92.05	21925	106.85	894	116.00	2479
79.95	7022	93.00	36448	107.80	95	116.90	4581
80.95	26661	94.10	95464	109.60	54	117.95	2656
82.00	4678	95.10	765845	109.85	245	119.00	4873
83.05	1030	96.05	50392	110.10	131	119.80	55
84.10	59	97.00	1264	110.70	265	120.10	173
85.75	655	102.70	301	110.95	435	121.70	55
86.00	116	102.90	142	112.05	773	122.85	217
87.00	24112	103.95	3683	112.50	221	123.80	82
87.95	23600	104.95	1058	112.75	349	124.10	365
90.95	2828	106.00	3345	114.90	950	124.95	214

Average of 13.780 to 13.786 min.: VL040527.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.95	306	134.90	1648	144.70	317	153.05	329
126.65	228	135.90	160	144.90	568	153.90	615
127.90	3050	137.00	1147	145.70	191	155.05	1441
128.95	1293	138.90	240	146.05	851	155.80	120
129.95	2633	139.70	247	147.10	287	156.10	154
130.80	231	140.00	143	147.90	1760	157.05	1371
130.95	845	141.05	7697	149.05	453	157.75	223
132.30	152	141.95	1142	149.90	781	158.10	71
133.30	88	142.95	7603	150.90	51	158.90	847
133.70	66	143.85	316	151.85	368	160.95	1154
134.10	109	144.10	274	152.80	228	161.60	56

Average of 13.780 to 13.786 min.: VL040527.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
165.90	61	175.05	31480				
168.90	63	176.00	437504				
169.70	161	177.05	29640				
170.05	185	178.05	996				
170.75	281	190.20	237				
171.10	174	236.00	60				
171.40	356	272.90	125				
172.00	2066						
172.60	473						
173.00	3701						
174.00	460011						

Instrument :

MSVOA_L

ClientSampleId :

BFB