

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL071818\
 Data File : VL032278.D
 Acq On : 19 Jul 2018 2:27
 Operator : SY/AP
 Sample : J3454-04DL 10X
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :

Quant Time: Jul 19 04:12:22 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL071818AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Jul 18 14:38:53 2018
 QLast Update : Wed Jul 18 14:38:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.84	49	1667821	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.37	114	3425781	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.33	117	4035754	10.00	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	14.67	95	3160299	9.66	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	96.60%


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) Dichlorodifluoromethane	3.13	85	21583	0.076	ppbv	92
3) Chlorodifluoromethane	3.04	51	112966	0.604	ppbv #	69
13) Ethanol	3.72	45	157412	6.735	ppbv	100
15) Acetone	3.97	43	185157	1.061	ppbv	96
19) Isopropyl Alcohol	4.11	45	33650	0.285	ppbv #	88
20) Methylene Chloride	4.47	84	29111	0.433	ppbv #	96
25) Ethyl Acetate	5.86	43	176522	0.464	ppbv #	79
26) Hexane	5.86	57	233689	1.338	ppbv #	43
34) 2-Butanone	5.42	43	17659	0.075	ppbv	91
39) 1,2-Dichloropropane	7.37	63	971312	7.276	ppbv #	26
53) Toluene	10.03	91	20903	0.051	ppbv	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL071818\
Data File : VL032278.D
Acq On : 19 Jul 2018 2:27
Operator : SY/AP
Sample : J3454-04DL 10X
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :

Quant Time: Jul 19 04:12:22 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL071818AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Jul 18 14:38:53 2018
QLast Update : Wed Jul 18 14:38:53 2018
Response via : Initial Calibration

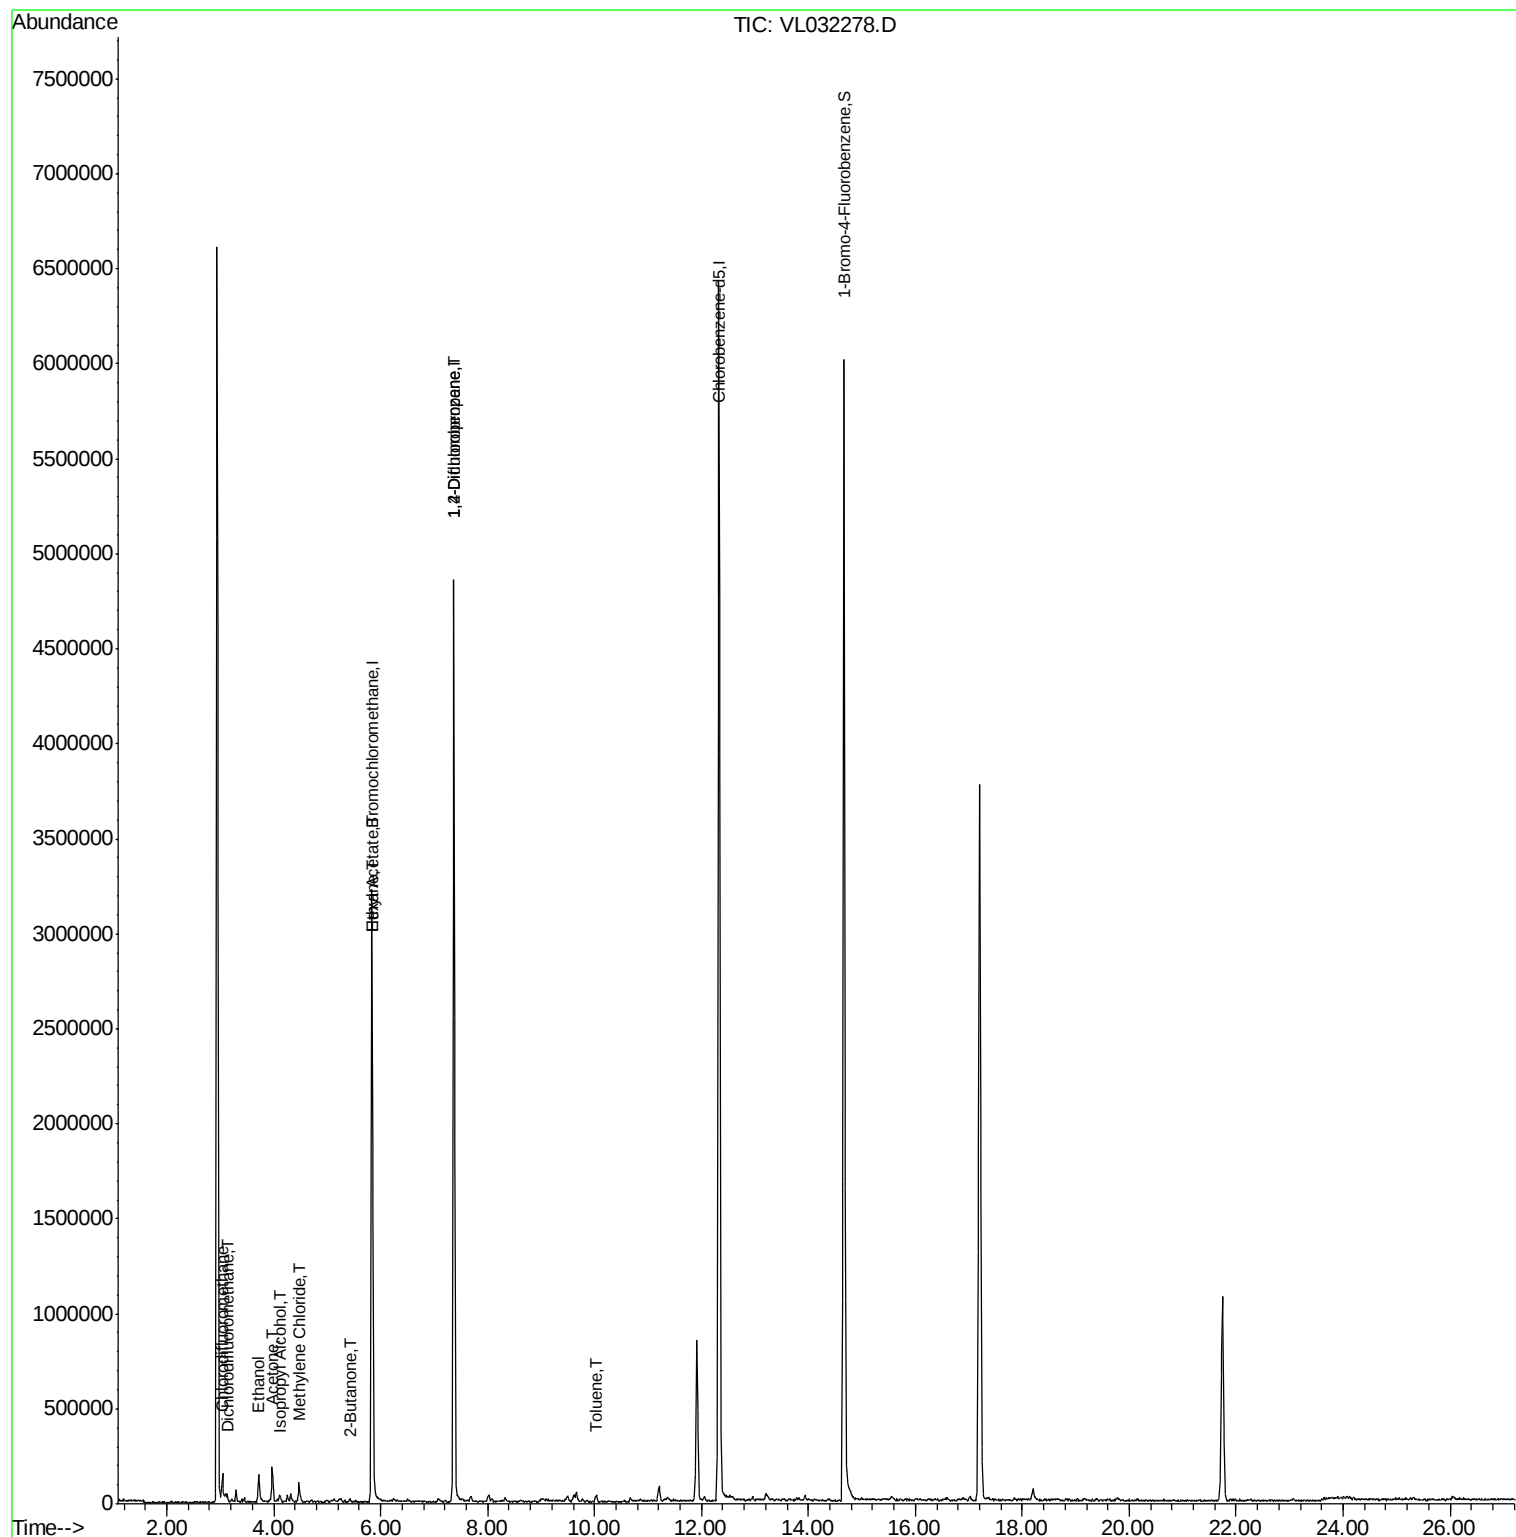

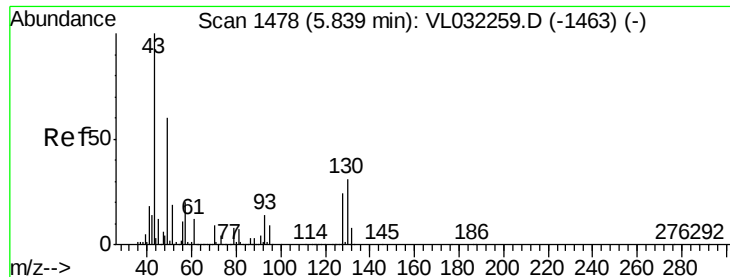

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.84 min Scan# 1477

Delta R.T. -0.00 min

Lab File: VL032278.D

Acq: 19 Jul 2018 2:27

Instrument :

MSVOA_L

ClientSampleId :


Tot Ion: 49 Resp: 1667821

Ion Ratio Lower Upper

49 100

128 40.1 20.1 60.2




130 51.4 25.9 77.6

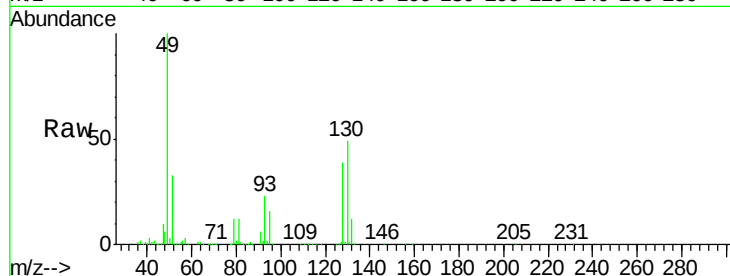

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

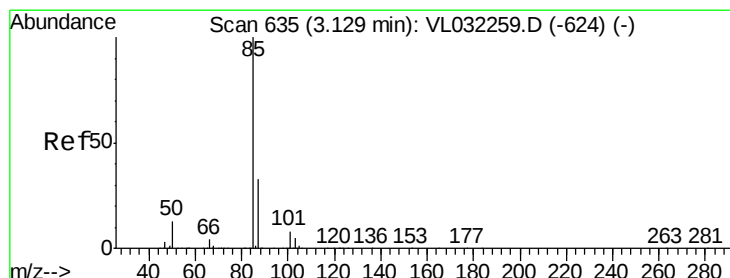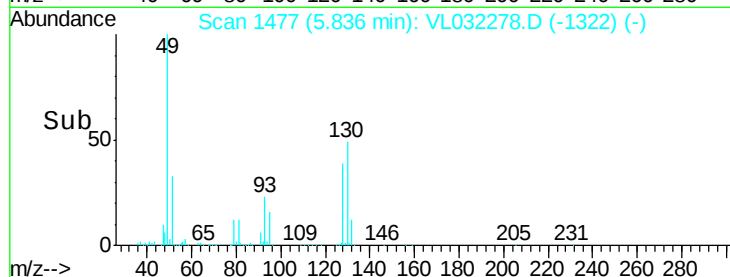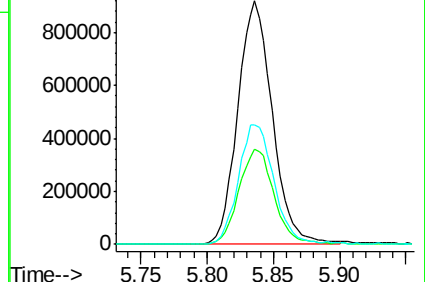

#2

Dichlorodifluoromethane

Concen: 0.076 ppbv

RT: 3.13 min Scan# 634

Delta R.T. -0.00 min

Lab File: VL032278.D


Acq: 19 Jul 2018 2:27

Tgt Ion: 85 Resp: 21583

Ion Ratio Lower Upper



85 100


87 37.2 26.2 39.2

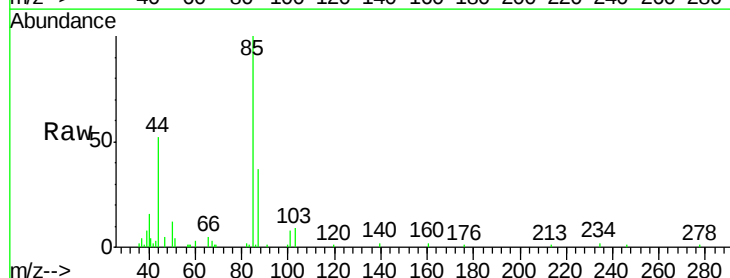

Abundance Ion 85.00 (84.70 to 85.70): VL0

Ion 87.00 (86.70 to 87.70): VL0



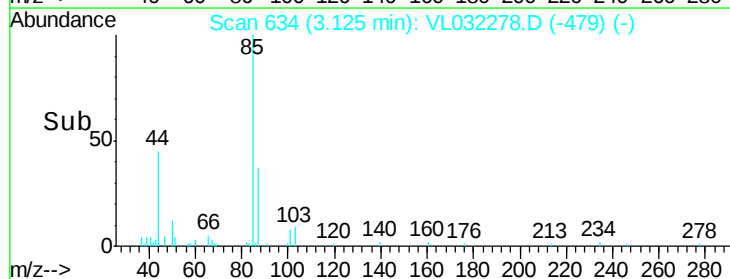
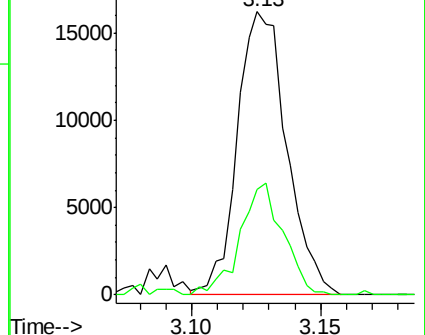


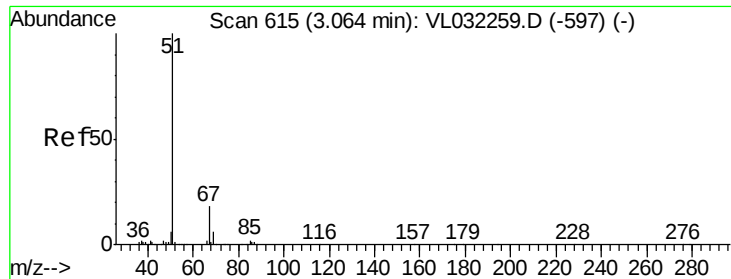

#3
 Chlorodifluoromethane
 Concen: 0.604 ppbv
 RT: 3.04 min Scan# 608
 Delta R.T. -0.02 min
 Lab File: VL032278.D
 Acq: 19 Jul 2018 2:27




Instrument :
 MSVOA_L
 ClientSampleId :


Tot Ion: 51 Resp: 112966
 Ion Ratio Lower Upper
 51 100
 67 4.2 14.2 21.4#

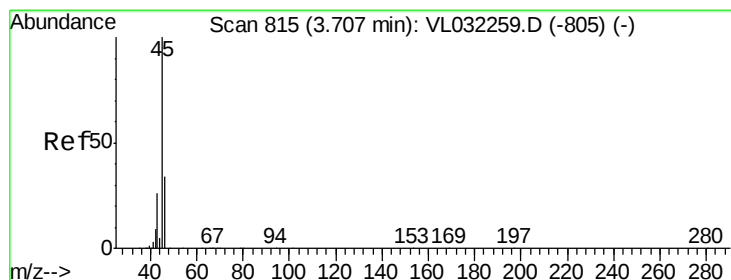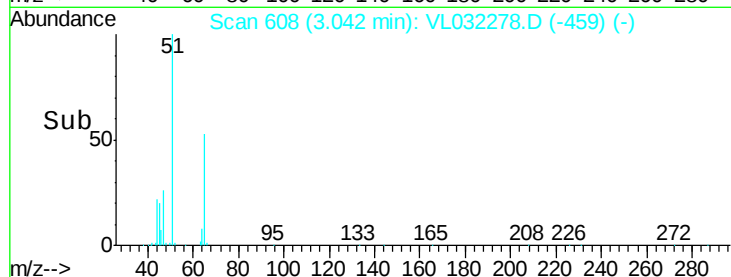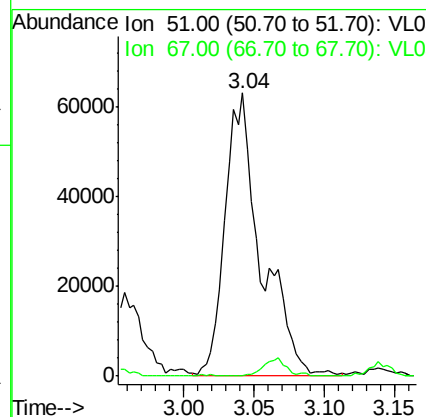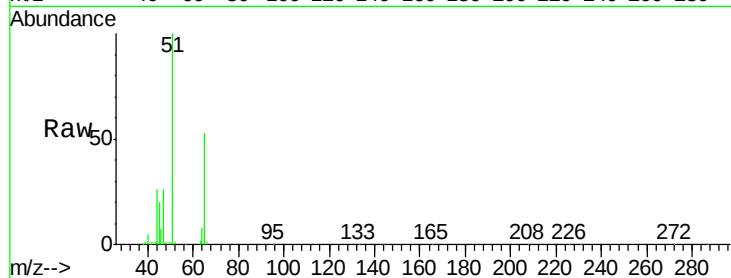

#13
 Ethanol
 Concen: 6.735 ppbv
 RT: 3.72 min Scan# 818
 Delta R.T. 0.01 min
 Lab File: VL032278.D
 Acq: 19 Jul 2018 2:27

Tgt Ion: 45 Resp: 157412
 Ion Ratio Lower Upper
 45 100
 46 38.0 15.2 60.8

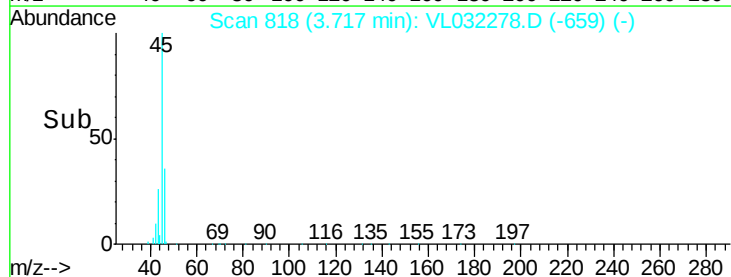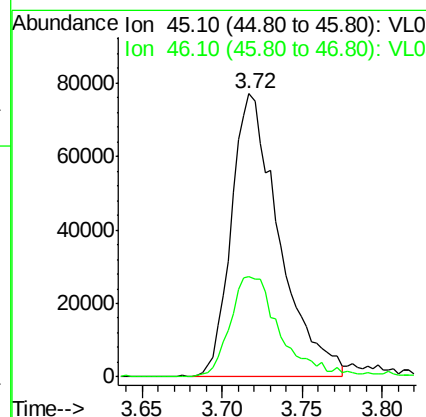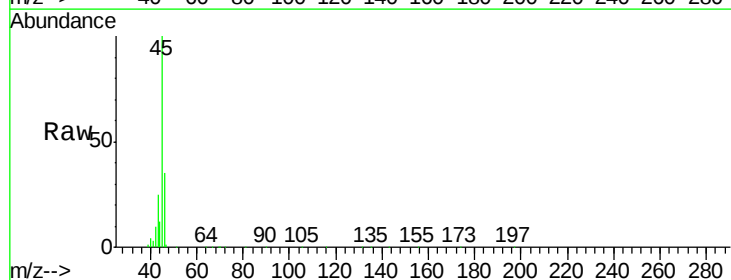

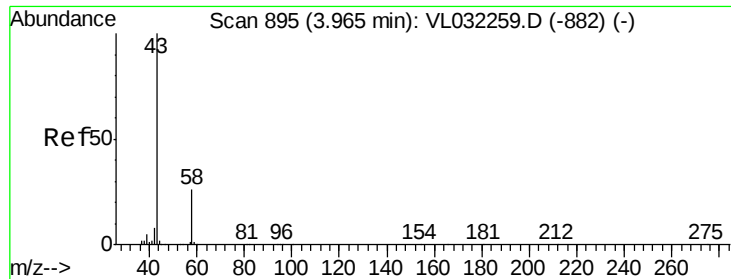

#15

Acetone

Concen: 1.061 ppbv

RT: 3.97 min Scan# 898

Delta R.T. 0.01 min

Lab File: VL032278.D

Acq: 19 Jul 2018 2:27

Instrument :

MSVOA_L


ClientSampleId :

Tot Ion: 43 Resp: 185157

Ion Ratio Lower Upper




43 100

58 29.4 21.8 32.6

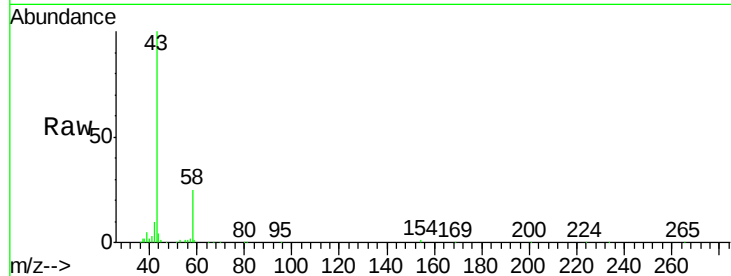

Abundance Ion 43.10 (42.80 to 43.80): VL0

Ion 58.10 (57.80 to 58.80): VL0

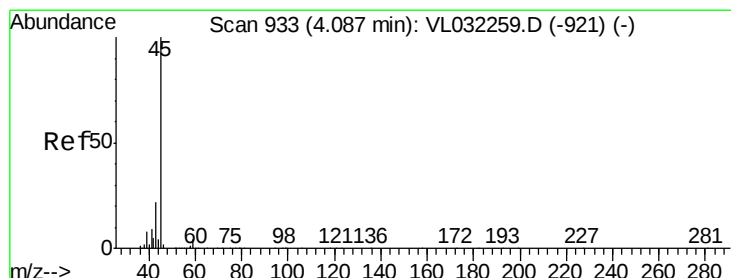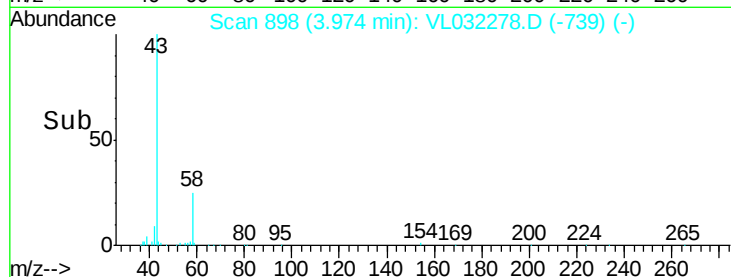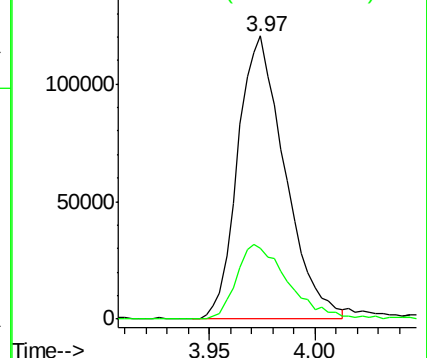

#19

Isopropyl Alcohol

Concen: 0.285 ppbv

RT: 4.11 min Scan# 940

Delta R.T. 0.02 min

Lab File: VL032278.D


Acq: 19 Jul 2018 2:27

Tgt Ion: 45 Resp: 33650

Ion Ratio Lower Upper



45 100


58 6.3 1.5 2.3#

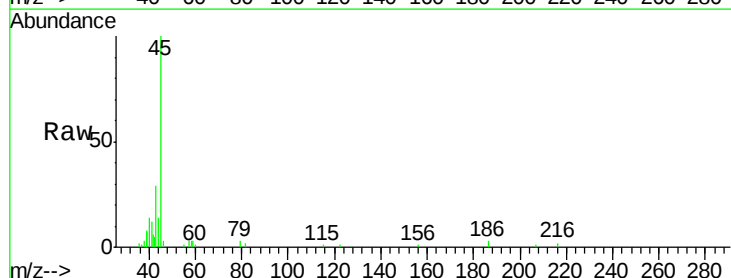

Abundance Ion 45.10 (44.80 to 45.80): VL0

Ion 58.10 (57.80 to 58.80): VL0



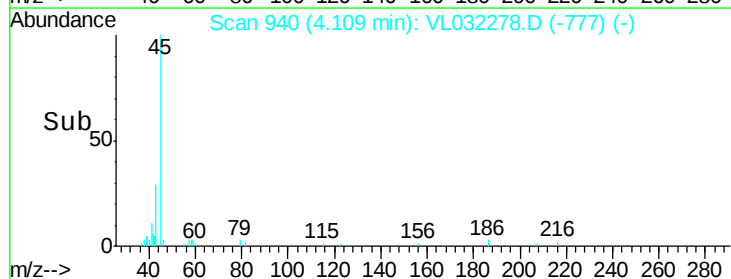
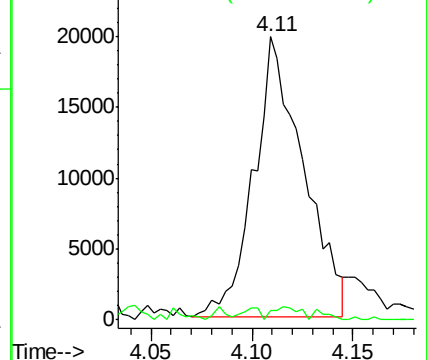


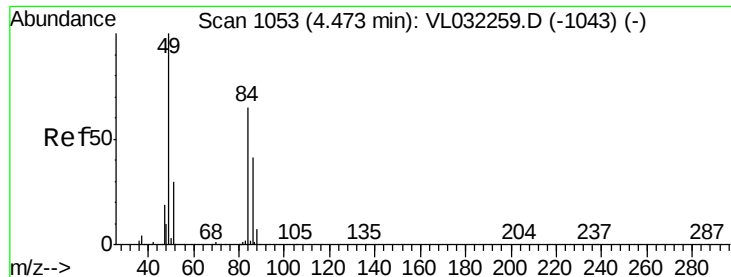

#20
Methylene Chloride
Concen: 0.433 ppbv
RT: 4.47 min Scan# 1053
Delta R.T. 0.00 min
Lab File: VL032278.D
Acq: 19 Jul 2018 2:27




Instrument :
MSVOA_L
ClientSampleId :


Tot Ion	Ion	Ratio	Lower	Upper
84	100			
49	155.3	122.4	183.6	
51	36.7	36.8	55.2#	
86	64.6	50.7	76.1	

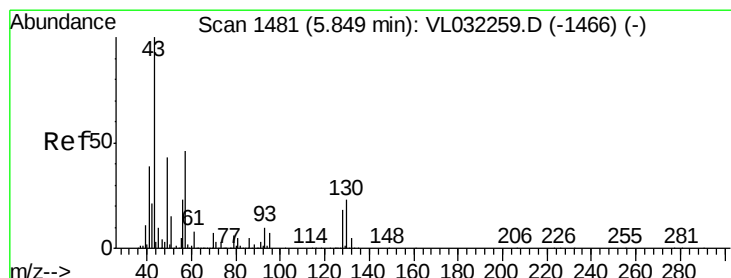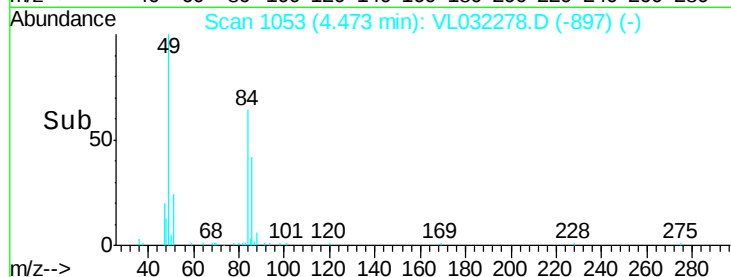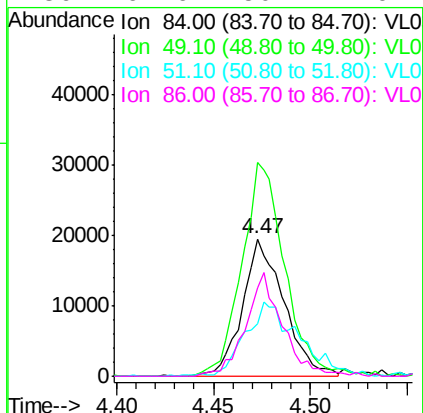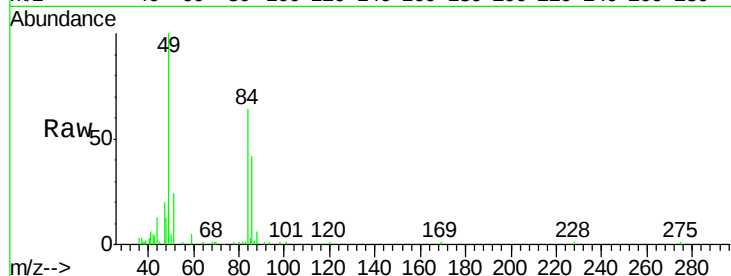

#25
Ethyl Acetate
Concen: 0.464 ppbv
RT: 5.86 min Scan# 1483
Delta R.T. 0.01 min
Lab File: VL032278.D
Acq: 19 Jul 2018 2:27

Tgt Ion	Ion	Ratio	Lower	Upper
43	100			
45	1.6	7.9	11.9#	
61	0.9	7.6	11.4#	
70	2.3	5.8	8.8#	

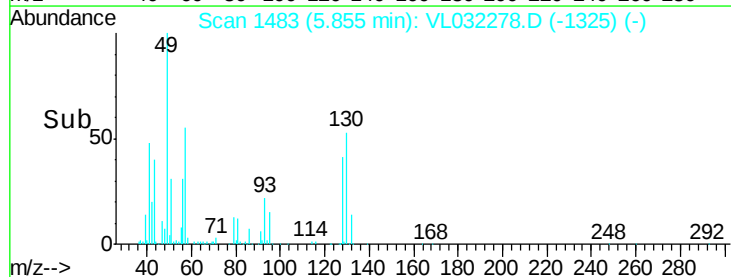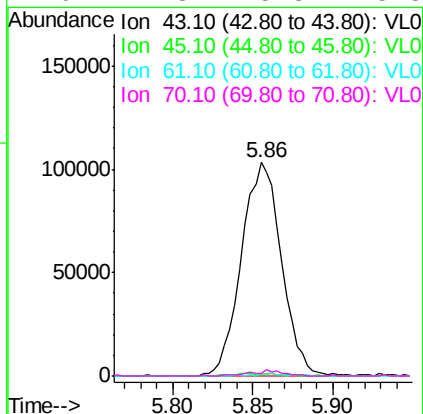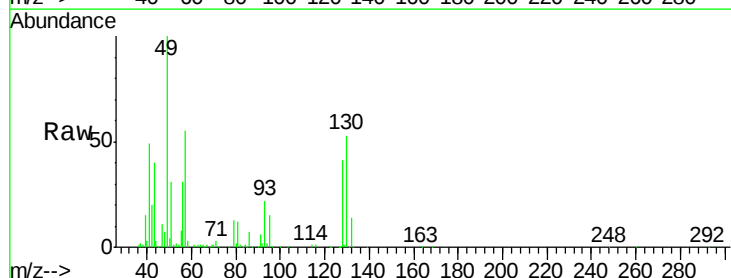


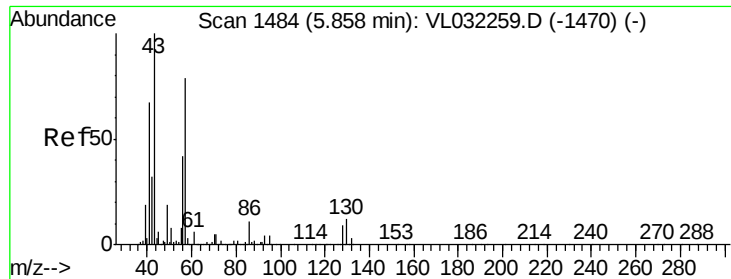




#26
Hexane
Concen: 1.338 ppbv
RT: 5.86 min Scan# 1483
Delta R.T. -0.00 min
Lab File: VL032278.D
Acq: 19 Jul 2018 2:27

Instrument :
MSVOA_L
ClientSampled :

Tot Ion: 57 Resp: 233689
Ion Ratio Lower Upper
57 100
41 89.8 67.9 101.9
43 75.8 175.9 263.9#
56 56.1 41.9 62.9

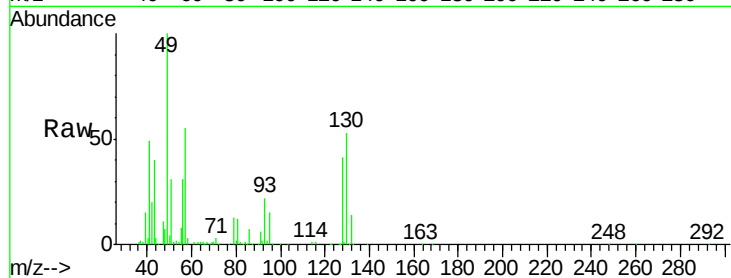


Abundance Ion 57.10 (56.80 to 57.80): VL0
Ion 41.10 (40.80 to 41.80): VL0
Ion 43.10 (42.80 to 43.80): VL0
Ion 56.10 (55.80 to 56.80): VL0

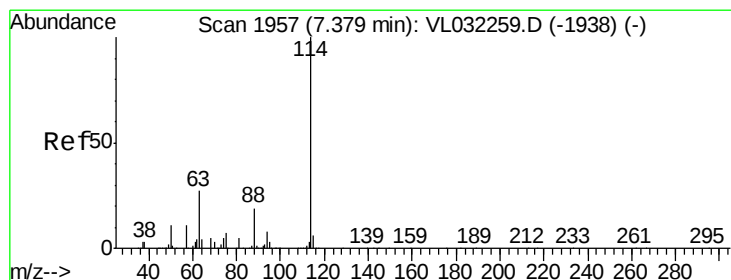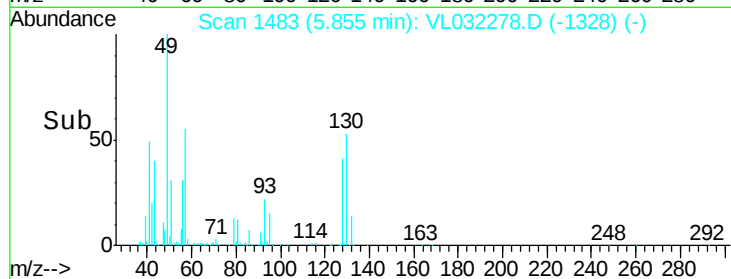
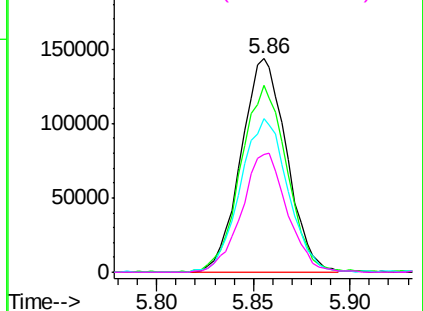



#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 7.37 min Scan# 1955
Delta R.T. -0.01 min
Lab File: VL032278.D
Acq: 19 Jul 2018 2:27

Tgt Ion: 114 Resp: 3425781
Ion Ratio Lower Upper
114 100
63 28.5 22.6 33.8
88 19.1 15.2 22.8

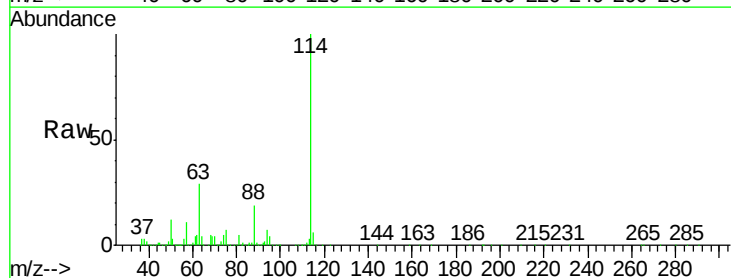

Abundance Ion 114.10 (113.80 to 114.80): V
Ion 63.10 (62.80 to 63.80): VL0
Ion 88.10 (87.80 to 88.80): VL0



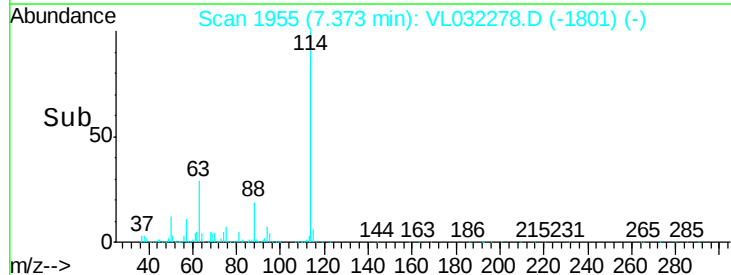
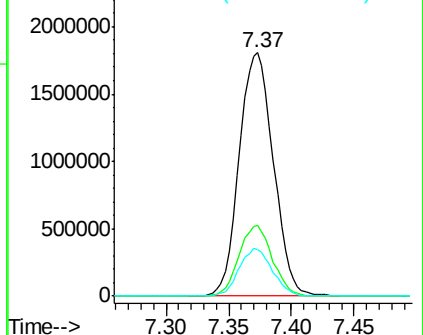


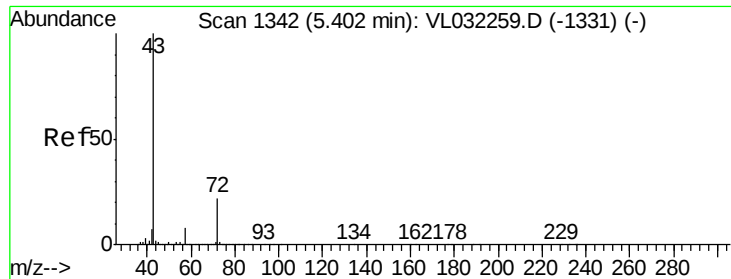

#34
 2-Butanone
 Concen: 0.075 ppbv
 RT: 5.42 min Scan# 1348
 Delta R.T. 0.02 min
 Lab File: VL032278.D
 Acq: 19 Jul 2018 2:27




Instrument :
 MSVOA_L
 ClientSampleId :


Tot Ion: 43 Resp: 17659
 Ion Ratio Lower Upper
 43 100
 72 26.5 17.7 26.5

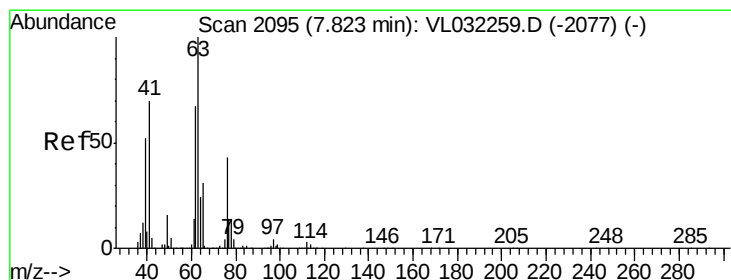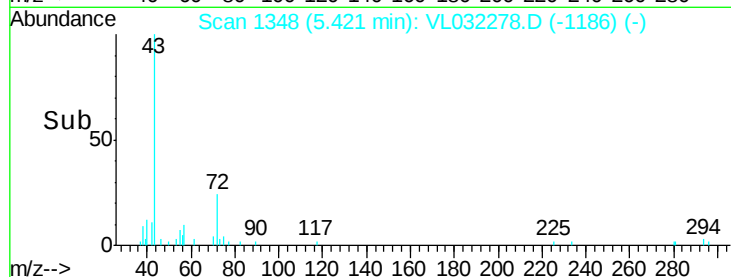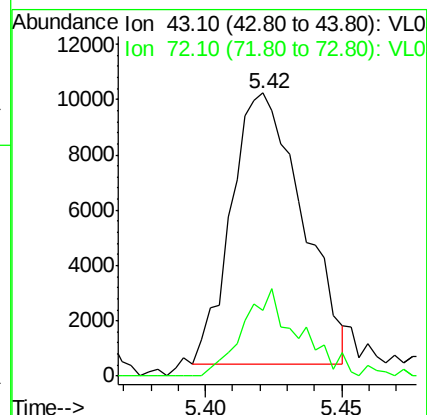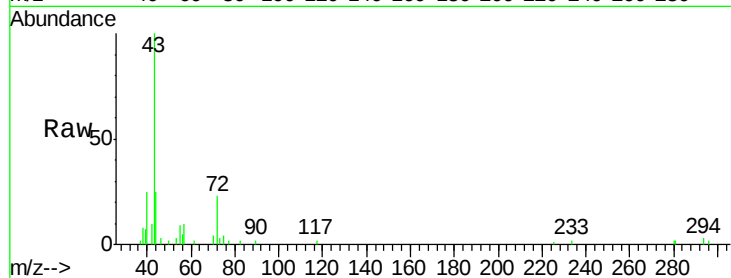

#39
 1,2-Dichloropropane
 Concen: 7.276 ppbv
 RT: 7.37 min Scan# 1955
 Delta R.T. -0.45 min
 Lab File: VL032278.D
 Acq: 19 Jul 2018 2:27

Tgt Ion: 63 Resp: 971312
 Ion Ratio Lower Upper
 63 100
 41 0.1 55.8 83.6#
 62 16.2 53.8 80.8#

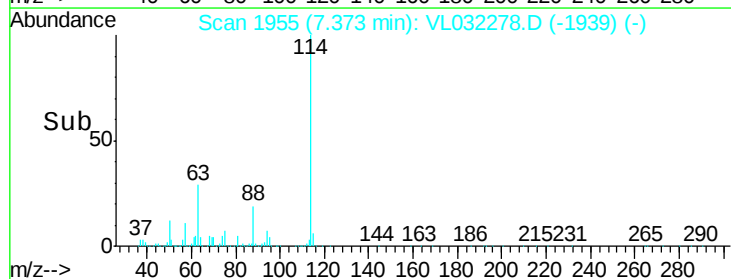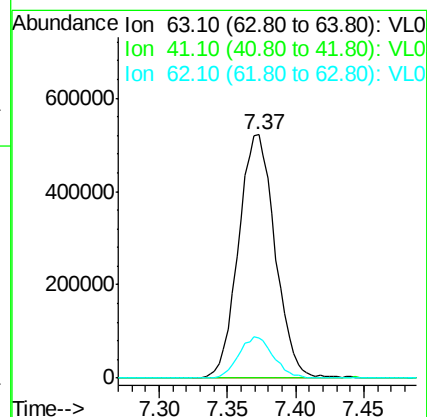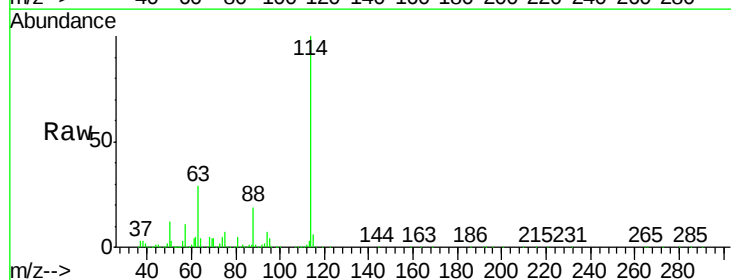

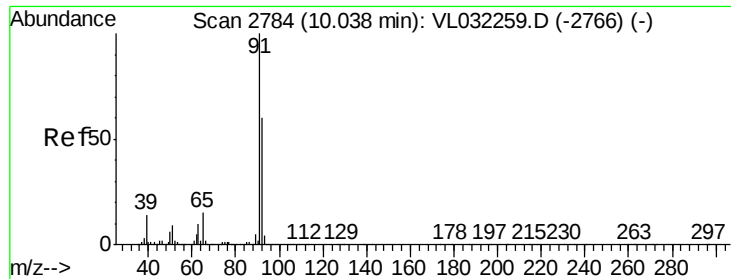

#53

Toluene

Concen: 0.051 ppbv

RT: 10.03 min Scan# 2782

Delta R.T. -0.01 min

Lab File: VL032278.D

Acq: 19 Jul 2018 2:27

Instrument :

MSVOA_L





ClientSampled :

Tot Ion: 91 Resp: 20903

Ion Ratio Lower Upper

91 100

92 68.2 48.6 72.8

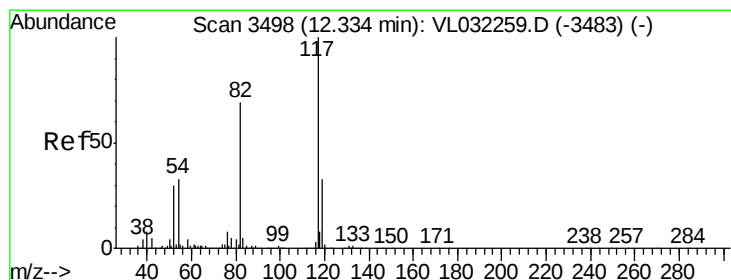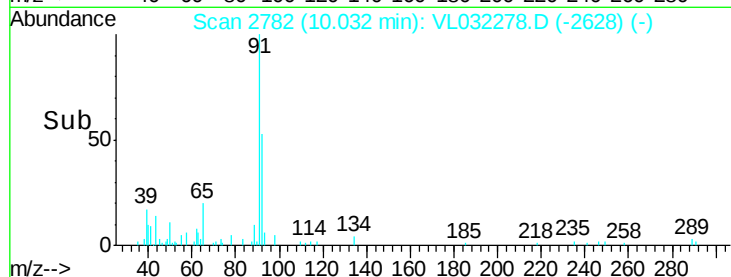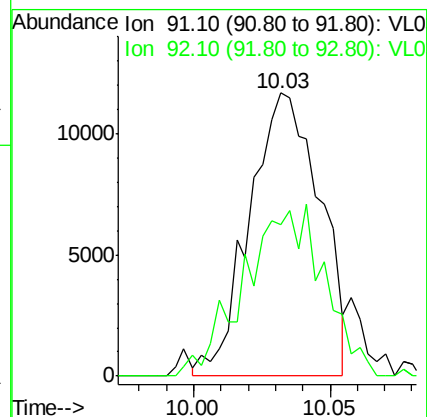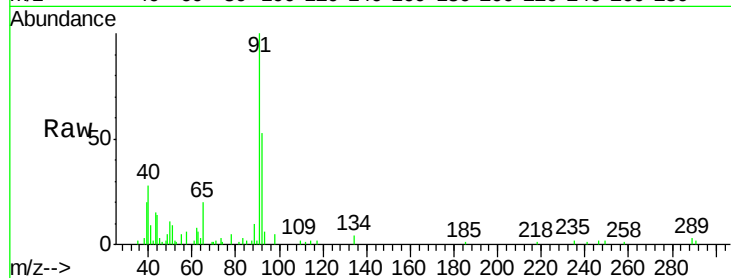

#55

Chlorobenzene-d5

Concen: 10.000 ppbv

RT: 12.33 min Scan# 3496

Delta R.T. -0.01 min

Lab File: VL032278.D

Acq: 19 Jul 2018 2:27




Tgt Ion: 117 Resp: 4035754


Ion Ratio Lower Upper

117 100

82 69.8 53.9 80.9

119 32.7 25.5 38.3

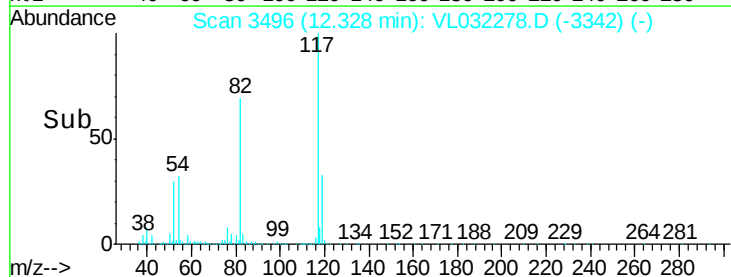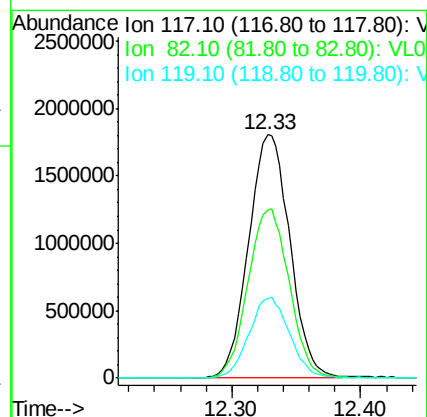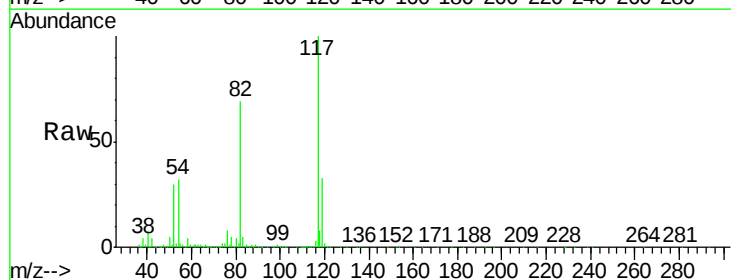

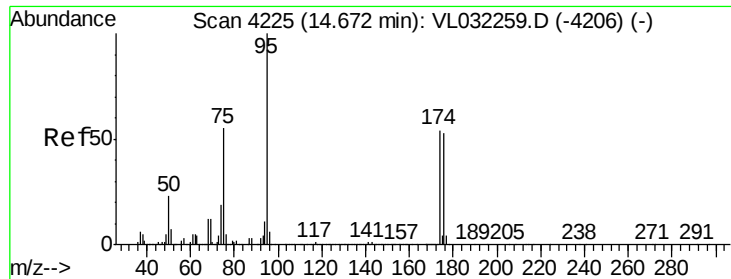

#68
 1-Bromo-4-Fluorobenzene
 Concen: 9.658 ppbv
 RT: 14.67 min Scan# 4223
 Delta R.T. -0.01 min
 Lab File: VL032278.D
 Acq: 19 Jul 2018 2:27

Instrument :
 MSVOA_L
 ClientSampleId :

Tot Ion: 95 Resp: 3160299

Ion	Ratio	Lower	Upper
95	100		
174	56.4	44.3	66.5
175	3.9	3.3	4.9

