


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL071818\
Data File : VL032258.D
Acq On : 18 Jul 2018 8:40
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL071818AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Jul 18 14:38:53 2018
Last Update : Fri Jul 20 14:50:24 2018

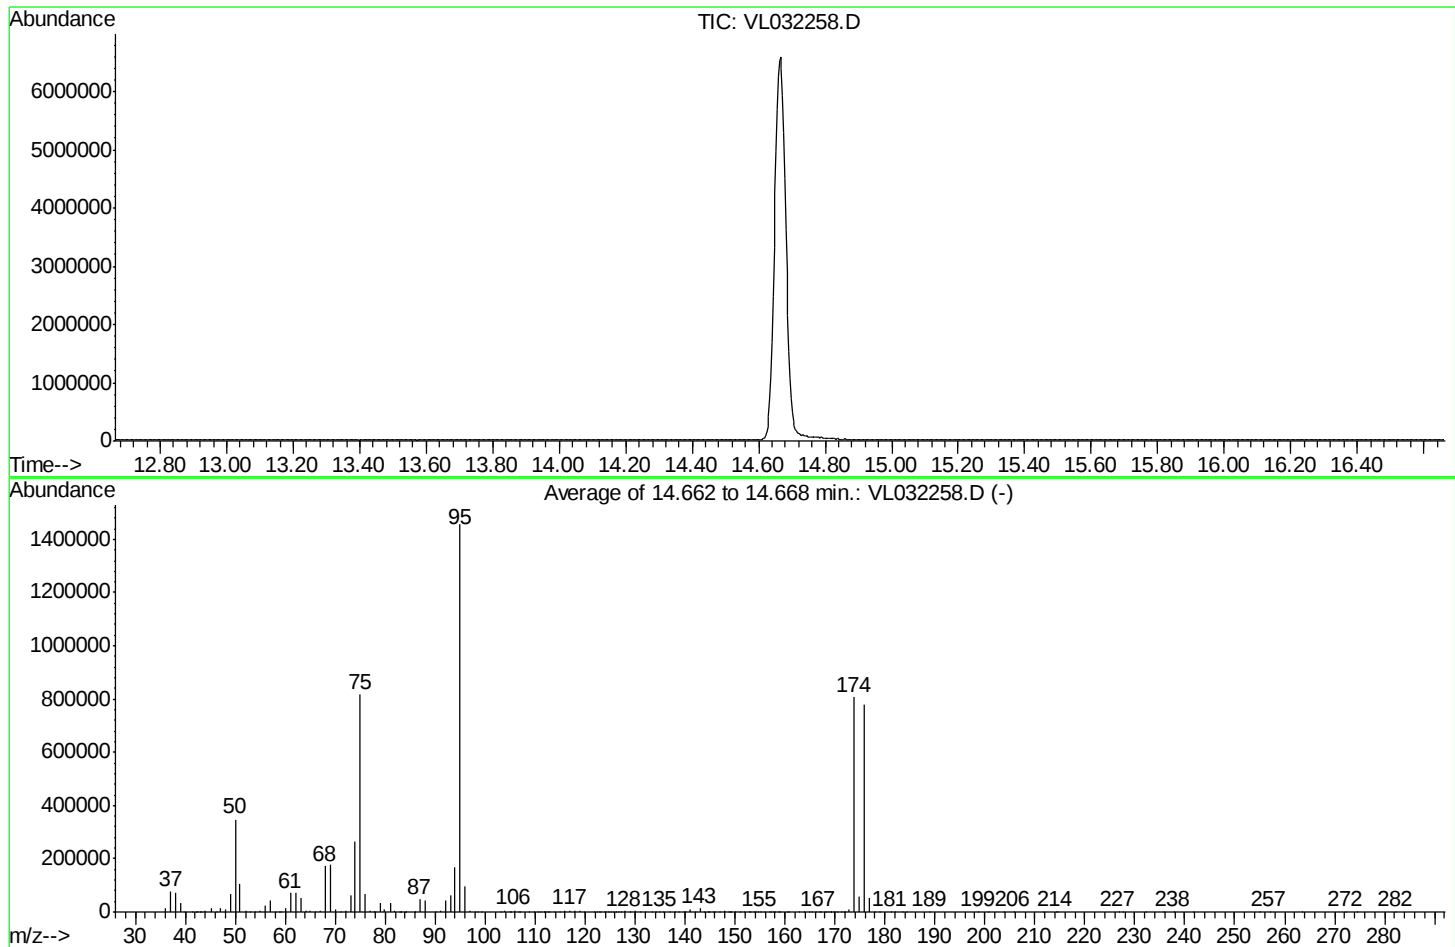

AutoFind: Scans 4222, 4223, 4224; Background Corrected with Scan 4197

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	347489	PASS
75	95	30	66	56.1	817408	PASS
95	95	100	100	100.0	1456298	PASS
96	95	5	9	6.7	98218	PASS
173	174	0.00	2	1.0	8069	PASS
174	95	50	120	55.4	807338	PASS
175	174	4	9	7.2	58152	PASS
176	174	93	101	96.8	781184	PASS
177	176	5	9	6.5	50922	PASS