


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL071918\
Data File : VL032289.D
Acq On : 19 Jul 2018 13:47
Operator : SY/AP
Sample : BFB
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL071818AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Jul 18 14:38:53 2018
Last Update : Wed Jul 18 14:38:53 2018

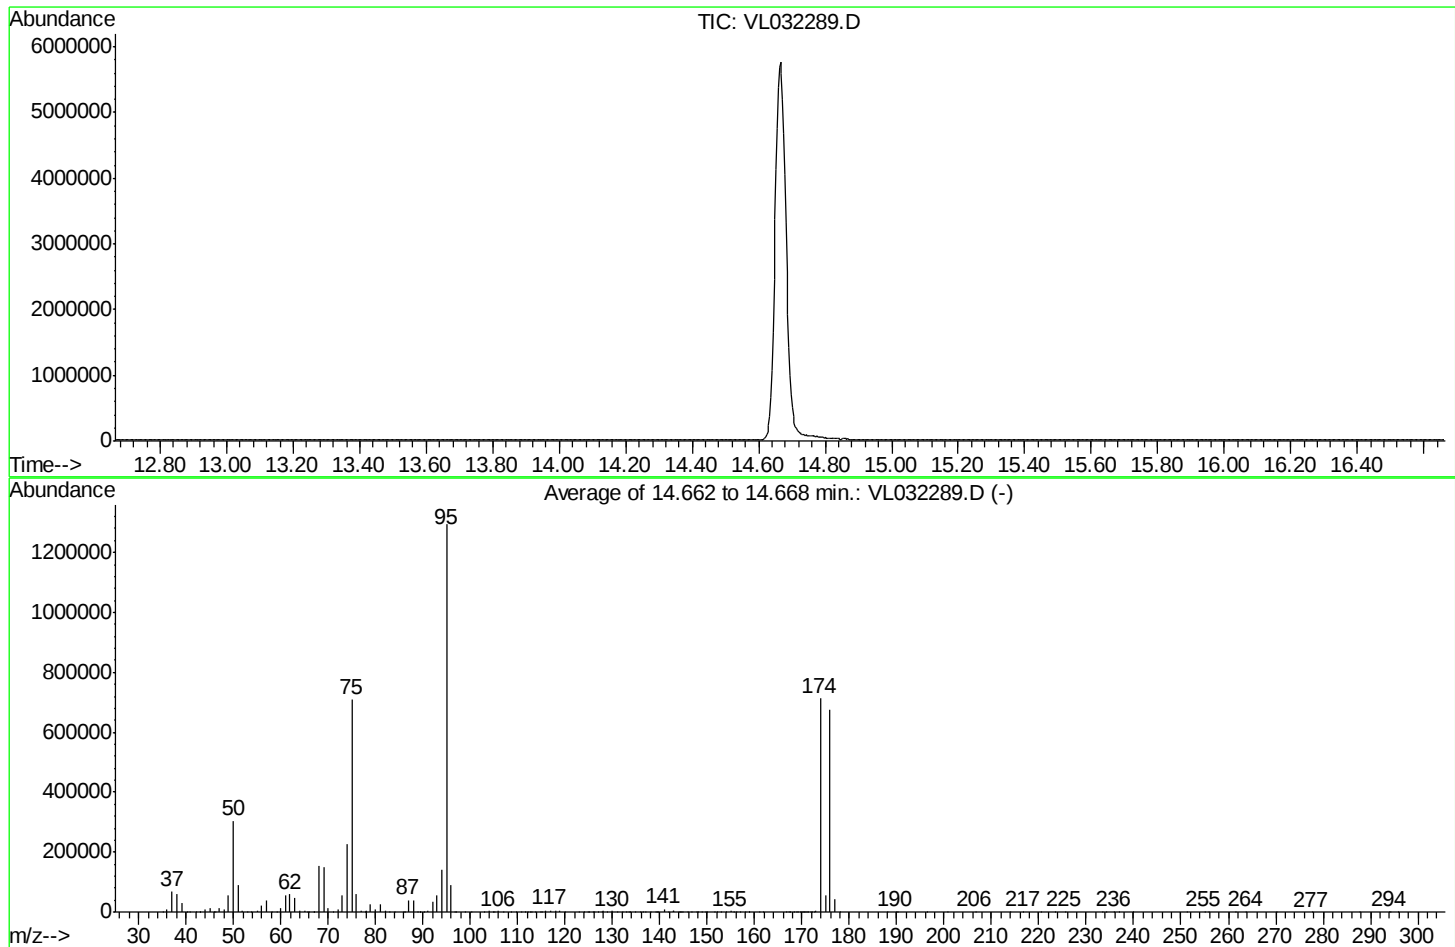

AutoFind: Scans 4222, 4223, 4224; Background Corrected with Scan 4194

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.6	304981	PASS
75	95	30	66	54.8	708800	PASS
95	95	100	100	100.0	1294165	PASS
96	95	5	9	6.8	88416	PASS
173	174	0.00	2	0.6	4567	PASS
174	95	50	120	55.0	711765	PASS
175	174	4	9	7.8	55264	PASS
176	174	93	101	95.0	675882	PASS
177	176	5	9	6.6	44461	PASS