


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL071922\
Data File : VL039479.D
Acq On : 19 Jul 2022 11:54
Operator : SY/AP
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL062922AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jul 06 02:15:38 2022
Last Update : Wed Jul 06 02:15:38 2022

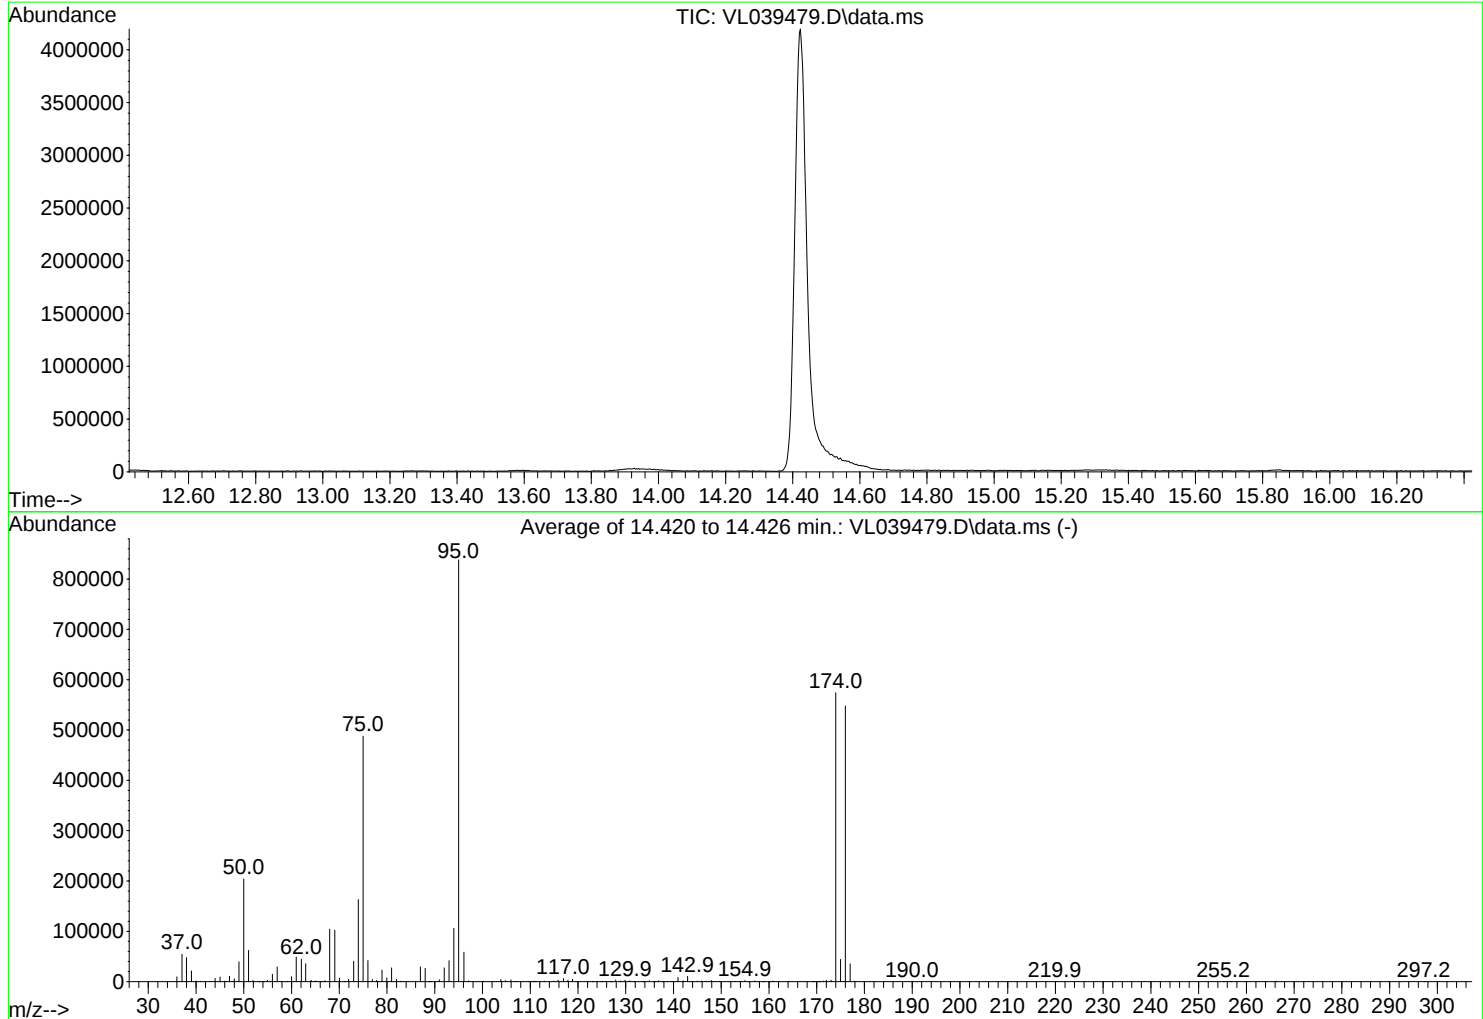

AutoFind: Scans 3618, 3619, 3620; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.4	204203	PASS
75	95	30	66	58.2	487637	PASS
95	95	100	100	100.0	838208	PASS
96	95	5	9	7.0	58397	PASS
173	174	0.00	2	0.5	2946	PASS
174	95	50	120	68.5	574144	PASS
175	174	4	9	7.7	44213	PASS
176	174	93	101	95.4	547989	PASS
177	176	5	9	6.5	35424	PASS

Average of 14.420 to 14.426 min.: VL039479.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	9524	47.00	10416	57.00	28968	65.80	401
37.05	54339	48.00	5790	57.95	1129	66.20	15
38.00	47701	49.00	39400	59.00	93	66.90	103
39.05	21309	50.00	204203	60.00	10007	67.05	161
40.05	1339	51.00	61882	61.00	49107	68.00	104168
40.95	592	51.90	2293	62.05	44579	69.05	102531
43.20	714	53.00	350	62.95	35616	70.05	7090
44.00	6472	53.20	60	63.90	1358	71.00	102
45.05	9377	54.00	58	64.15	2167	71.95	4437
45.95	875	54.95	2765	64.90	1014	73.00	40493
46.30	695	56.00	14496	65.15	1184	74.00	163093

Average of 14.420 to 14.426 min.: VL039479.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.00	487637	85.95	1082	97.10	1669	110.85	869
76.00	42069	87.00	29133	100.20	204	111.10	134
76.95	4191	88.00	26496	102.90	436	111.85	737
77.80	2306	88.80	113	103.85	4059	112.10	308
78.10	801	89.10	85	104.85	1772	112.95	973
78.95	23003	90.95	3896	105.95	3605	114.90	1080
79.95	7233	92.00	27501	106.80	407	115.85	2848
80.95	27443	93.00	41765	107.05	329	116.95	6063
81.95	4445	94.00	105912	109.65	360	117.90	2851
82.85	702	95.00	838208	110.20	459	118.85	4780
83.10	337	96.10	58397	110.50	187	119.75	133

Average of 14.420 to 14.426 min.: VL039479.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
122.00	53	128.95	1296	138.80	192	147.90	2244
123.00	52	129.70	1223	139.55	294	148.75	437
123.90	463	129.90	2426	139.90	476	149.65	549
124.75	271	130.85	1638	140.95	8591	149.80	355
125.00	58	131.70	63	142.05	1700	151.65	214
125.75	395	133.65	130	142.95	10453	152.00	204
126.00	272	134.95	1927	143.70	214	152.95	782
126.75	175	135.80	169	144.00	372	153.80	327
127.00	176	136.00	104	144.95	1091	154.20	279
127.90	3149	136.90	1934	145.85	1391	154.95	2395
128.80	273	137.70	65	146.85	938	155.70	147

Average of 14.420 to 14.426 min.: VL039479.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.95	427	169.40	99	177.00	35424		
157.05	1689	169.95	184	177.95	1021		
157.80	77	170.30	321	190.00	79		
158.70	179	170.50	157	219.90	61		
158.95	806	170.80	245	255.20	124		
159.90	290	171.45	976	256.70	76		
160.10	84	172.00	2800	266.20	76		
160.85	1372	173.00	2946	289.70	50		
164.00	63	174.00	574144	297.20	63		
166.85	218	175.00	44213				
169.10	87	176.00	547989				