


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072721\
 Data File : VL037278.D
 Acq On : 27 Jul 2021 1:56
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL072721AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Tue Jul 27 07:36:57 2021
 Last Update : Tue Jul 27 07:36:57 2021

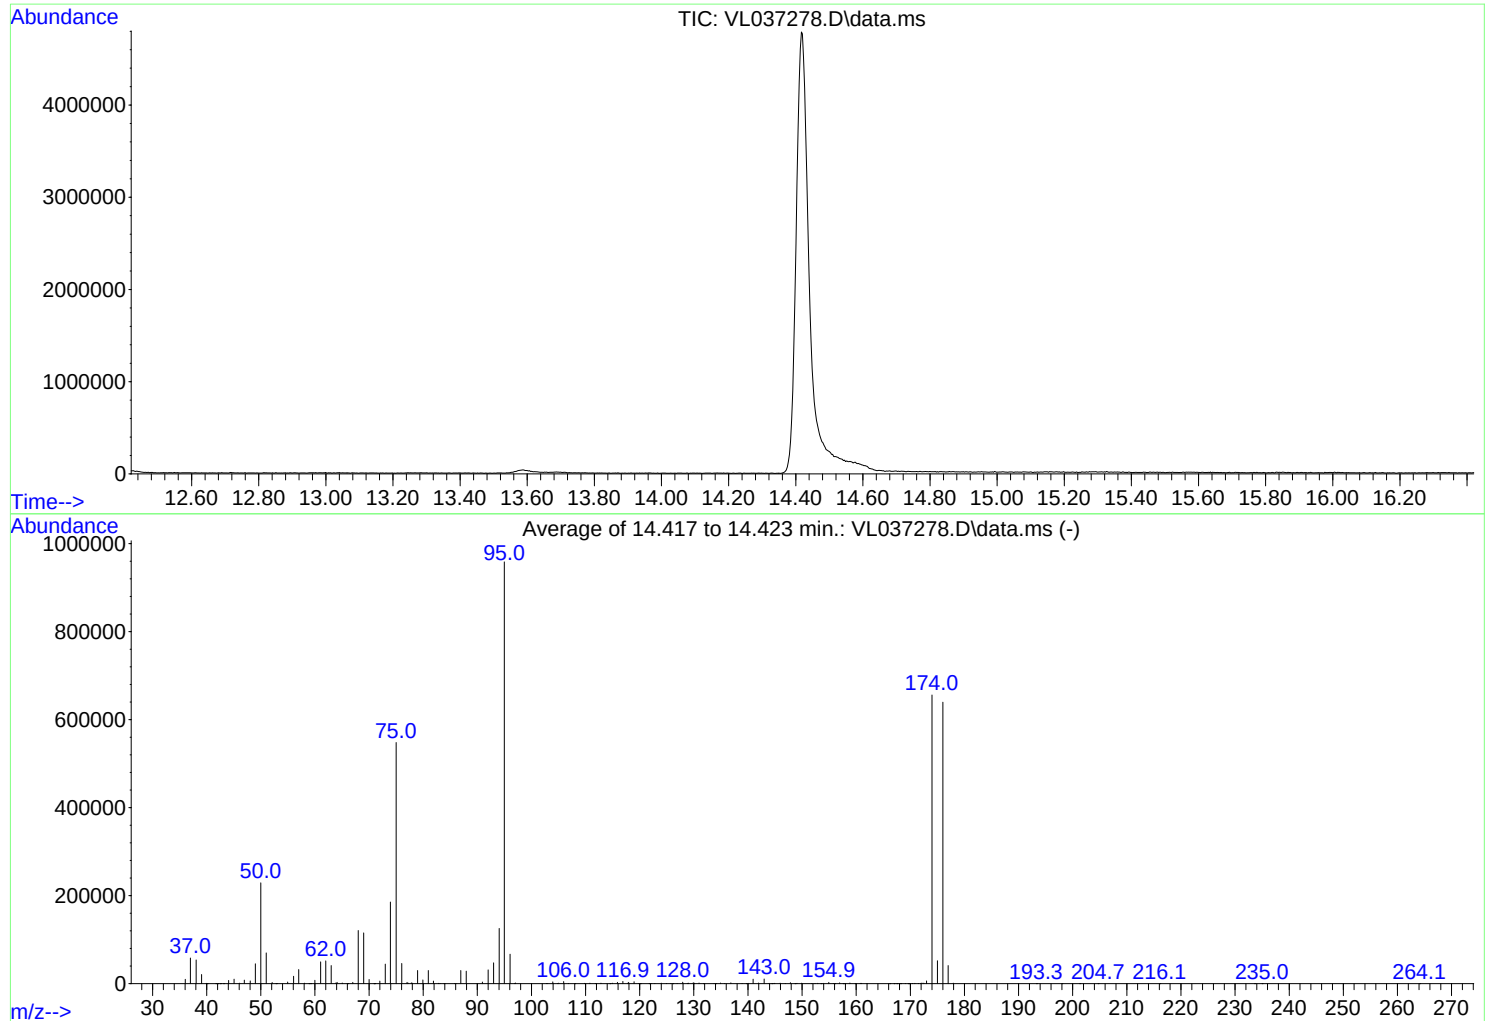

AutoFind: Scans 3617, 3618, 3619; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	229077	PASS
75	95	30	66	57.2	547883	PASS
95	95	100	100	100.0	958635	PASS
96	95	5	9	7.0	67067	PASS
173	174	0.00	2	0.9	6157	PASS
174	95	50	120	68.5	656192	PASS
175	174	4	9	7.9	52147	PASS
176	174	93	101	97.5	639808	PASS
177	176	5	9	6.4	40931	PASS

Average of 14.417 to 14.423 min.: VL037278.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	9891	44.05	7487	54.95	3583	64.10	2943
37.00	58053	45.05	10276	56.05	16737	65.05	1441
38.05	53867	46.10	1206	57.00	31928	66.00	166
39.05	20696	46.95	8107	58.05	1096	66.15	302
39.90	718	48.05	6373	58.90	106	67.00	2852
40.10	42	49.00	45080	59.20	113	68.00	120733
41.70	50	50.00	229077	60.00	7830	69.00	115347
42.05	143	51.00	69691	61.05	49368	70.00	9603
42.50	62	52.10	2590	62.00	51608	70.90	192
42.75	321	52.80	70	63.00	41205	71.00	179
43.10	205	53.05	433	63.90	1736	71.15	483

Average of 14.417 to 14.423 min.: VL037278.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
72.00	5884	80.95	29736	93.00	47219	105.95	4644
73.00	44397	81.90	5695	94.05	125603	106.85	547
73.95	185361	82.85	765	95.00	958635	108.00	54
75.00	547883	83.10	334	96.05	67067	109.80	732
76.05	45941	83.85	170	96.90	833	110.80	1070
77.00	3088	85.80	245	97.05	1410	111.80	305
77.20	1644	86.05	538	102.80	263	112.00	456
77.80	1762	86.95	29880	103.00	326	112.85	1050
78.00	947	87.95	28381	103.95	4086	114.50	54
78.95	29891	90.95	3635	104.80	454	114.95	1234
79.95	8440	92.00	31203	105.05	1191	115.90	3069

Average of 14.417 to 14.423 min.: VL037278.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.90	5063	125.75	343	134.00	123	144.40	125
117.80	1150	126.10	114	134.95	1434	144.80	501
117.95	2921	126.90	339	135.70	345	144.95	921
118.95	4495	127.95	3340	136.85	1905	145.95	1282
119.85	272	128.80	798	138.90	558	146.90	399
120.10	64	129.00	1192	139.70	182	147.85	2247
121.75	208	129.90	2318	140.05	859	148.70	65
122.10	309	130.10	1207	140.95	10116	149.05	716
122.80	337	130.95	1635	141.95	1653	149.95	1127
124.00	1110	131.80	50	143.00	10663	151.80	319
124.95	322	133.75	245	143.90	592	152.40	287

Average of 14.417 to 14.423 min.: VL037278.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
152.90	700	160.75	804	170.40	575	177.95	1214
153.50	56	161.00	601	170.85	747	193.30	74
153.90	612	162.00	249	171.50	440	198.00	60
154.95	3048	166.20	111	171.90	756	201.30	52
155.75	346	167.00	89	172.15	1512	204.70	55
156.00	162	167.50	134	172.50	1159	216.10	56
156.95	1789	167.90	144	173.00	6157	233.60	92
157.60	139	168.20	113	174.00	656192	235.00	183
157.90	110	169.10	238	175.00	52147	264.10	67
158.85	1512	169.60	97	176.00	639808		
159.80	97	169.80	130	177.00	40931		

Instrument :
MSVOA_L
ClientSampleId :
BFB