


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL073019\
 Data File : VL034047.D
 Acq On : 30 Jul 2019 1:28
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL073019AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Jul 30 06:55:18 2019
 Last Update : Tue Jul 30 06:55:18 2019

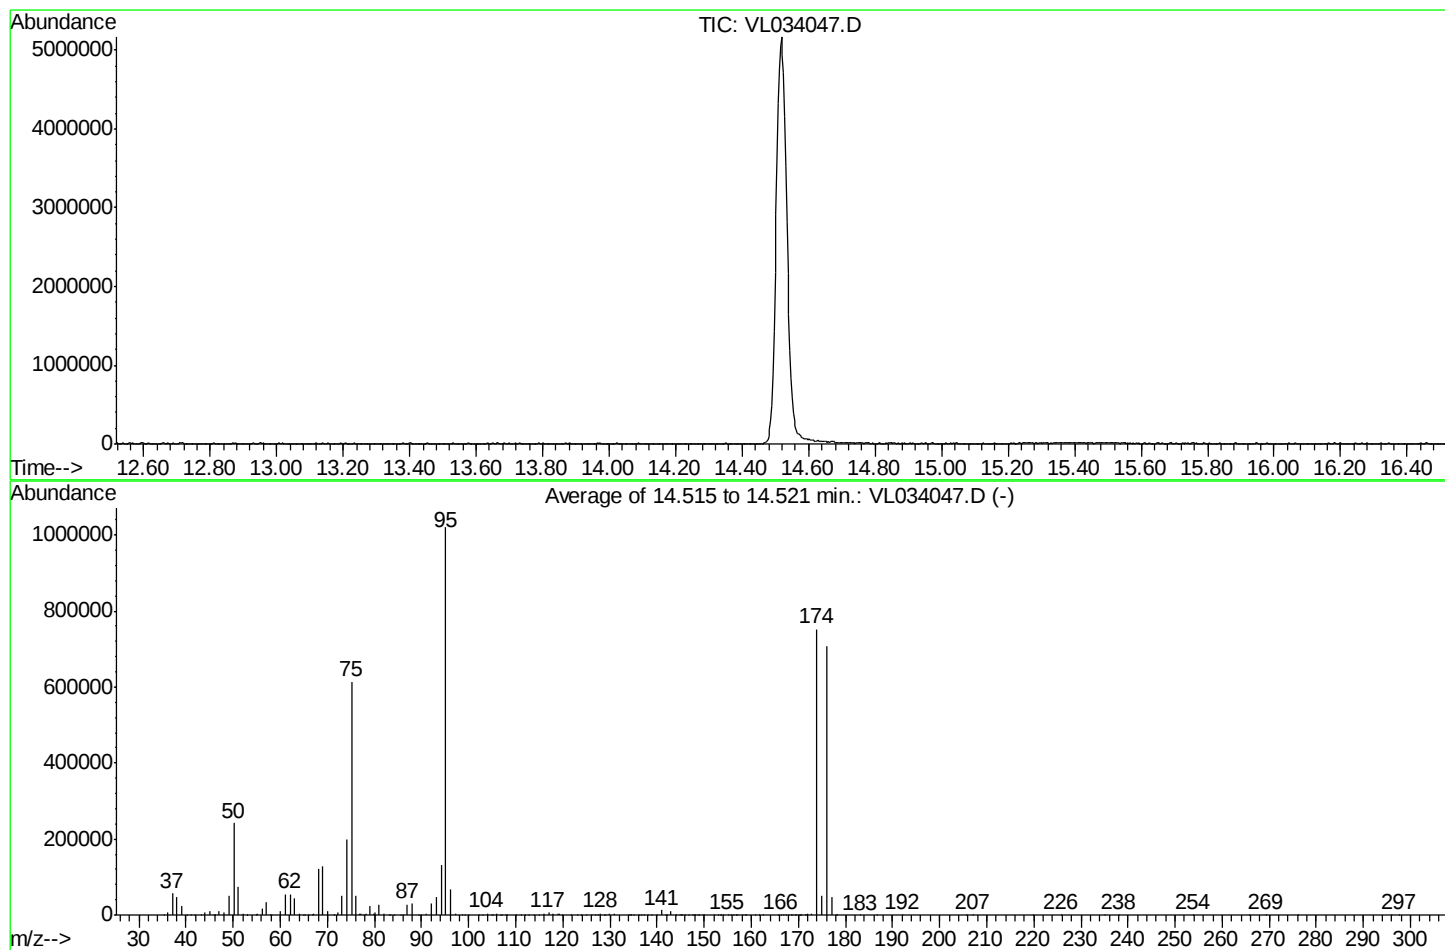

AutoFind: Scans 3601, 3602, 3603; Background Corrected with Scan 3579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.6	241088	PASS
75	95	30	66	60.1	612992	PASS
95	95	100	100	100.0	1020053	PASS
96	95	5	9	6.7	67981	PASS
173	174	0.00	2	0.7	4943	PASS
174	95	50	120	73.7	751872	PASS
175	174	4	9	6.7	50725	PASS
176	174	93	101	94.0	706794	PASS
177	176	5	9	6.6	46824	PASS