


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL073021\
 Data File : VL037287.D
 Acq On : 30 Jul 2021 16:22
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL073021AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Jul 30 23:19:30 2021
 Last Update : Fri Jul 30 23:19:30 2021

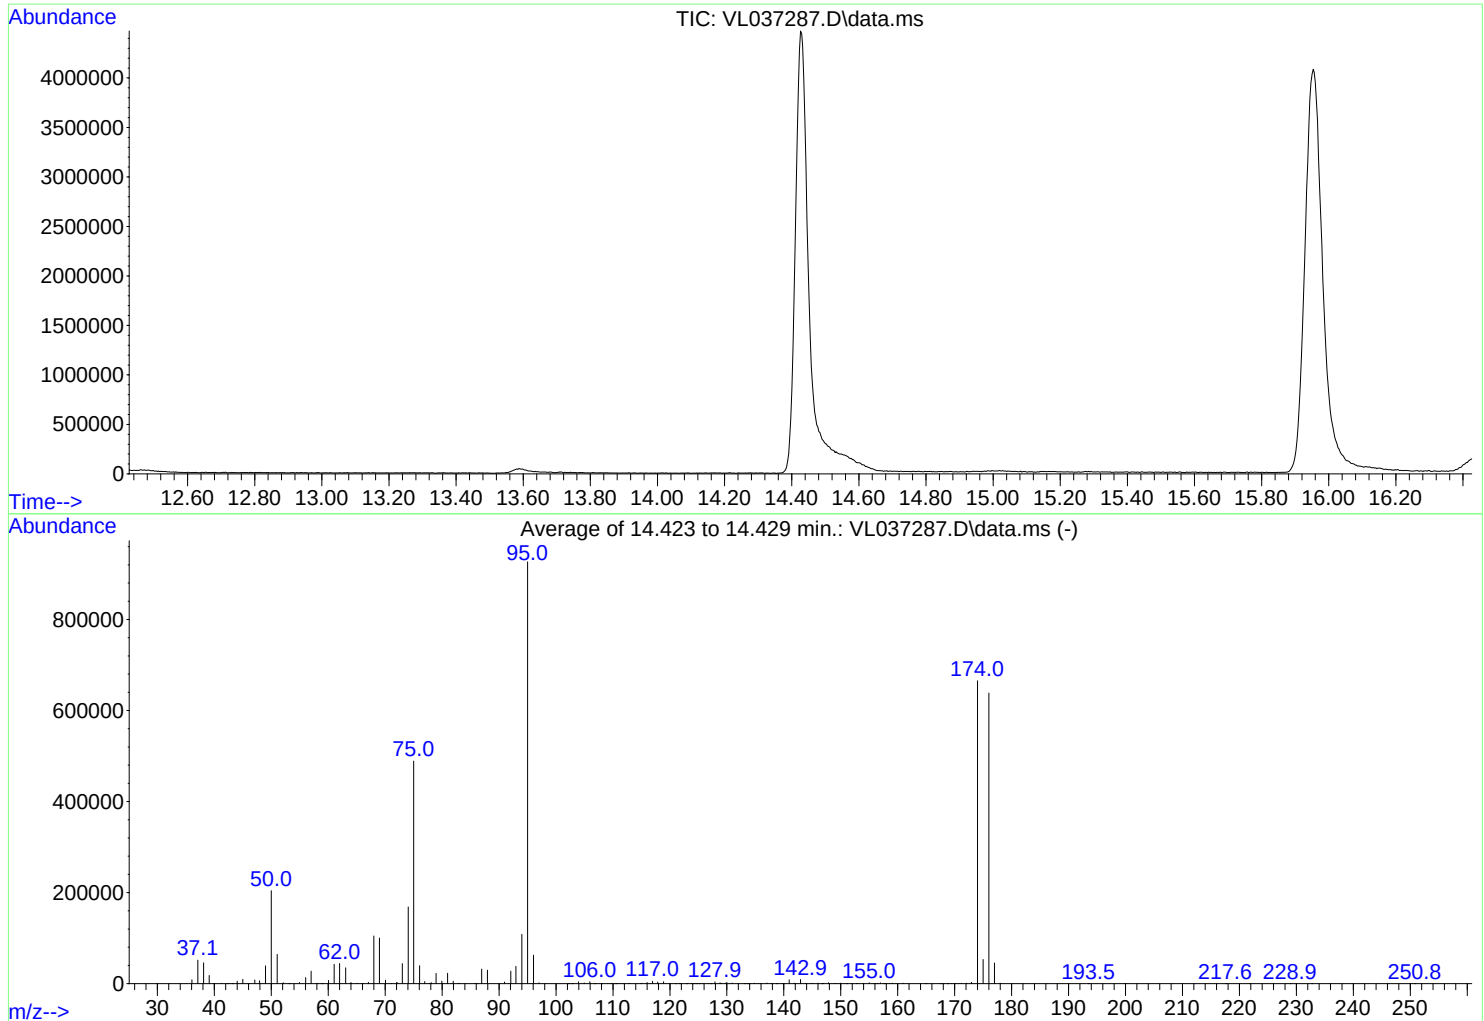

AutoFind: Scans 3619, 3620, 3621; Background Corrected with Scan 3591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.1	204395	PASS
75	95	30	66	52.8	488853	PASS
95	95	100	100	100.0	926592	PASS
96	95	5	9	6.8	62736	PASS
173	174	0.00	2	0.4	2717	PASS
174	95	50	120	71.8	665490	PASS
175	174	4	9	8.0	53184	PASS
176	174	93	101	95.9	638165	PASS
177	176	5	9	7.1	45320	PASS

Average of 14.423 to 14.429 min.: VL037287.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.05	231	45.00	9465	56.05	13254	65.05	771
36.05	8447	45.90	297	57.00	27573	65.95	147
37.10	51787	46.25	442	57.95	876	67.05	2883
38.10	45851	47.10	8186	58.20	651	68.00	104613
39.10	17919	47.95	6502	58.90	115	69.00	100275
39.95	629	49.00	38963	60.05	7144	70.05	7712
41.25	612	50.00	204395	61.05	42475	71.15	365
42.30	189	51.05	64325	62.00	44269	72.00	2507
42.90	430	52.10	2303	63.05	34880	72.20	1665
43.20	179	53.10	100	63.90	1348	73.00	43800
44.00	5292	54.95	2471	64.05	1881	74.05	168277

Average of 14.423 to 14.429 min.: VL037287.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.00	488853	85.85	804	102.20	83	110.05	334
76.05	39451	86.20	422	102.80	161	110.50	147
76.95	4714	86.95	32136	103.00	302	110.75	337
77.80	617	87.95	29616	103.95	3745	111.20	205
78.10	1988	90.95	3704	104.95	1528	111.75	407
78.95	22645	92.05	27352	105.95	4121	112.80	687
79.95	5614	92.95	38131	106.80	123	113.00	321
80.95	22712	94.00	108123	106.95	518	114.80	228
81.95	5270	95.00	926592	108.00	70	115.10	876
82.80	327	96.05	62736	109.10	217	116.00	2638
83.05	370	97.00	1839	109.70	217	116.95	5218

Average of 14.423 to 14.429 min.: VL037287.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.85	3458	125.80	229	133.60	111	140.95	8530
118.90	4269	126.75	266	133.90	163	141.90	1189
119.90	245	127.20	168	134.85	1187	142.95	9217
121.00	82	127.90	3760	135.50	210	143.85	658
121.70	109	128.80	1760	135.90	262	144.70	251
123.00	111	129.00	549	137.05	1522	144.95	711
123.75	681	129.80	1021	137.90	52	146.00	1145
124.10	148	130.00	2997	138.70	120	146.70	110
124.50	199	130.90	1248	138.90	317	146.95	610
124.70	121	132.00	293	139.70	265	147.85	2298
125.15	134	133.10	133	140.00	434	148.90	429

Average of 14.423 to 14.429 min.: VL037287.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
149.10	278	156.40	93	168.95	396	178.00	1054
149.50	263	156.95	1628	169.50	348	193.50	72
150.00	902	157.60	55	169.95	183	199.90	69
151.00	101	157.90	204	170.70	229	217.55	176
151.95	340	158.60	248	171.15	594	221.80	58
152.80	270	159.05	1027	172.10	1117	228.90	118
152.95	537	160.95	1116	172.95	2717	232.70	66
153.95	590	164.90	144	174.00	665490	250.80	57
155.00	2032	167.50	143	175.00	53184		
155.80	158	168.00	80	176.00	638165		
156.10	201	168.70	174	177.00	45320		

Instrument :
MSVOA_L
ClientSampleId :
BFB