

Data Path : W:\HPCHEM1\MSVOA_L\DATA\VL073115\
Data File : VL025811.D
Acq On : 31 Jul 2015 13:40
Operator : SY/MD
Sample : QC073015 CAN 10060
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC073015 CAN 10060

Quant Time: Jul 31 15:43:19 2015
Quant Method : W:\HPCHEM1\MSVOA_L\METHODS\VL070715AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_LWed Jul 08 02:22:55 2015
QLast Update : Wed Jul 08 02:22:55 2015
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	6.67	49	519007	10.00	ppbv	0.01
33) 1,4-Difluorobenzene	8.34	114	1386045	10.00	ppbv	0.00
55) Chlorobenzene-d5	13.76	117	1648201	10.00	ppbv	0.01

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	16.30	95	1466171	10.55	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	105.50%


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA_L\DATA\VL073115\
Data File : VL025811.D
Acq On : 31 Jul 2015 13:40
Operator : SY/MD
Sample : QC073015 CAN 10060
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC073015 CAN 10060

Quant Time: Jul 31 15:43:19 2015
Quant Method : W:\HPCHEM1\MSVOA_L\METHODS\VL070715AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Jul 08 02:22:55 2015
QLast Update : Wed Jul 08 02:22:55 2015
Response via : Initial Calibration

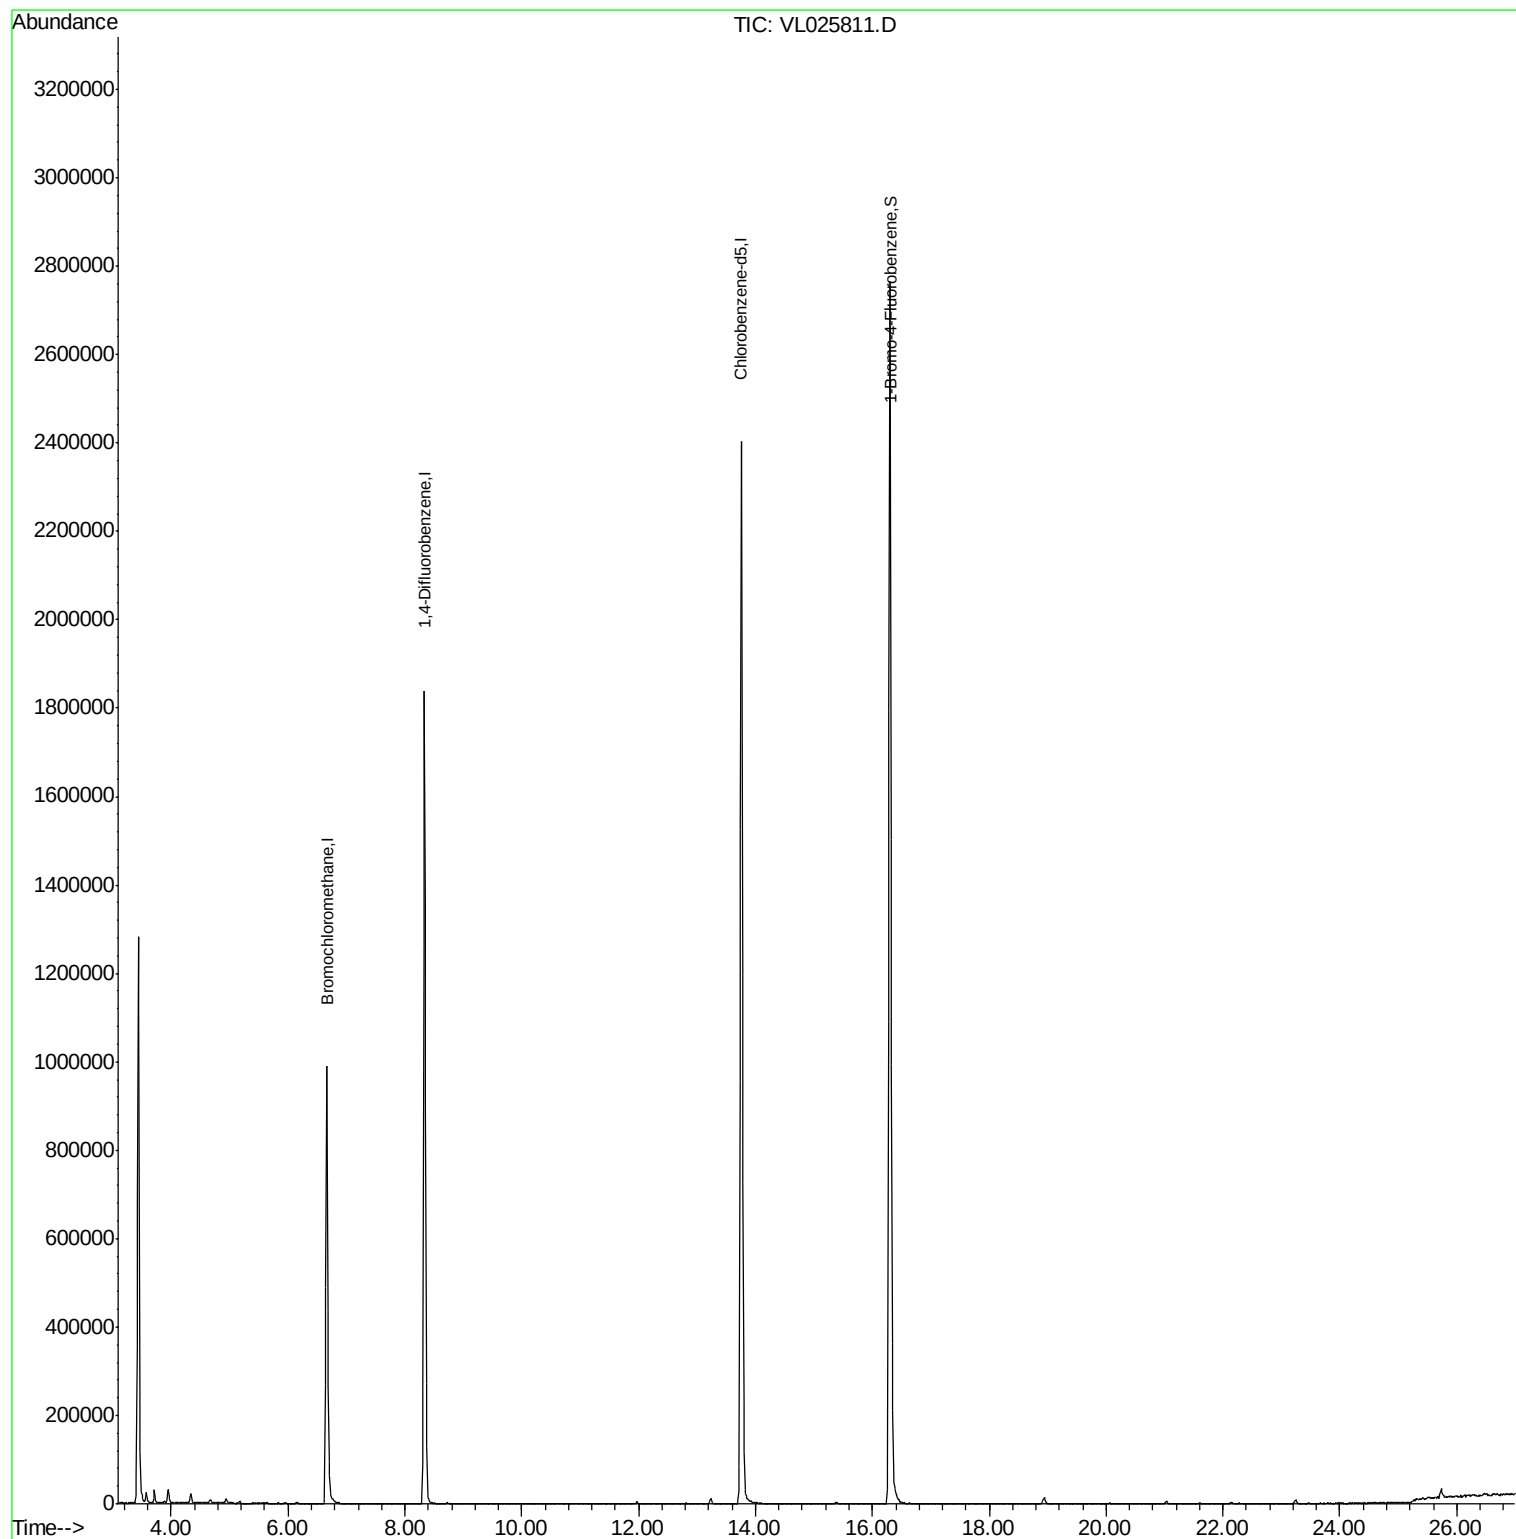

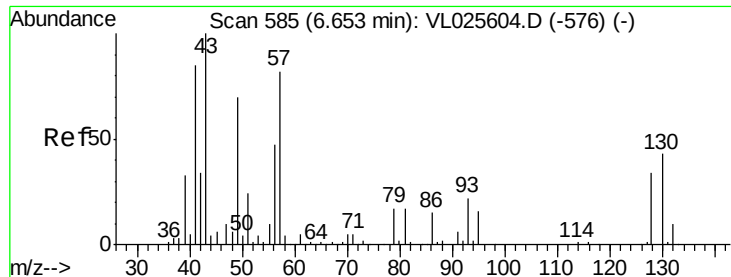

#1

Bromochloromethane

Concen: 10.00 ppbv

RT: 6.67 min Scan# 587

Delta R.T. 0.01 min

Lab File: VL025811.D

Acq: 31 Jul 2015 13:40

Instrument :

MSVOA_L

ClientSampleId :

QC073015 CAN 10060


Tgt Ion: 49 Resp: 519007

Ion Ratio Lower Upper

49 100

128 52.5 25.4 76.0




130 67.0 31.9 95.9

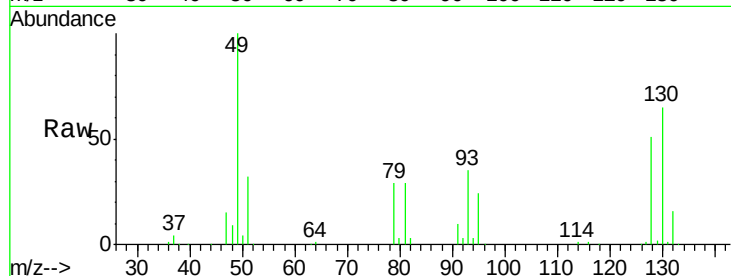

Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

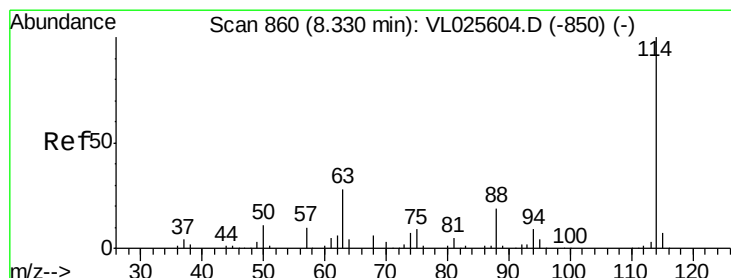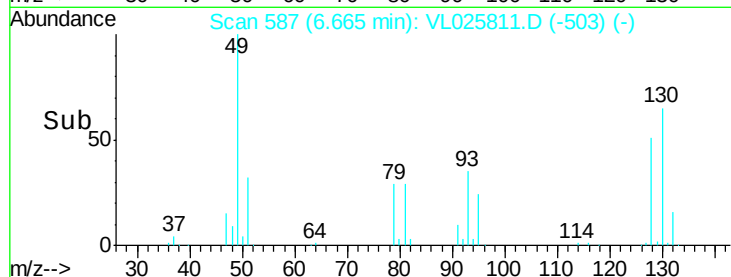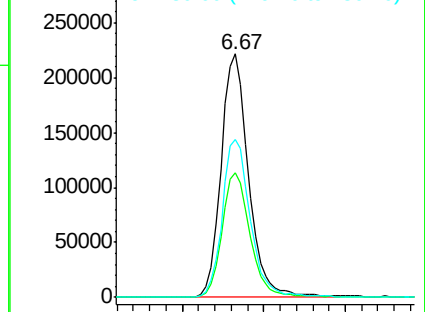

#33

1,4-Difluorobenzene

Concen: 10.00 ppbv

RT: 8.34 min Scan# 861

Delta R.T. 0.01 min

Lab File: VL025811.D

Acq: 31 Jul 2015 13:40


Tgt Ion: 114 Resp: 1386045

Ion Ratio Lower Upper

114 100

63 28.0 22.4 33.6



88 18.6 15.0 22.4

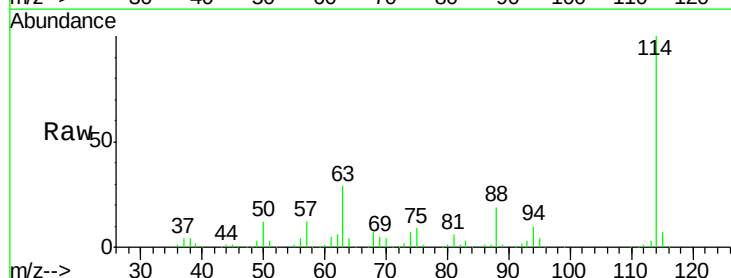


Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0



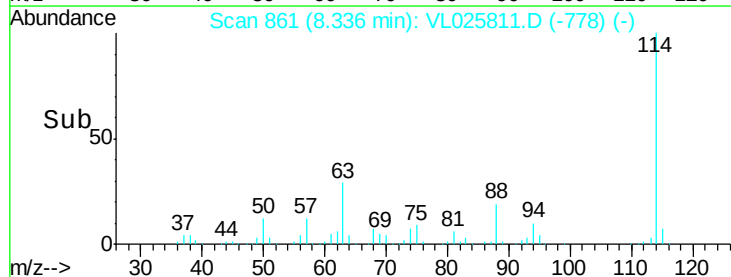
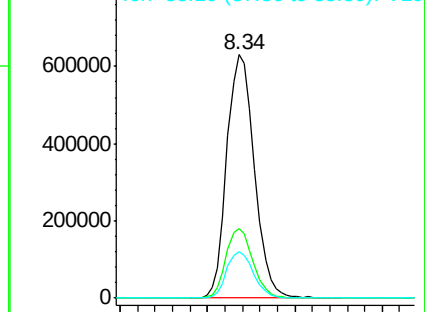


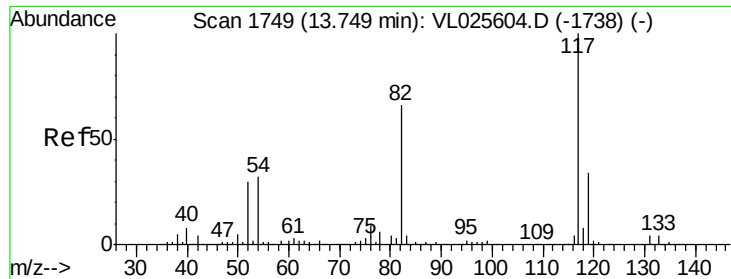

#55
Chlorobenzene-d5
Concen: 10.00 ppbv
RT: 13.76 min Scan# 1751
Delta R.T. 0.01 min
Lab File: VL025811.D
Acq: 31 Jul 2015 13:40

Instrument :
MSVOA_L
ClientSampleId :
QC073015 CAN 10060

Tgt Ion: 117 Resp: 1648201
Ion Ratio Lower Upper
117 100
82 68.2 50.5 75.7
119 32.4 45.1 67.7#

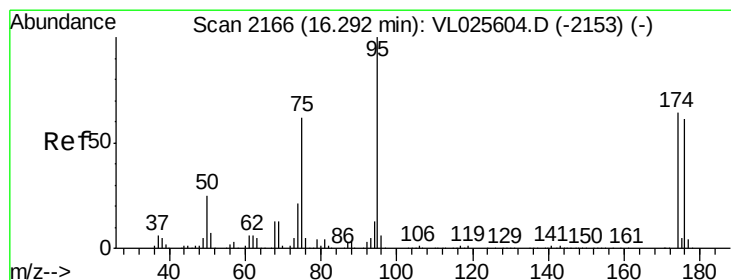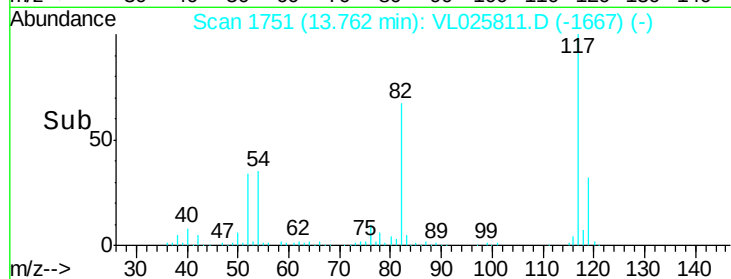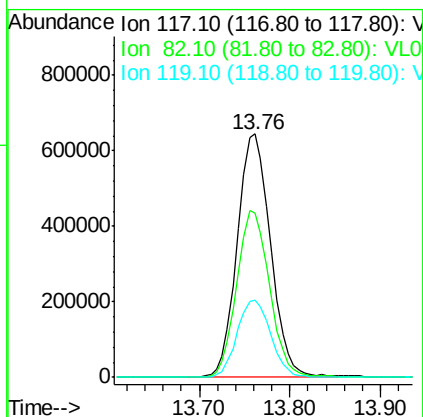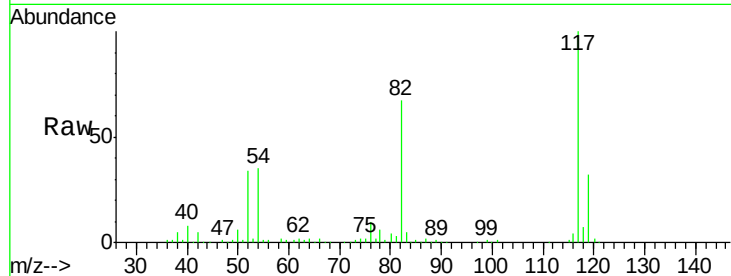

#68
1-Bromo-4-Fluorobenzene
Concen: 10.55 ppbv
RT: 16.30 min Scan# 2167
Delta R.T. 0.01 min
Lab File: VL025811.D
Acq: 31 Jul 2015 13:40

Tgt Ion: 95 Resp: 1466171
Ion Ratio Lower Upper
95 100
174 64.0 52.0 78.0
175 4.7 3.9 5.9

