
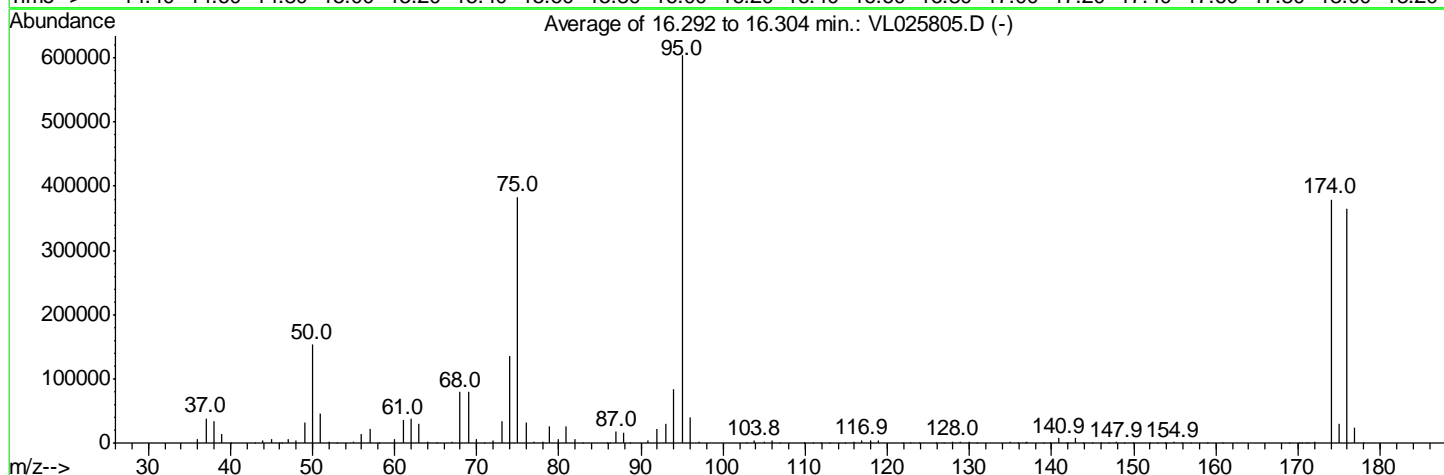


Data Path : W:\HPCHEM1\MSVOA_L\Data\VL073115\
 Data File : VL025805.D
 Acq On : 31 Jul 2015 8:21
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_L\METHODS\VL070715AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jul 08 02:22:55 2015
 Last Update : Wed Jul 08 02:22:55 2015

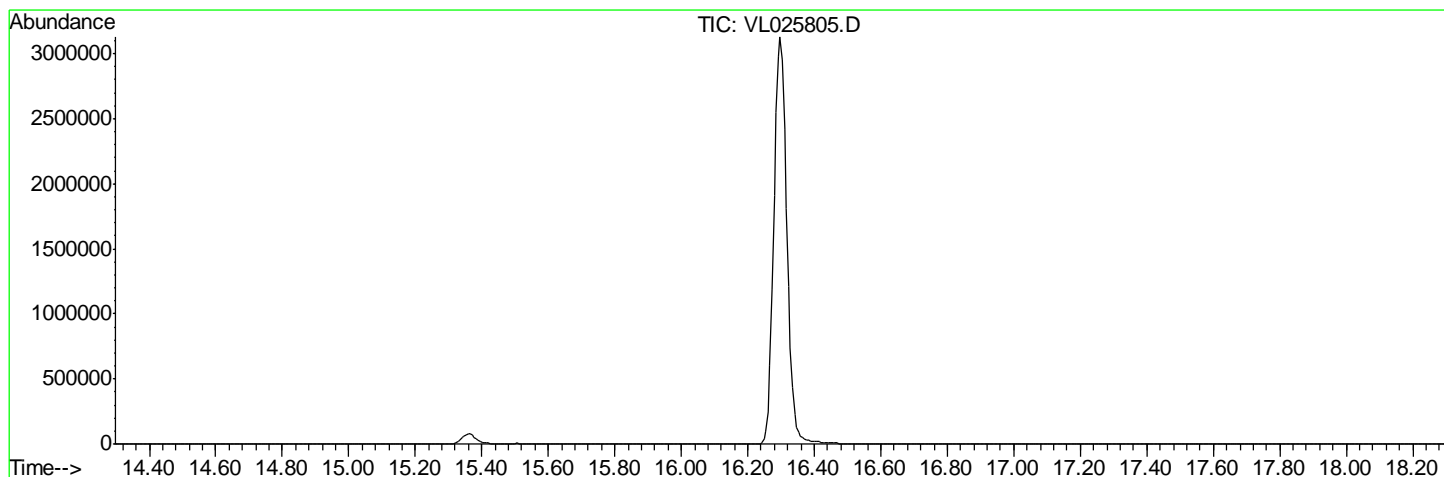

AutoFind: Scans 2166, 2167, 2168; Background Corrected with Scan 2151

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.4	153344	PASS
75	95	30	66	63.5	383530	PASS
95	95	100	100	100.0	604117	PASS
96	95	5	9	6.6	39653	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	62.9	379882	PASS
175	174	4	9	7.8	29685	PASS
176	174	93	101	96.1	365226	PASS
177	176	5	9	6.4	23400	PASS