

Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL073120\
 Data File : VL035308.D
 Acq On : 31 Jul 2020 18:38
 Operator : SY/AP
 Sample : CAN 10448
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 CAN 10448

Quant Time: Aug 01 04:05:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA L\METHODS\VL072920AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LWed Jul 29 07:14:29 2020
 QLast Update : Wed Jul 29 07:14:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.67	49	1084070	10.00	ppbv	0.00
33) 1,4-Difluorobenzene	7.19	114	2716845	10.00	ppbv	0.00
55) Chlorobenzene-d5	12.12	117	2486228	10.00	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	14.46	95	2034627	10.24	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	102.40%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA L\DATA\VL073120\
Data File : VL035308.D
Acq On : 31 Jul 2020 18:38
Operator : SY/AP
Sample : CAN 10448
Misc : 400ml/MSVOA L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
CAN 10448

Quant Time: Aug 01 04:05:40 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA L\METHODS\VL072920AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Wed Jul 29 07:14:29 2020
QLast Update : Wed Jul 29 07:14:29 2020
Response via : Initial Calibration

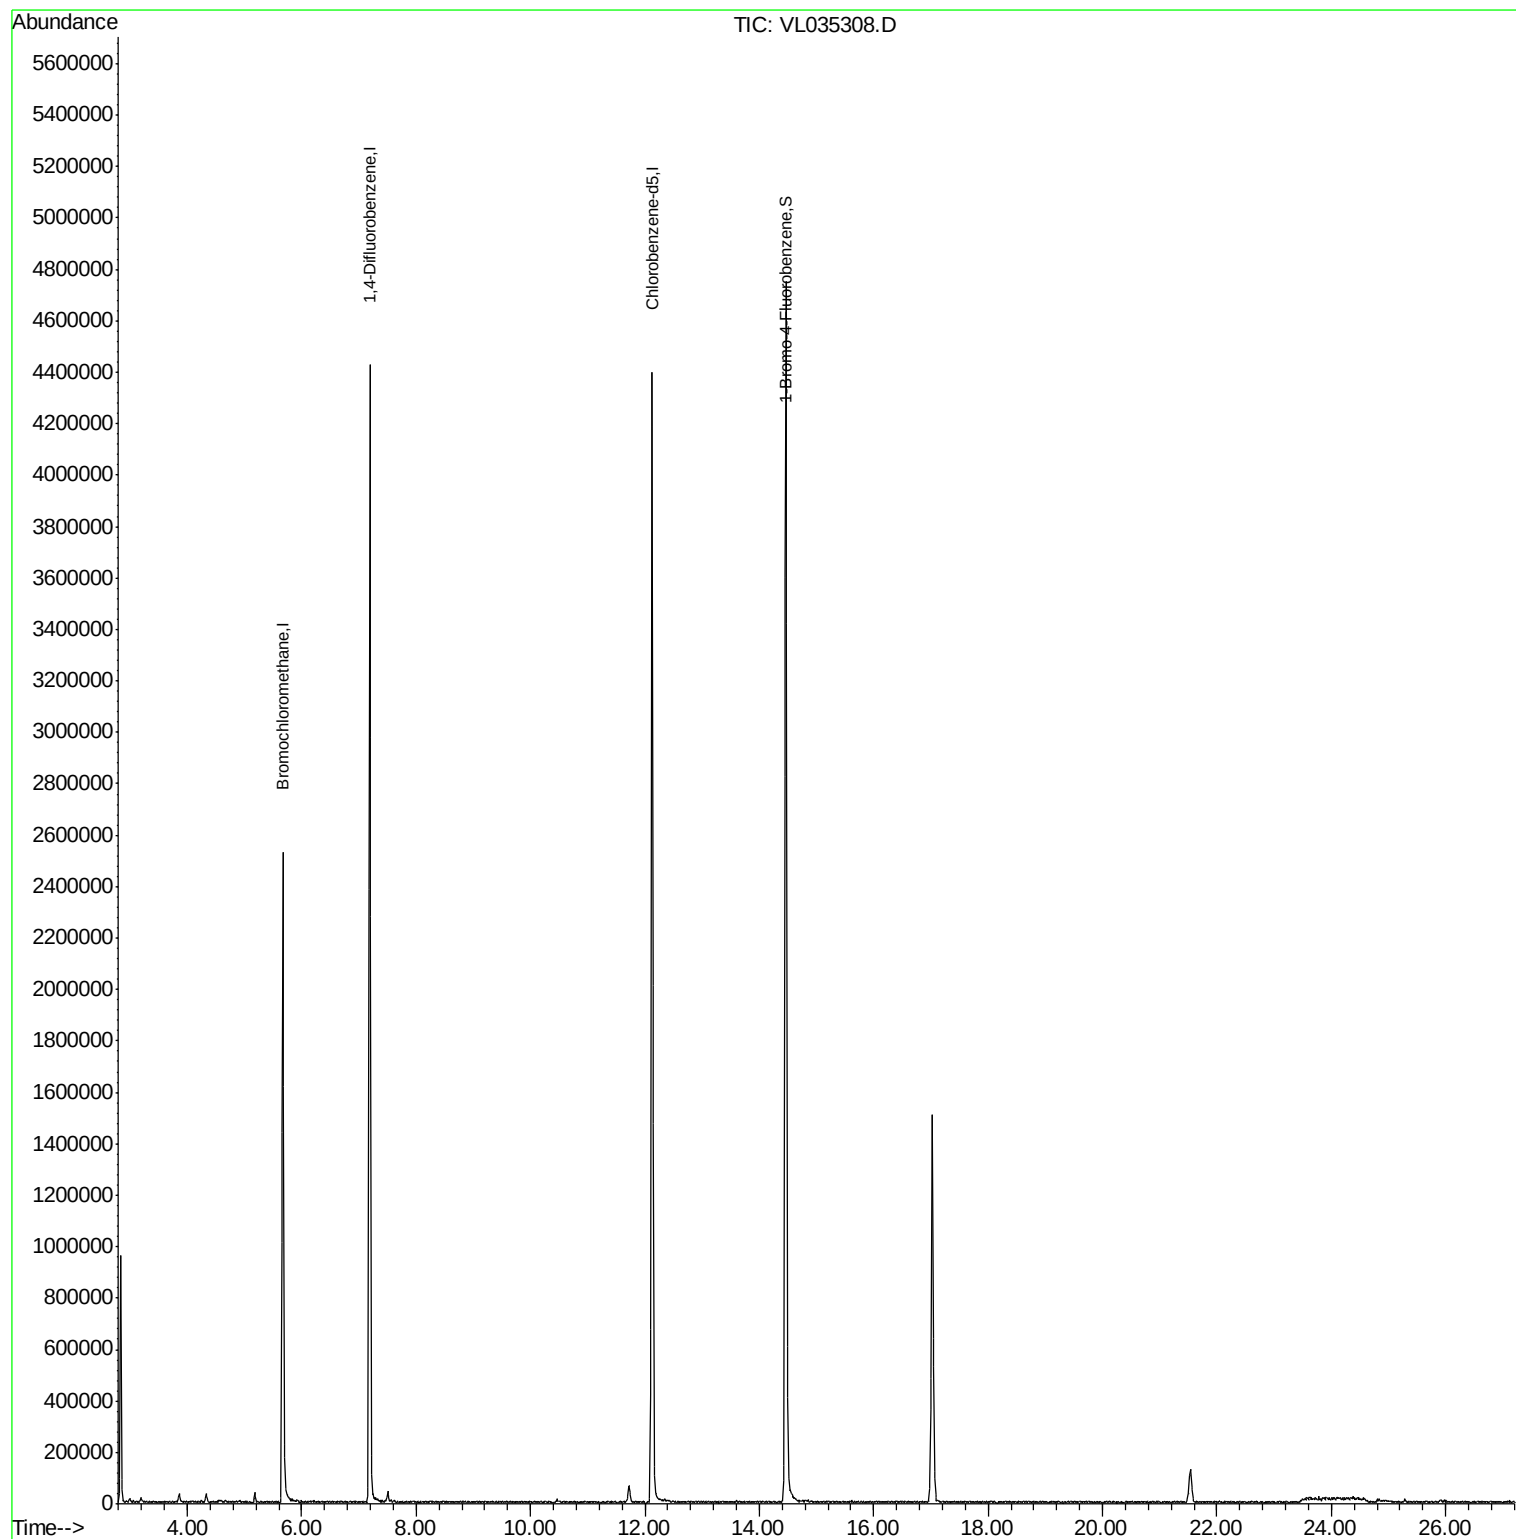

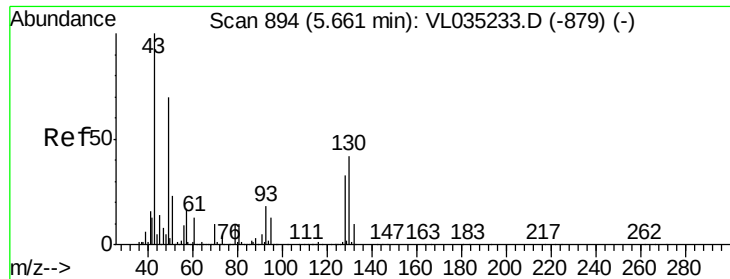

#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.67 min Scan# 896

Delta R.T. 0.01 min

Lab File: VL035308.D

Acq: 31 Jul 2020 18:38

Instrument :

MSVOA_L

ClientSampleId :

CAN 10448


Tot Ion: 49 Resp: 1084070

Ion Ratio Lower Upper

49 100

128 51.4 24.0 72.0

130 65.5 30.7 92.1



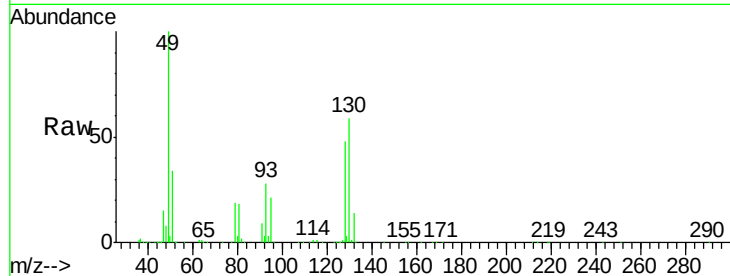


Abundance Ion 49.10 (48.80 to 49.80): VL0

Ion 128.00 (127.70 to 128.70): VL0

Ion 130.00 (129.70 to 130.70): VL0

5.67

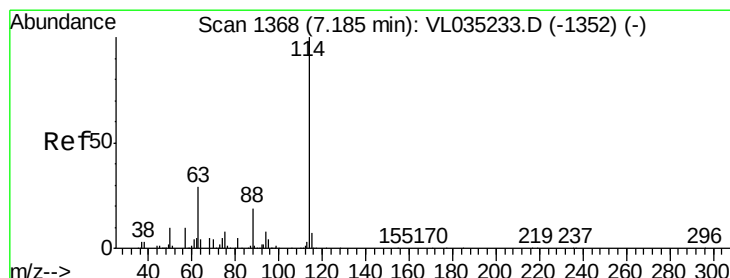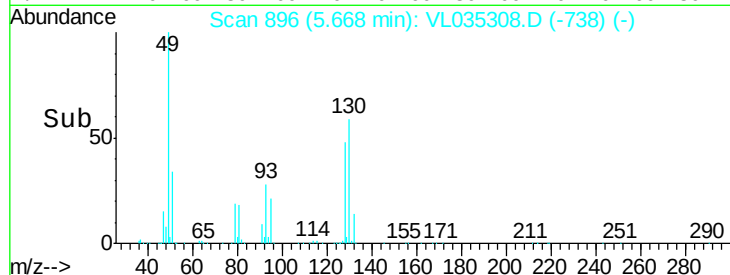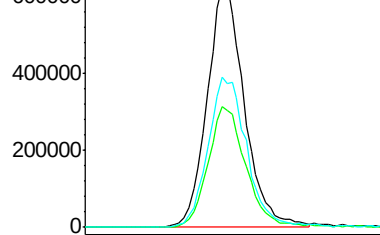

#33

1,4-Difluorobenzene

Concen: 10.000 ppbv

RT: 7.19 min Scan# 1369

Delta R.T. 0.00 min

Lab File: VL035308.D

Acq: 31 Jul 2020 18:38


Tgt Ion: 114 Resp: 2716845

Ion Ratio Lower Upper

114 100

63 27.9 22.2 33.2

88 19.2 15.4 23.0


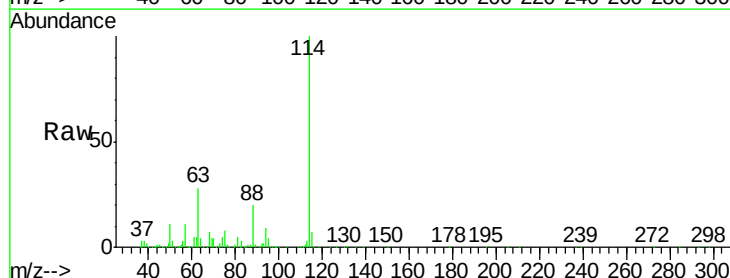



Abundance Ion 114.10 (113.80 to 114.80): VL0

Ion 63.10 (62.80 to 63.80): VL0

Ion 88.10 (87.80 to 88.80): VL0

7.19



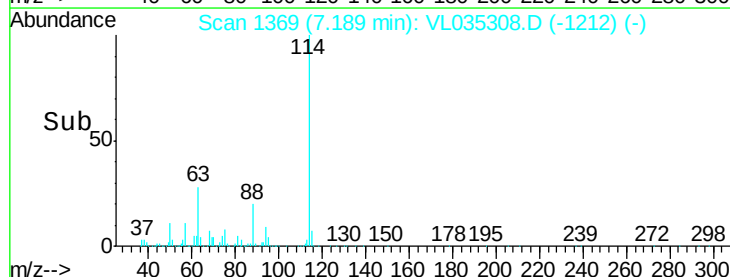
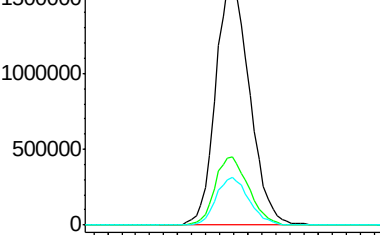


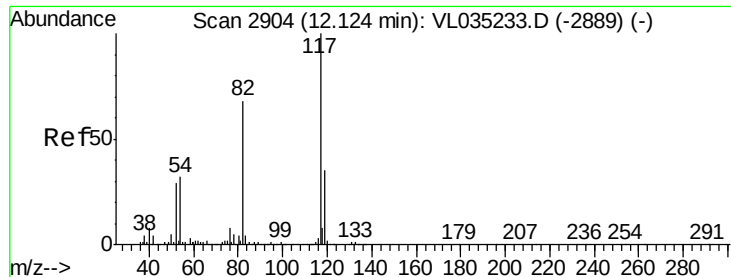

#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 12.12 min Scan# 2904
Delta R.T. 0.00 min
Lab File: VL035308.D
Acq: 31 Jul 2020 18:38

Instrument :
MSVOA_L
ClientSampleId :
CAN 10448

Tot Ion:117 Resp: 2486228
Ion Ratio Lower Upper
117 100
82 69.1 52.4 78.6
119 32.9 24.6 36.8

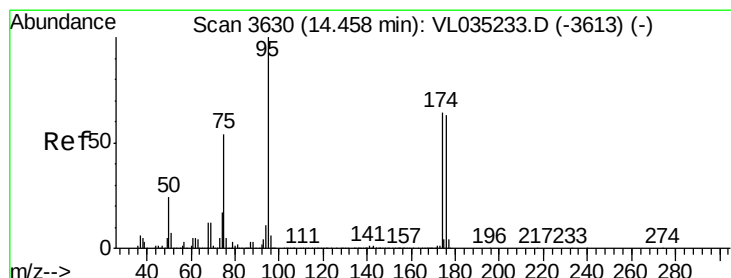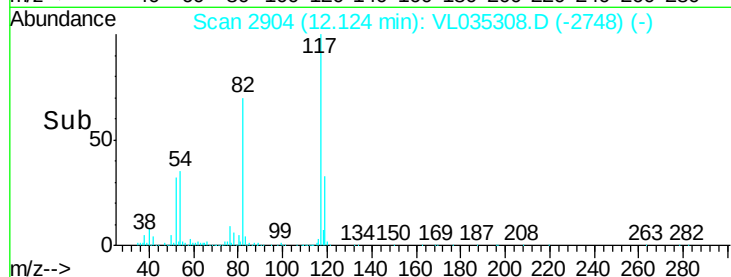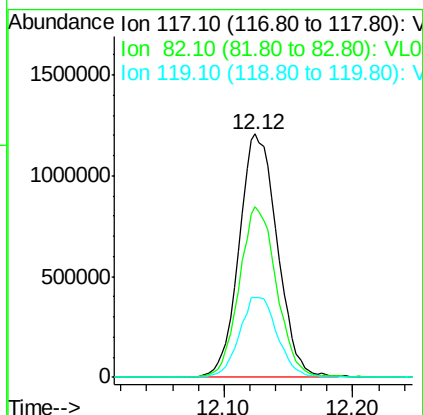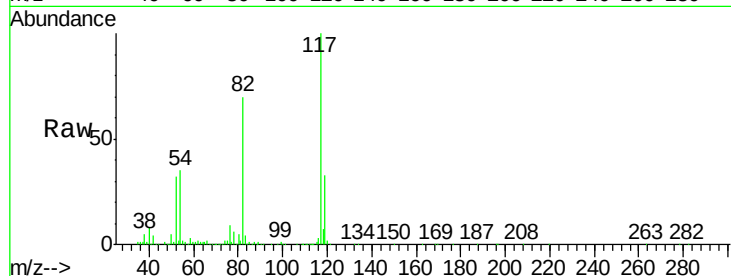

#68
1-Bromo-4-Fluorobenzene
Concen: 10.241 ppbv
RT: 14.46 min Scan# 3631
Delta R.T. 0.00 min
Lab File: VL035308.D
Acq: 31 Jul 2020 18:38

Tgt Ion: 95 Resp: 2034627
Ion Ratio Lower Upper
95 100
174 65.5 52.7 79.1
175 4.9 3.9 5.9

