
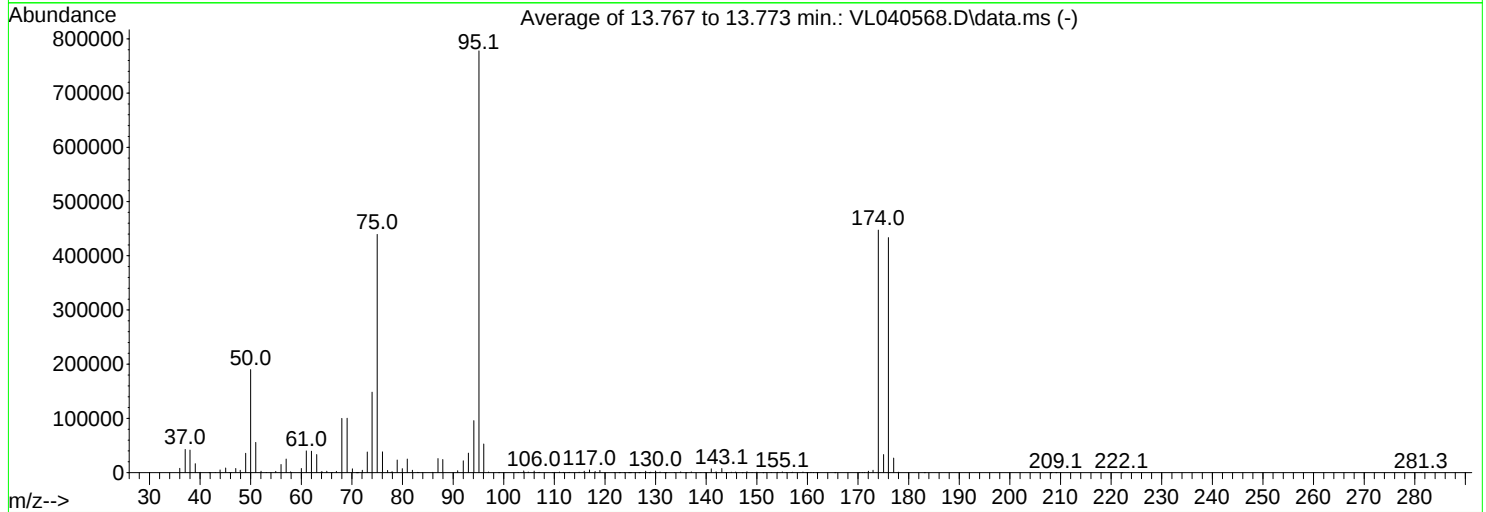


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL073123\
 Data File : VL040568.D
 Acq On : 31 Jul 2023 11:06
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL071023AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Mon Jul 10 16:32:00 2023

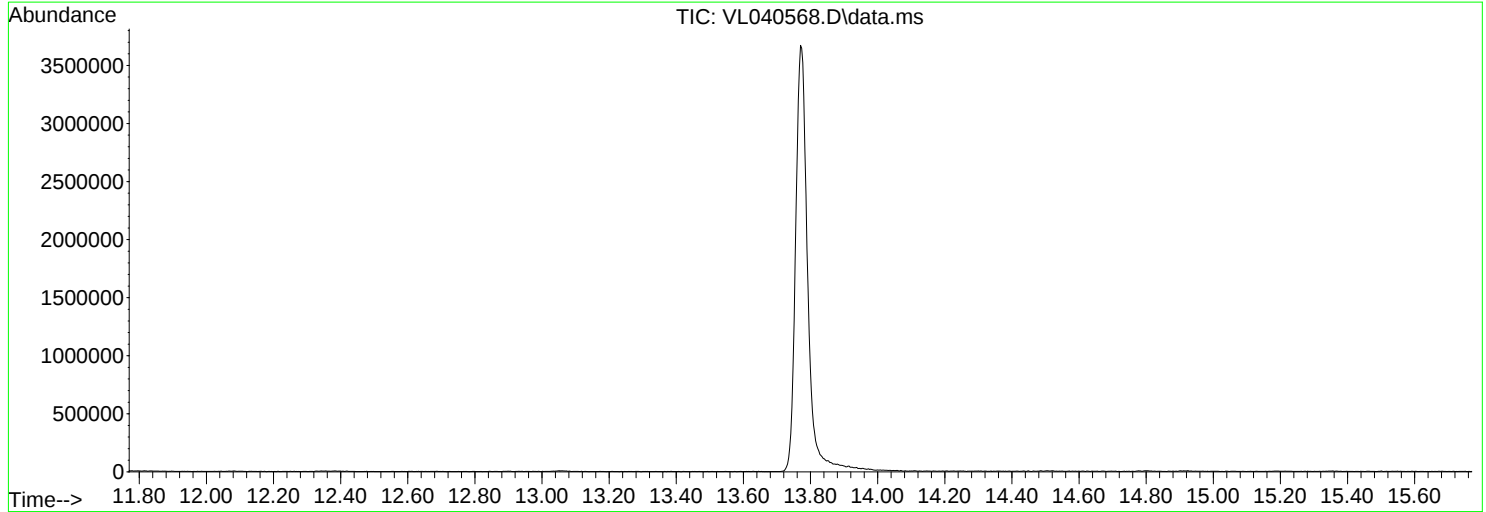

AutoFind: Scans 3472, 3473, 3474; Background Corrected with Scan 3450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.4	189973	PASS
75	95	30	66	56.5	439445	PASS
95	95	100	100	100.0	777899	PASS
96	95	5	9	6.8	52760	PASS
173	174	0.00	2	1.0	4342	PASS
174	95	50	120	57.5	447253	PASS
175	174	4	9	7.5	33469	PASS
176	174	93	101	96.9	433493	PASS
177	176	5	9	6.2	26973	PASS

Average of 13.767 to 13.773 min.: VL040568.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	7875	47.05	7683	57.90	1361	66.95	243
37.05	42843	47.95	4559	58.10	363	68.00	10000
38.00	41752	49.00	35664	60.00	7803	69.05	10032
39.05	16456	50.00	189973	61.00	40237	70.10	703
40.05	511	51.00	55872	62.00	39565	70.90	100
41.80	82	52.05	2712	63.05	33267	71.10	60
43.00	359	53.10	386	63.95	1888	72.05	4329
43.95	4898	54.00	330	64.15	1059	73.05	37979
45.05	8460	54.95	2461	65.05	2570	74.00	148544
45.80	389	56.00	15206	65.90	357	75.00	439445
46.15	444	57.00	25243	66.20	259	76.05	38499

Average of 13.767 to 13.773 min.: VL040568.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.05	4058	87.00	25883	103.95	3224	112.95	519
77.70	612	87.95	24064	104.85	1313	114.90	854
77.95	1738	90.90	3492	106.00	3049	115.90	2603
78.95	23227	92.00	21912	106.80	248	116.95	4915
79.95	7392	93.00	36099	107.10	647	118.05	2075
80.95	25027	94.10	95797	109.70	180	119.00	4061
81.95	4336	95.10	777899	110.05	623	121.85	198
83.00	672	96.05	52760	111.00	1086	122.80	156
83.20	246	97.00	1294	111.75	591	123.00	161
83.95	298	99.00	102	112.05	415	123.85	233
85.95	544	102.85	203	112.70	214	124.70	65

Average of 13.767 to 13.773 min.: VL040568.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
125.00	126	133.75	432	144.10	273	155.05	1409
126.00	470	134.95	1443	144.95	896	155.85	422
126.70	142	136.00	89	145.85	1089	156.80	346
127.05	328	137.05	1603	147.10	77	157.10	774
128.05	2745	138.95	280	148.05	1938	159.10	1058
128.75	156	139.80	477	149.05	418	159.90	147
129.05	926	140.10	285	150.00	966	160.70	572
130.00	2837	141.00	7059	151.20	66	161.20	311
130.90	1333	141.95	1410	151.85	194	161.90	77
131.70	210	143.10	7803	152.85	363	165.40	152
132.00	56	143.90	379	154.10	676	170.25	271

Average of 13.767 to 13.773 min.: VL040568.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.85	414	209.10	78				
171.30	213	222.10	56				
172.05	2730	281.25	217				
172.95	4342						
174.00	447253						
175.05	33469						
176.00	433493						
177.05	26973						
178.00	843						
183.10	53						
208.10	73						