


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL073124\
Data File : VL041452.D
Acq On : 31 Jul 2024 7:28
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Aug 01 02:36:30 2024

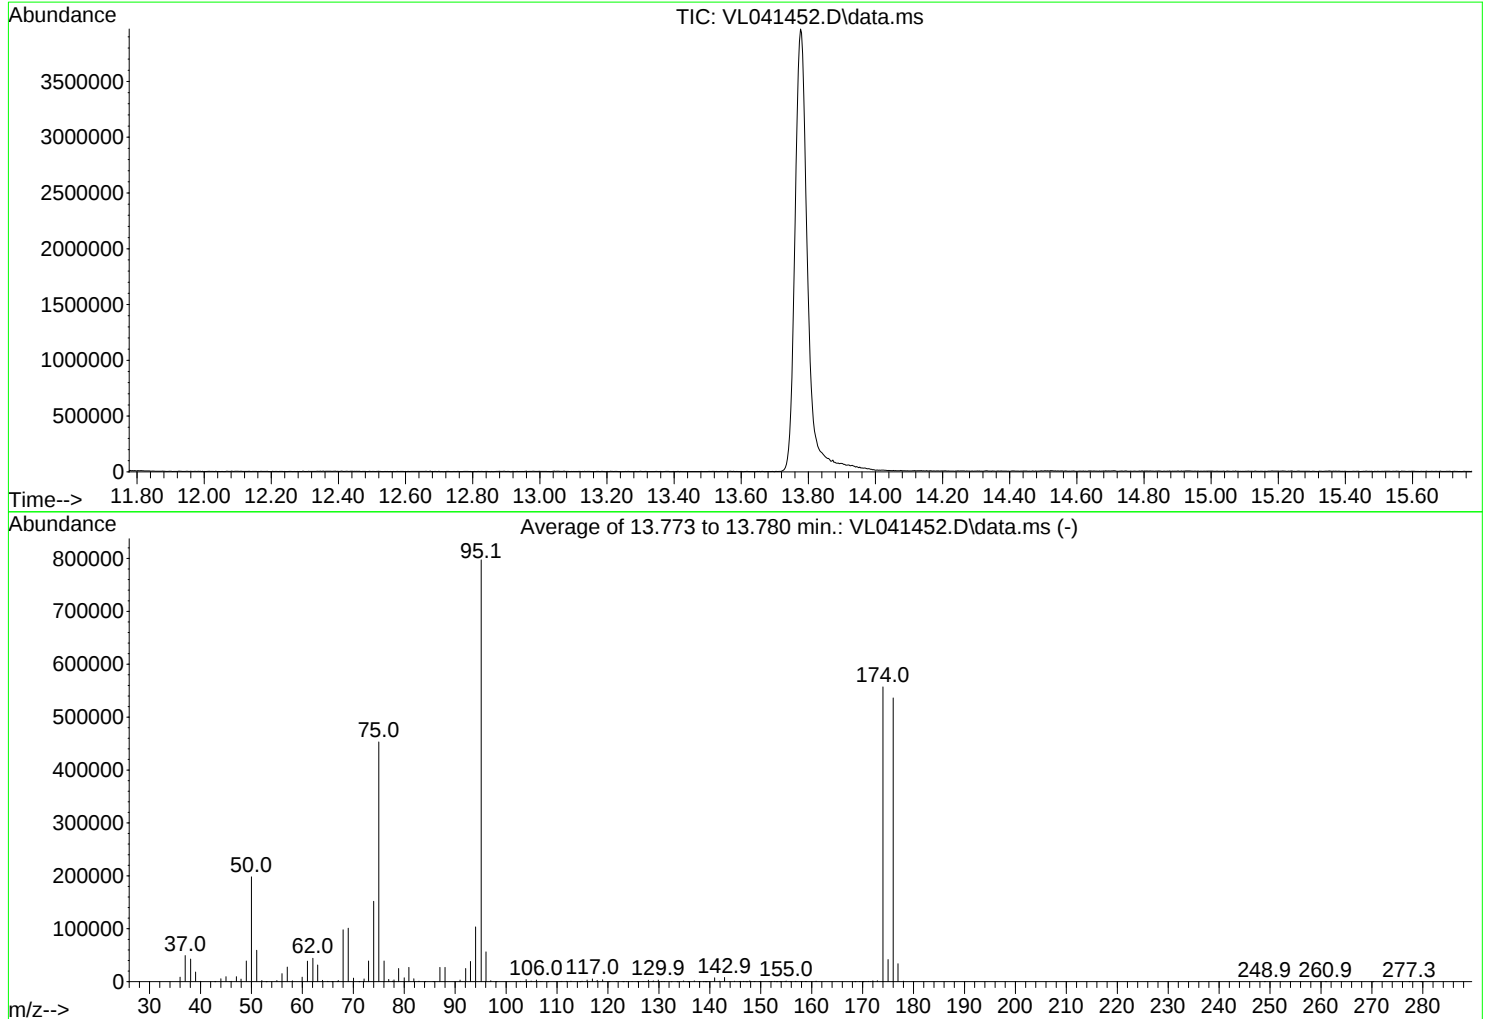

AutoFind: Scans 3474, 3475, 3476; Background Corrected with Scan 3447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.8	197995	PASS
75	95	30	66	56.8	453227	PASS
95	95	100	100	100.0	797355	PASS
96	95	5	9	7.1	56309	PASS
173	174	0.00	2	0.3	1862	PASS
174	95	50	120	69.9	557248	PASS
175	174	4	9	7.5	41757	PASS
176	174	93	101	96.3	536405	PASS
177	176	5	9	6.3	33896	PASS

Average of 13.773 to 13.780 min.: VL041452.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	8520	47.95	5020	61.00	38597	70.05	6761
37.00	49325	49.00	38955	62.05	44091	71.10	1330
38.05	42793	50.00	197995	63.00	31549	72.10	529
39.05	18075	51.05	59245	63.95	2559	73.00	3912
40.00	725	52.05	2274	64.95	571	74.00	151744
42.80	73	52.90	56	65.20	313	75.00	453227
44.00	5570	55.00	2175	65.80	73	76.05	39155
45.00	9273	56.00	15174	66.90	744	76.95	4169
45.80	205	57.05	27629	67.05	2174	77.70	871
46.05	648	58.05	1443	68.00	98019	78.00	3441
47.05	9543	59.95	8542	69.00	101123	78.90	24915

Average of 13.773 to 13.780 min.: VL041452.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.00	7410	93.00	38048	107.05	362	117.90	2384
80.90	26832	94.00	103501	108.20	118	118.95	3752
81.90	5451	95.10	797355	109.95	474	120.20	58
82.90	896	96.05	56309	110.60	210	121.70	195
84.00	74	97.00	1722	110.95	489	122.80	213
85.70	196	98.00	98	111.90	504	123.00	85
85.90	317	102.85	532	112.75	870	123.70	261
87.00	27000	103.95	3910	114.50	91	124.00	406
88.00	27096	104.90	1235	114.90	813	124.75	396
90.95	3152	105.95	3152	115.90	3072	125.80	126
92.05	24811	106.80	381	116.95	5052	126.00	216

Average of 13.773 to 13.780 min.: VL041452.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.90	401	135.70	93	143.90	388	149.95	596
127.95	2716	136.95	1492	144.85	866	151.65	251
128.70	353	137.90	136	145.80	358	152.10	251
128.90	1419	138.70	162	146.00	723	152.75	697
129.90	3131	139.10	88	146.60	527	153.10	145
130.50	365	139.30	170	146.90	300	153.80	76
130.80	251	139.80	208	147.20	105	153.95	414
131.10	333	140.00	301	147.85	1655	154.80	344
132.40	77	140.95	7350	148.70	223	155.00	1319
133.60	129	141.85	1038	148.85	423	155.80	86
134.85	1622	142.90	7984	149.70	196	156.80	615

Average of 13.773 to 13.780 min.: VL041452.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
157.10	458	172.00	1469	279.60	98		
157.90	88	172.90	1862				
158.80	439	174.00	557248				
159.00	311	175.00	41757				
160.85	1021	176.00	536405				
168.50	116	176.95	33896				
169.45	302	178.00	871				
170.10	78	248.90	59				
170.65	296	260.90	65				
171.10	497	270.20	95				
171.60	264	277.30	117				