

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL080124\
 Data File : VL041488.D
 Acq On : 1 Aug 2024 22:01
 Operator : SY/MD
 Sample : P3445-05
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 3RD-FLOOR

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 08/02/2024
 Supervised By :Mahesh Dadoda 08/03/2024

Quant Time: Aug 02 04:15:57 2024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug 2

QLast Update : Fri Aug 02 03:13:29 2024

Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	5.195	49	926420	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	6.655	114	2420057	10.000	ppbv	0.00
55) Chlorobenzene-d5	11.468	117	2240524	10.000	ppbv	# 0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	13.773	95	1738618	10.083	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	= 100.800%	
Target Compounds						Qvalue
2) Dichlorodifluoromethane	2.735	85	49744m	0.312	ppbv	
3) Chlorodifluoromethane	2.677	51	456790	4.142	ppbv	93
4) Chloromethane	2.819	50	41418	0.706	ppbv	91
9) Propene	2.709	41	317306m	6.263	ppbv	
10) Heptane	7.581	43	17509	0.154	ppbv #	76
11) Trichlorofluoromethane	3.565	101	30781	0.217	ppbv	92
13) Ethanol	3.256	45	6211199	1371.689	ppbv	96
15) Acetone	3.468	43	1846064	17.538	ppbv	99
17) tert-Butyl alcohol	3.902	59	38461m	0.401	ppbv	
19) Isopropyl Alcohol	3.597	45	1602682	26.044	ppbv	100
20) Methylene Chloride	3.934	84	3352491	85.409	ppbv	95
26) Hexane	5.214	57	1606829	18.523	ppbv #	43
29) Chloroform	5.275	83	94091	0.665	ppbv	90
30) Cyclohexane	6.603	84	13242m	0.187	ppbv	
34) 2-Butanone	4.793	43	111354	0.951	ppbv	95
35) Carbon Tetrachloride	6.494	117	9076m	0.068	ppbv	
36) Benzene	6.372	78	55333	0.313	ppbv	95
41) Tetrahydrofuran	5.565	42	19120m	0.286	ppbv	
44) 2,2,4-Trimethylpentane	7.330	57	110780m	0.375	ppbv	
53) Toluene	9.227	91	216118	1.097	ppbv	100
58) Ethyl Benzene	12.088	91	29086m	0.113	ppbv	
59) m/p-Xylene	12.352	91	72758m	0.326	ppbv	
60) o-Xylene	13.056	91	32129m	0.152	ppbv	
61) Styrene	12.905	104	10250m	0.108	ppbv	
69) p-Isopropyltoluene	16.995	119	34809m	0.105	ppbv	
73) 1,3,5-Trimethylbenzene	15.352	105	30105m	0.141	ppbv	
74) 1,2,4-Trimethylbenzene	16.108	105	91771	0.369	ppbv #	69
76) 1,4-Dichlorobenzene	16.474	146	39484m	0.261	ppbv	
79) Naphthalene	21.384	128	34229m	0.156	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL080124\
Data File : VL041488.D
Acq On : 1 Aug 2024 22:01
Operator : SY/MD
Sample : P3445-05
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_L
ClientSampleId :
3RD-FLOOR

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 08/02/2024
Supervised By :Mahesh Dadoda 08/03/2024

Quant Time: Aug 02 04:15:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Fri Aug 02 03:13:29 2024
Response via : Initial Calibration

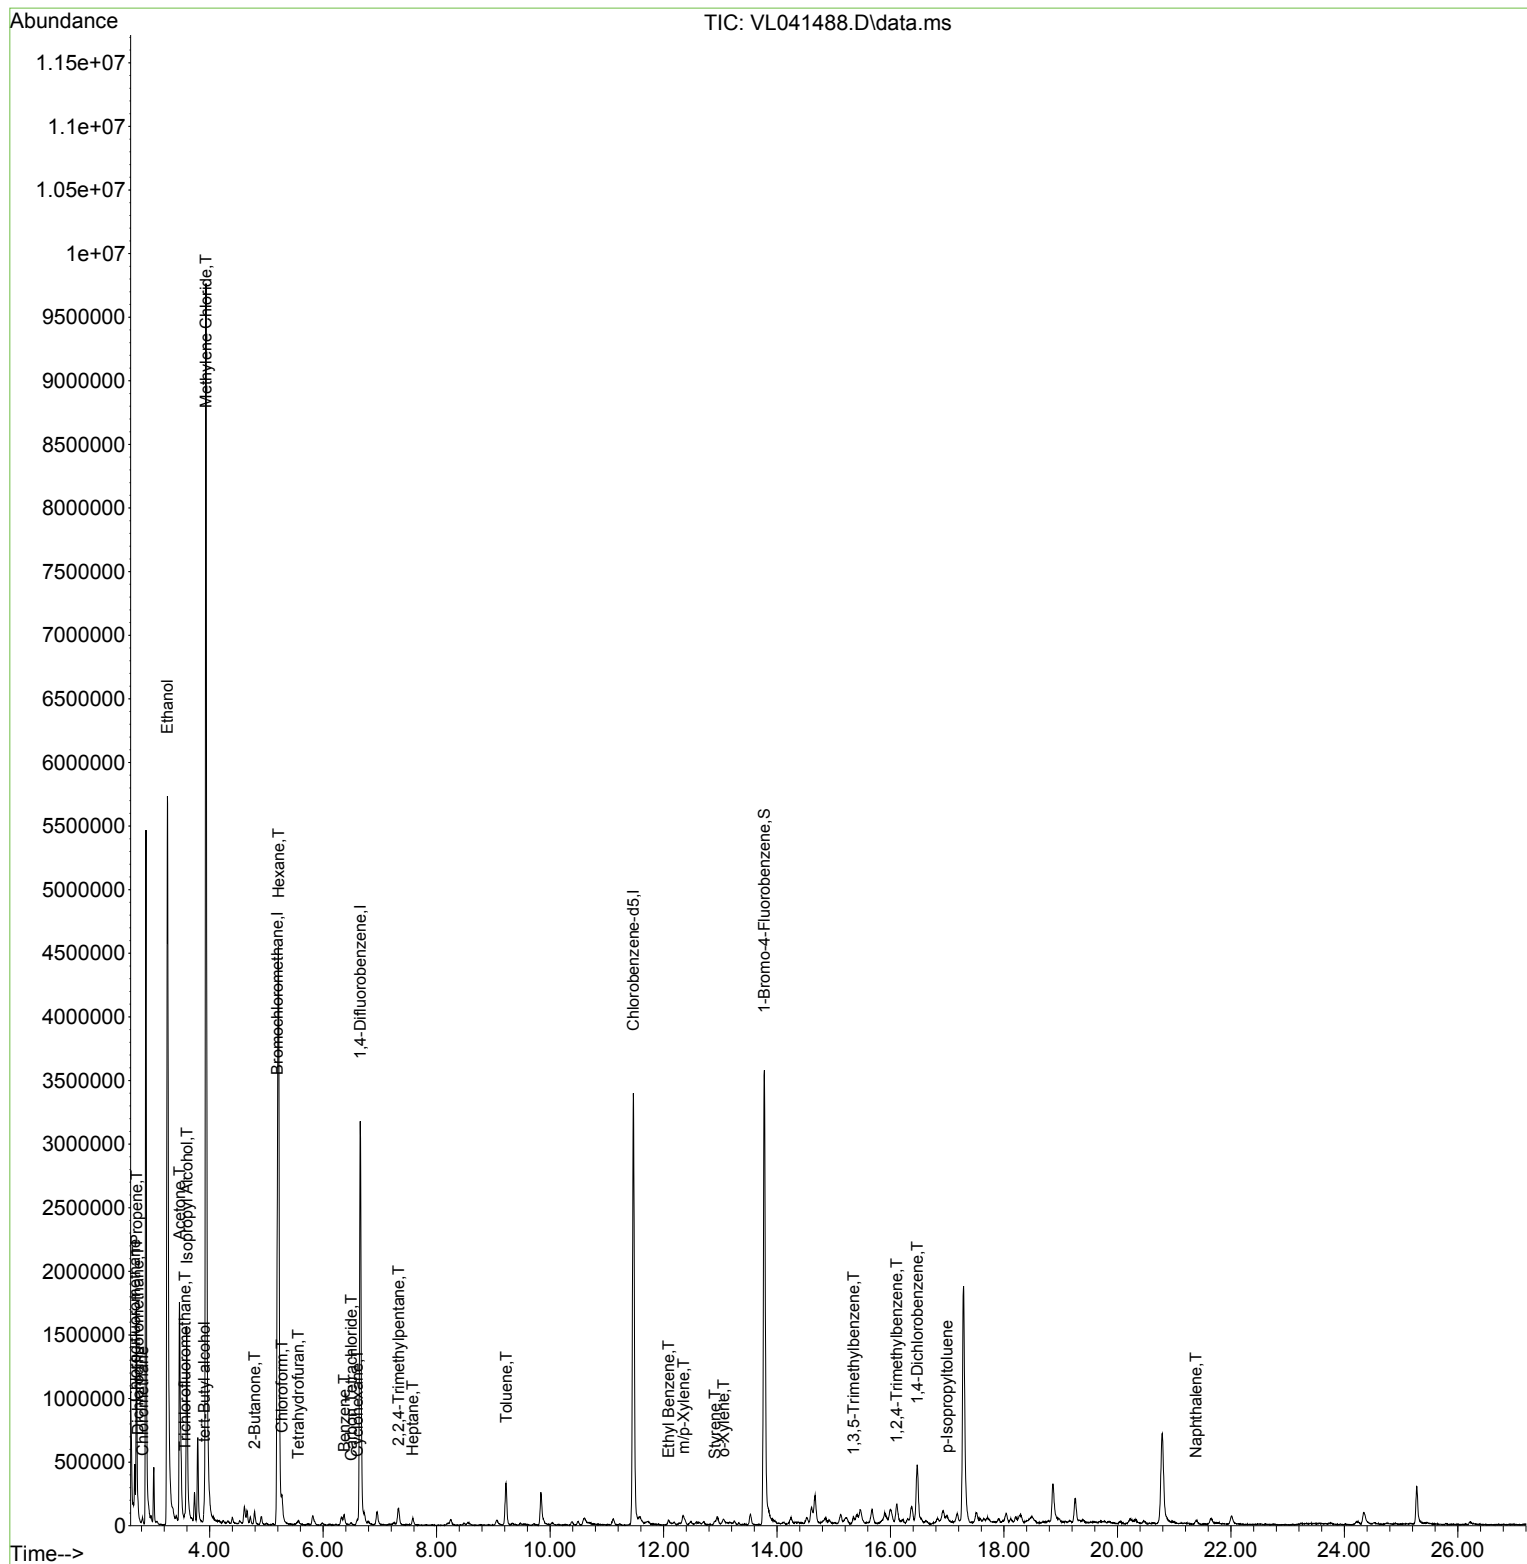



#1

Bromochloromethane

Concen: 10.000 ppbv

RT: 5.195 min Scan# 80

Delta R.T. 0.006 min

Lab File: VL041488.D


Acq: 1 Aug 2024 22:01

Instrument :

MSVOA_L

ClientSampleId :

3RD-FLOOR



Tgt Ion: 49 Resp: 926420

Ion Ratio Lower Upper

49 100

128 45.9 23.8 71.4




130 58.6 30.8 92.4

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 08/02/2024

Supervised By :Mahesh Dadoda 08/03/2024

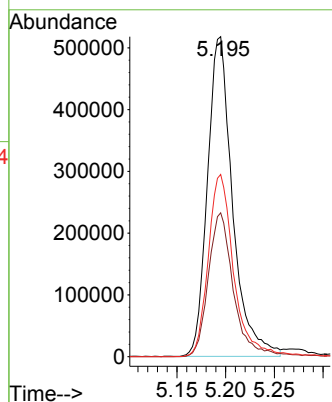

#2

Dichlorodifluoromethane

Concen: 0.312 ppbv m

RT: 2.735 min Scan# 41

Delta R.T. 0.006 min

Lab File: VL041488.D




Acq: 1 Aug 2024 22:01


Tgt Ion: 85 Resp: 49744

Ion Ratio Lower Upper

85 100


87 31.3 26.0 39.0

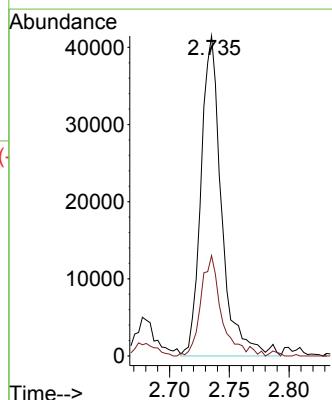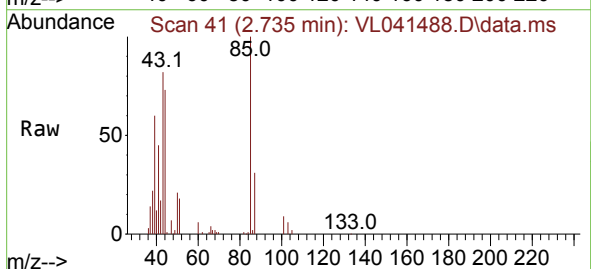

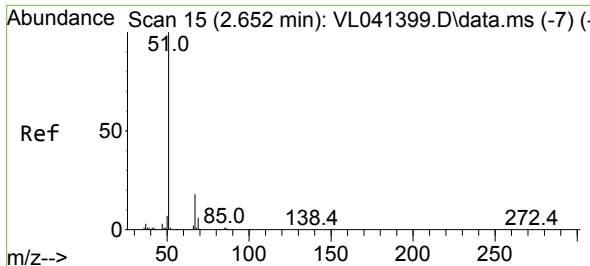

#3
Chlorodifluoromethane
Concen: 4.142 ppbv
RT: 2.677 min Scan# 21
Delta R.T. 0.003 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01




Instrument :
MSVOA_L
ClientSampleId :
3RD-FLOOR



Tgt Ion: 51 Resp: 456790
Ion Ratio Lower Upper
51 100
67 15.2 14.5 21.7




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/02/2024
Supervised By :Mahesh Dadoda 08/03/2024

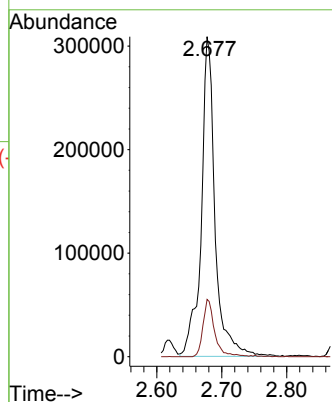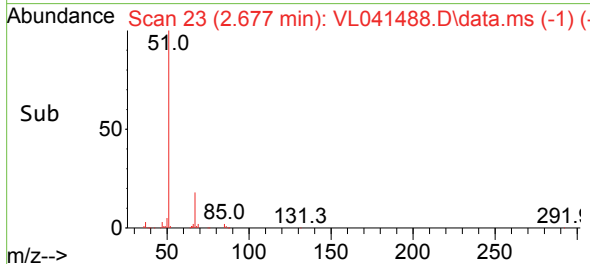

#4
Chloromethane
Concen: 0.706 ppbv
RT: 2.819 min Scan# 67
Delta R.T. 0.006 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01


Tgt Ion: 50 Resp: 41418
Ion Ratio Lower Upper
50 100
52 27.8 26.1 39.1

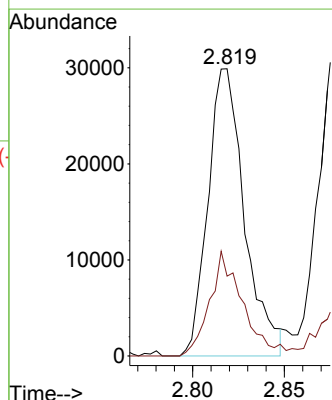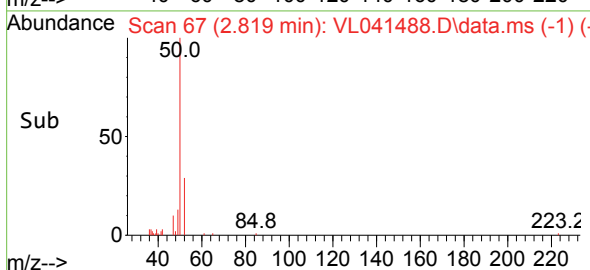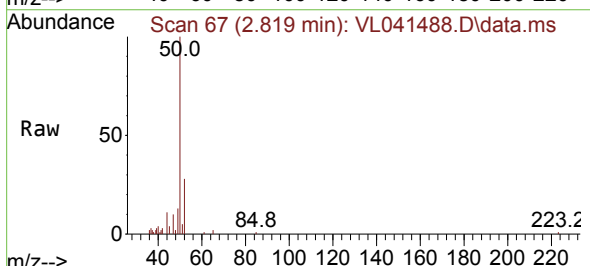

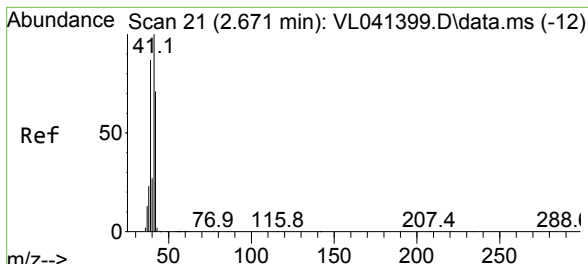

#9
 Propene
 Concen: 6.263 ppbv m
 RT: 2.709 min Scan# 31
 Delta R.T. 0.016 min
 Lab File: VL041488.D
 Acq: 1 Aug 2024 22:01




Instrument :
 MSVOA_L
 ClientSampleId :
 3RD-FLOOR

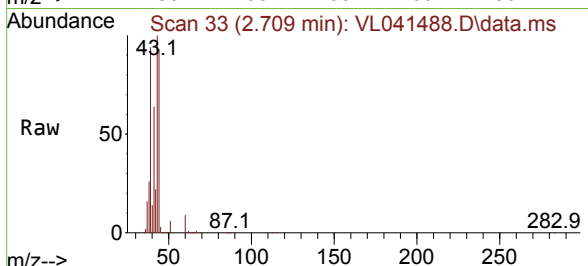


Tgt Ion: 41 Resp: 317300
 Ion Ratio Lower Upper
 41 100
 42 312.4 55.9 83.9

Manual Integrations
 APPROVED



Reviewed By :Semsettin Yesilyurt 08/02/2024
 Supervised By :Mahesh Dadoda 08/03/2024

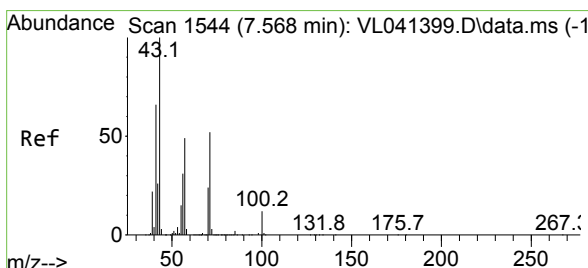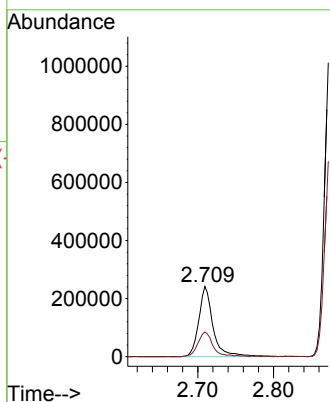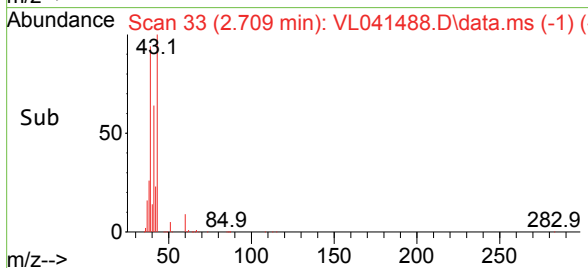


#10
 Heptane
 Concen: 0.154 ppbv
 RT: 7.581 min Scan# 1548
 Delta R.T. 0.003 min
 Lab File: VL041488.D
 Acq: 1 Aug 2024 22:01

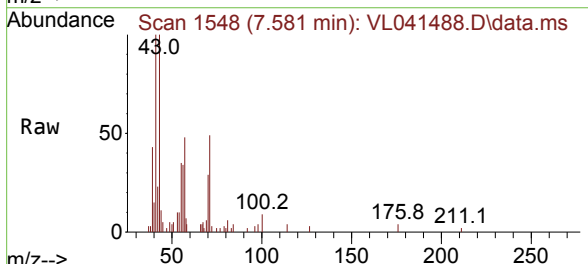


Tgt Ion: 43 Resp: 17509
 Ion Ratio Lower Upper
 43 100
 57 67.3 40.5 60.7

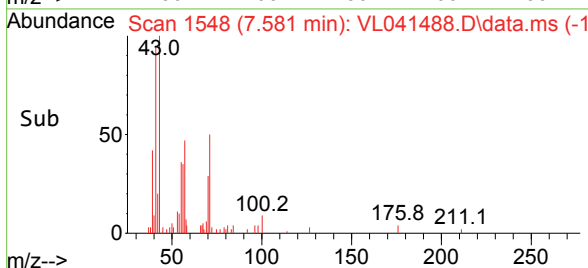



#11
Trichlorofluoromethane
Concen: 0.217 ppbv
RT: 3.565 min Scan# 203
Delta R.T. 0.003 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01




Instrument :
MSVOA_L
ClientSampleId :
3RD-FLOOR



Tgt Ion:101 Resp: 3078
Ion Ratio Lower Upper
101 100
103 59.4 52.6 79.0




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/02/2024
Supervised By :Mahesh Dadoda 08/03/2024

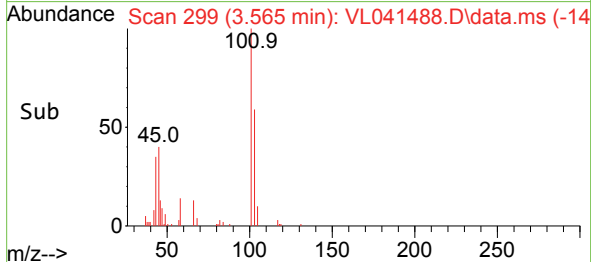

#13
Ethanol
Concen: 1371.689 ppbv
RT: 3.256 min Scan# 203
Delta R.T. 0.009 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01


Tgt Ion: 45 Resp: 6211199
Ion Ratio Lower Upper
45 100
46 35.7 13.4 53.4





#15
Acetone
Concen: 17.538 ppbv
RT: 3.468 min Scan# 20
Delta R.T. 0.003 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01




Instrument :
MSVOA_L
ClientSampleId :
3RD-FLOOR



Tgt Ion: 43 Resp: 1846064
Ion Ratio Lower Upper
43 100
58 26.2 21.4 32.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/02/2024
Supervised By :Mahesh Dadoda 08/03/2024

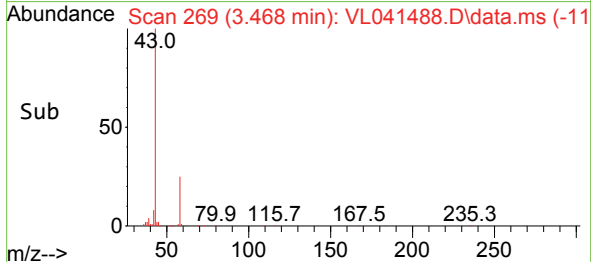

#17
tert-Butyl alcohol
Concen: 0.401 ppbv m
RT: 3.902 min Scan# 404
Delta R.T. 0.029 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01


Tgt Ion: 59 Resp: 38461
Ion Ratio Lower Upper
59 100
57 18.4 8.6 12.8#





#19
Isopropyl Alcohol
Concen: 26.044 ppbv
RT: 3.597 min Scan# 309
Delta R.T. 0.022 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01




Instrument :
MSVOA_L
ClientSampleId :
3RD-FLOOR




Tgt Ion: 45 Resp: 160268
Ion Ratio Lower Upper
45 100
58 2.3 1.9 2.9

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 08/02/2024
Supervised By :Mahesh Dadoda 08/03/2024




#20
Methylene Chloride
Concen: 85.409 ppbv
RT: 3.934 min Scan# 414
Delta R.T. 0.003 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01




Tgt Ion: 84 Resp: 3352491
Ion Ratio Lower Upper
84 100
49 149.1 126.6 190.0
51 51.3 38.6 58.0
86 65.8 53.0 79.4

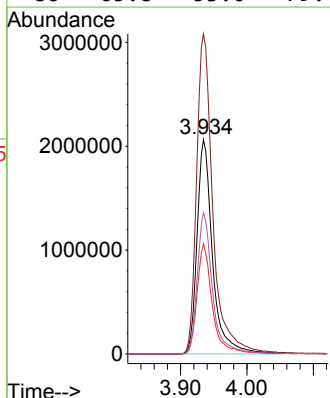



#26
Hexane
Concen: 18.523 ppbv
RT: 5.214 min Scan# 812
Delta R.T. 0.003 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01




Instrument :
MSVOA_L
ClientSampleId :
3RD-FLOOR

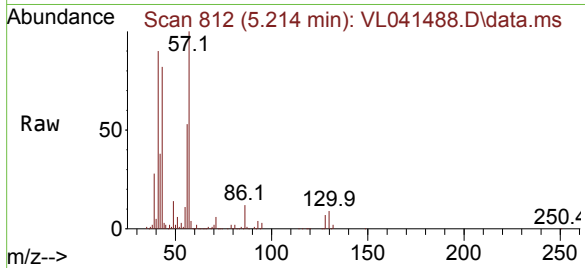

Tgt Ion: 57 Resp: 1606829
Ion Ratio Lower Upper
57 100
41 90.3 74.0 111.0
43 88.2 193.6 290.4
56 53.2 43.1 64.7




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/02/2024
Supervised By :Mahesh Dadoda 08/03/2024



#29
Chloroform
Concen: 0.665 ppbv
RT: 5.275 min Scan# 831
Delta R.T. 0.003 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01


Tgt Ion: 83 Resp: 94091
Ion Ratio Lower Upper
83 100
85 58.4 53.1 79.7

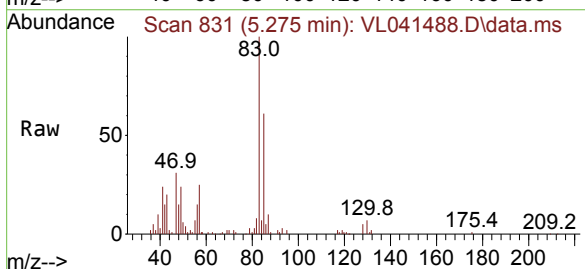



#30
Cyclohexane
Concen: 0.187 ppbv m
RT: 6.603 min Scan# 1240
Delta R.T. 0.006 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01




Instrument :
MSVOA_L
ClientSampleId :
3RD-FLOOR



Tgt Ion: 84 Resp: 13242
Ion Ratio Lower Upper
84 100
56 124.1 111.2 166.8
41 112.0 70.3 105.5




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/02/2024
Supervised By :Mahesh Dadoda 08/03/2024

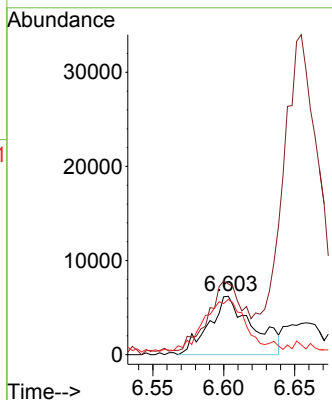

#33
1,4-Difluorobenzene
Concen: 10.000 ppbv
RT: 6.655 min Scan# 1260
Delta R.T. -0.000 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01


Tgt Ion:114 Resp: 2420057
Ion Ratio Lower Upper
114 100
63 25.1 20.3 30.5
88 17.8 14.3 21.5

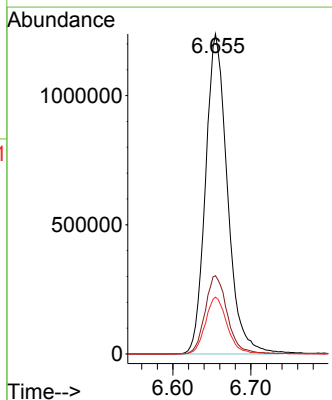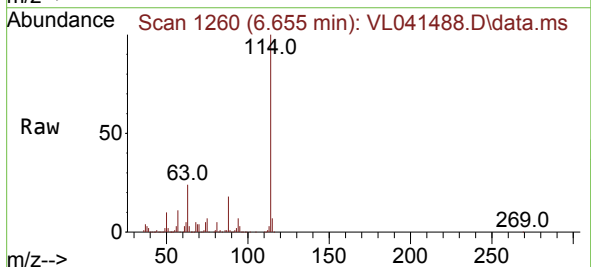



#34
2-Butanone
Concen: 0.951 ppbv
RT: 4.793 min Scan# 61
Delta R.T. 0.009 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01




Instrument :
MSVOA_L
ClientSampleId :
3RD-FLOOR



Tgt Ion: 43 Resp: 111354
Ion Ratio Lower Upper
43 100
72 24.0 17.3 25.9




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/02/2024
Supervised By :Mahesh Dadoda 08/03/2024

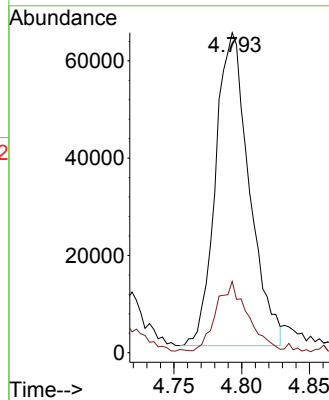

#35
Carbon Tetrachloride
Concen: 0.068 ppbv m
RT: 6.494 min Scan# 1210
Delta R.T. 0.003 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01


Tgt Ion:117 Resp: 9076
Ion Ratio Lower Upper
117 100
119 77.1 76.6 115.0
121 31.5 25.1 37.7

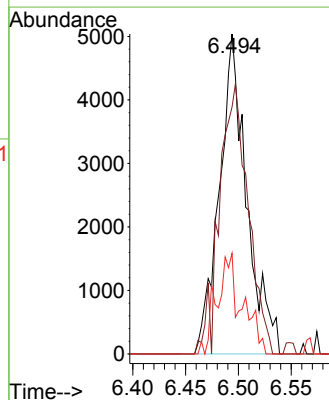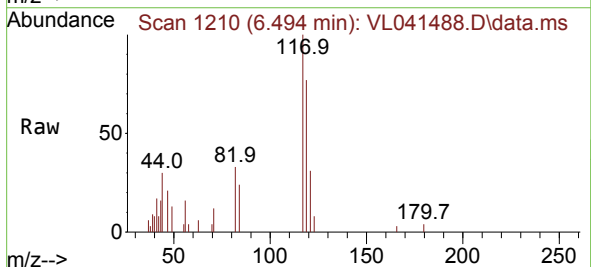



#36
Benzene
Concen: 0.313 ppbv
RT: 6.372 min Scan# 1168
Delta R.T. 0.003 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01




Instrument :
MSVOA_L
ClientSampleId :
3RD-FLOOR



Tgt Ion: 78 Resp: 5533
Ion Ratio Lower Upper
78 100
77 21.4 18.1 27.1
50 16.2 15.5 23.3




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/02/2024
Supervised By :Mahesh Dadoda 08/03/2024

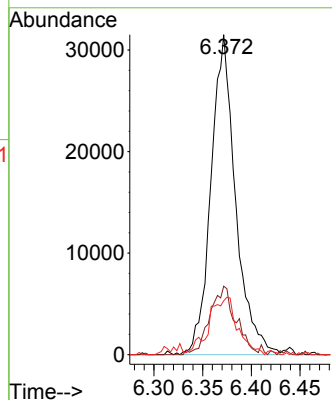

#41
Tetrahydrofuran
Concen: 0.286 ppbv m
RT: 5.565 min Scan# 921
Delta R.T. 0.013 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01


Tgt Ion: 42 Resp: 19120
Ion Ratio Lower Upper
42 100
72 26.0 31.2 46.8#
71 21.6 30.5 45.7#

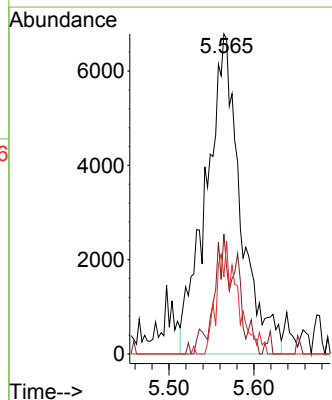



#44
2,2,4-Trimethylpentane
Concen: 0.375 ppbv m
RT: 7.330 min Scan# 1466
Delta R.T. 0.006 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01




Instrument :
MSVOA_L
ClientSampleId :
3RD-FLOOR



Tgt Ion: 57 Resp: 110780
Ion Ratio Lower Upper
57 100
41 43.7 27.0 40.6
56 38.5 25.2 37.8




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/02/2024
Supervised By :Mahesh Dadoda 08/03/2024

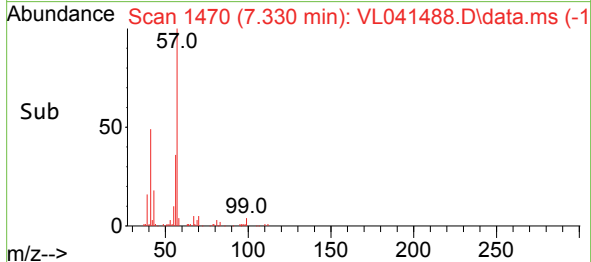

#53
Toluene
Concen: 1.097 ppbv
RT: 9.227 min Scan# 2060
Delta R.T. 0.006 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01


Tgt Ion: 91 Resp: 216118
Ion Ratio Lower Upper
91 100
92 61.0 48.7 73.1

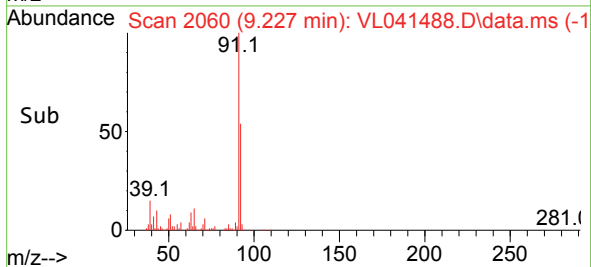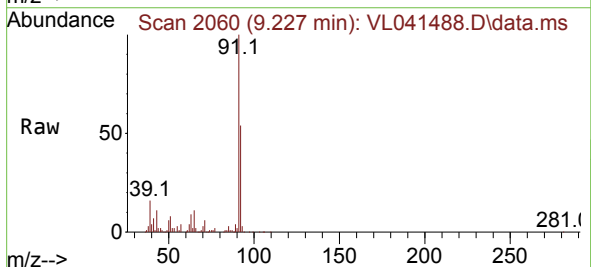



#55
Chlorobenzene-d5
Concen: 10.000 ppbv
RT: 11.468 min Scan# 21
Delta R.T. 0.003 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01




Instrument :
MSVOA_L
ClientSampleId :
3RD-FLOOR




Tgt Ion:117 Resp: 2240524
Ion Ratio Lower Upper
117 100
82 63.7 51.0 76.6
119 32.9 45.2 67.8

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 08/02/2024
Supervised By :Mahesh Dadoda 08/03/2024

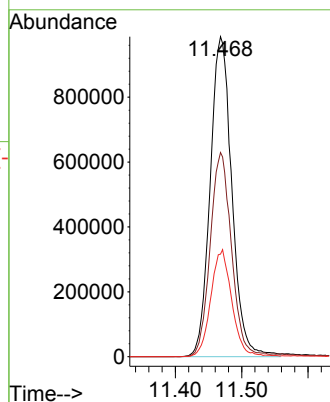


#58
Ethyl Benzene
Concen: 0.113 ppbv m
RT: 12.088 min Scan# 2950
Delta R.T. 0.003 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01




Tgt Ion: 91 Resp: 29086
Ion Ratio Lower Upper
91 100
106 26.0 25.8 38.8





#59
m/p-Xylene
Concen: 0.326 ppbv m
RT: 12.352 min Scan# 3032
Delta R.T. -0.016 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01




Instrument :
MSVOA_L
ClientSampleId :
3RD-FLOOR




Tgt Ion: 91 Resp: 72758
Ion Ratio Lower Upper
91 100
106 0.0 36.3 54.5

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 08/02/2024
Supervised By :Mahesh Dadoda 08/03/2024

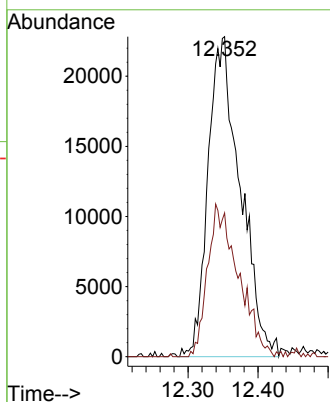


#60
o-Xylene
Concen: 0.152 ppbv m
RT: 13.056 min Scan# 3251
Delta R.T. -0.000 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01



Tgt Ion: 91 Resp: 32129
Ion Ratio Lower Upper
91 100
106 44.6 23.1 69.3



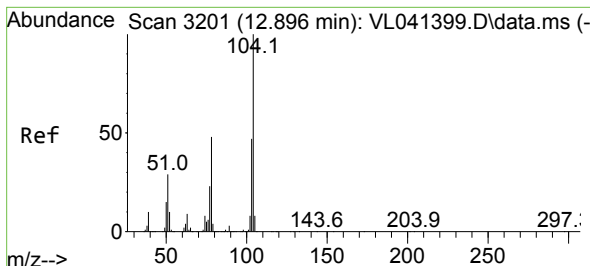

#61

Styrene

Concen: 0.108 ppbv m

RT: 12.905 min Scan# 3201

Delta R.T. 0.009 min

Lab File: VL041488.D


Acq: 1 Aug 2024 22:01

Instrument :

MSVOA_L

ClientSampleId :

3RD-FLOOR






Tgt Ion	Ratio	Lower	Upper
104	100		
78	61.4	40.8	61.2
103	49.5	38.2	57.4

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 08/02/2024
Supervised By :Mahesh Dadoda 08/03/2024

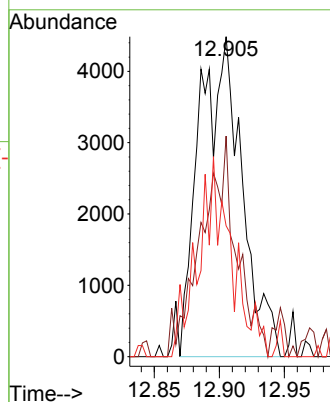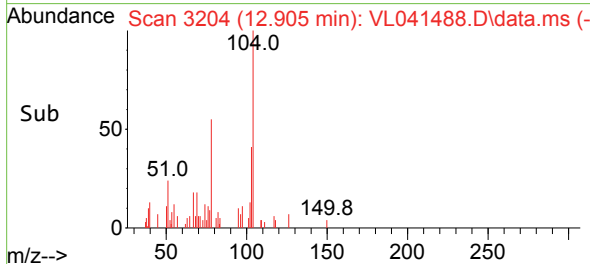

#68

1-Bromo-4-Fluorobenzene

Concen: 10.083 ppbv




RT: 13.773 min Scan# 3474


Delta R.T. -0.000 min

Lab File: VL041488.D

Acq: 1 Aug 2024 22:01


Tgt Ion	Ratio	Lower	Upper
95	100		
174	71.2	56.3	84.5
175	5.4	4.0	6.0

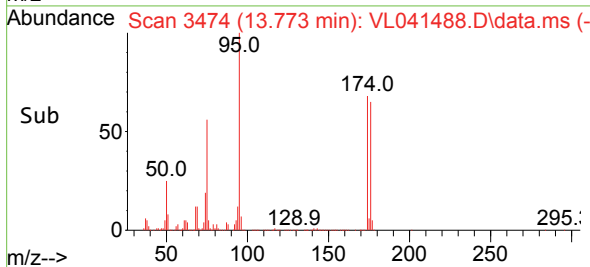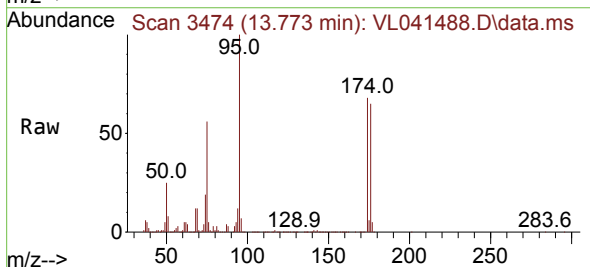



#69
p-Isopropyltoluene
Concen: 0.105 ppbv m
RT: 16.995 min Scan# 4476
Delta R.T. 0.003 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01




Instrument :
MSVOA_L
ClientSampleId :
3RD-FLOOR




Tgt Ion:119 Resp: 34809
Ion Ratio Lower Upper
119 100
134 28.9 20.5 30.7
91 34.3 23.2 34.8

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 08/02/2024
Supervised By :Mahesh Dadoda 08/03/2024

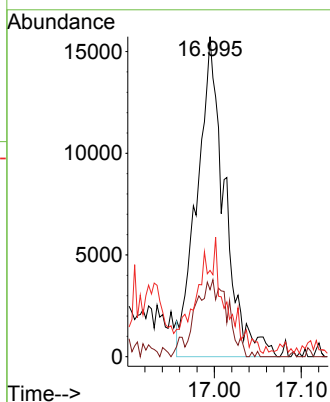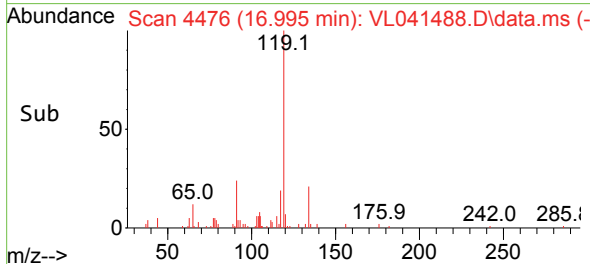


#73
1,3,5-Trimethylbenzene
Concen: 0.141 ppbv m
RT: 15.352 min Scan# 3965
Delta R.T. 0.003 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01

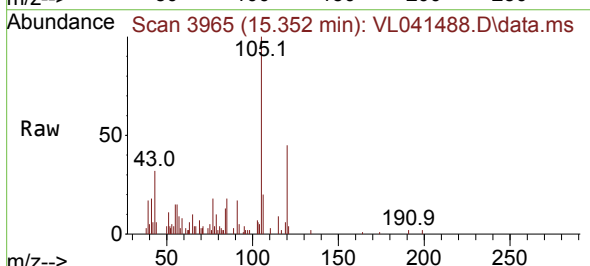


Tgt Ion:105 Resp: 30105
Ion Ratio Lower Upper
105 100
120 45.3 38.6 57.8

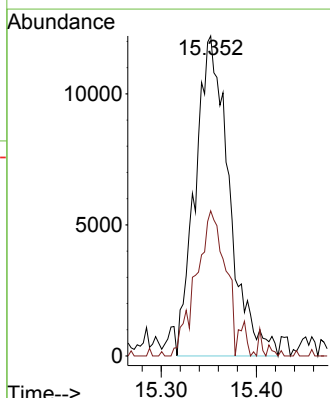



#74
1,2,4-Trimethylbenzene
Concen: 0.369 ppbv
RT: 16.108 min Scan# 4199
Delta R.T. -0.000 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01




Instrument :
MSVOA_L
ClientSampleId :
3RD-FLOOR

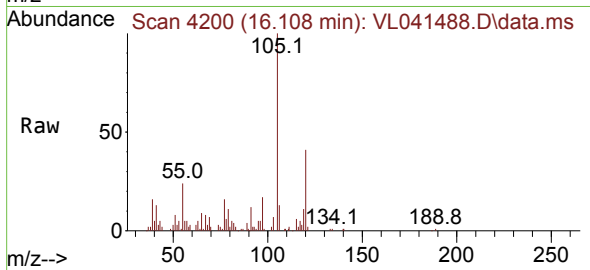

Tgt Ion:105 Resp: 9177
Ion Ratio Lower Upper
105 100
120 41.2 39.5 59.3
91 11.2 39.8 59.8
77 15.2 18.2 27.4#




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/02/2024
Supervised By :Mahesh Dadoda 08/03/2024

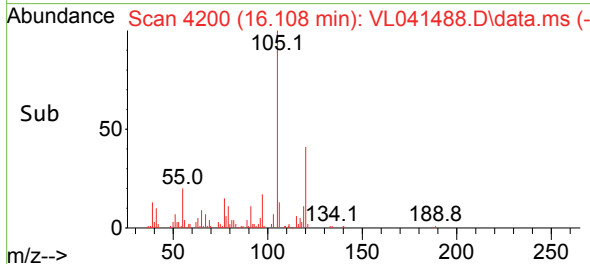

#76
1,4-Dichlorobenzene
Concen: 0.261 ppbv m
RT: 16.474 min Scan# 4314
Delta R.T. 0.003 min
Lab File: VL041488.D
Acq: 1 Aug 2024 22:01

Tgt Ion:146 Resp: 39484
Ion Ratio Lower Upper
146 100
111 0.0 22.4 67.0#
148 0.0 33.1 99.5#

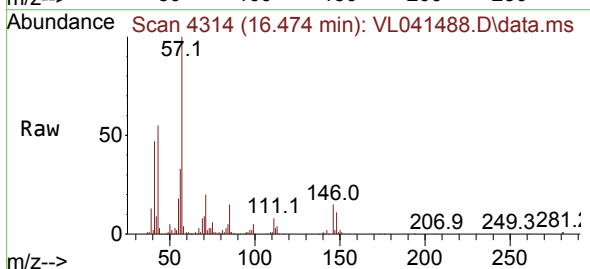

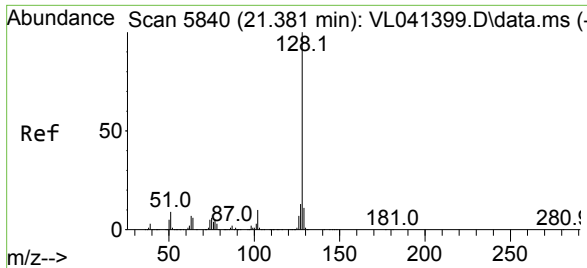

#79

Naphthalene

Concen: 0.156 ppbv m

RT: 21.384 min Scan# 5840

Delta R.T. 0.003 min

Lab File: VL041488.D


Acq: 1 Aug 2024 22:01

Instrument :

MSVOA_L

ClientSampleId :

3RD-FLOOR

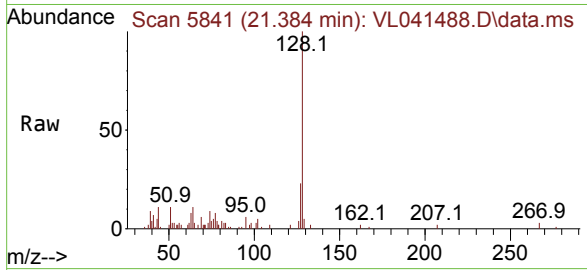

Tgt Ion:128 Resp: 34229

Ion Ratio Lower Upper

128 100

127 22.9 10.3 15.5

129 5.0 9.0 13.4

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 08/02/2024

Supervised By :Mahesh Dadoda 08/03/2024

