


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL080124\
Data File : VL041468.D
Acq On : 1 Aug 2024 7:47
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072524AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Aug 02 03:13:29 2024

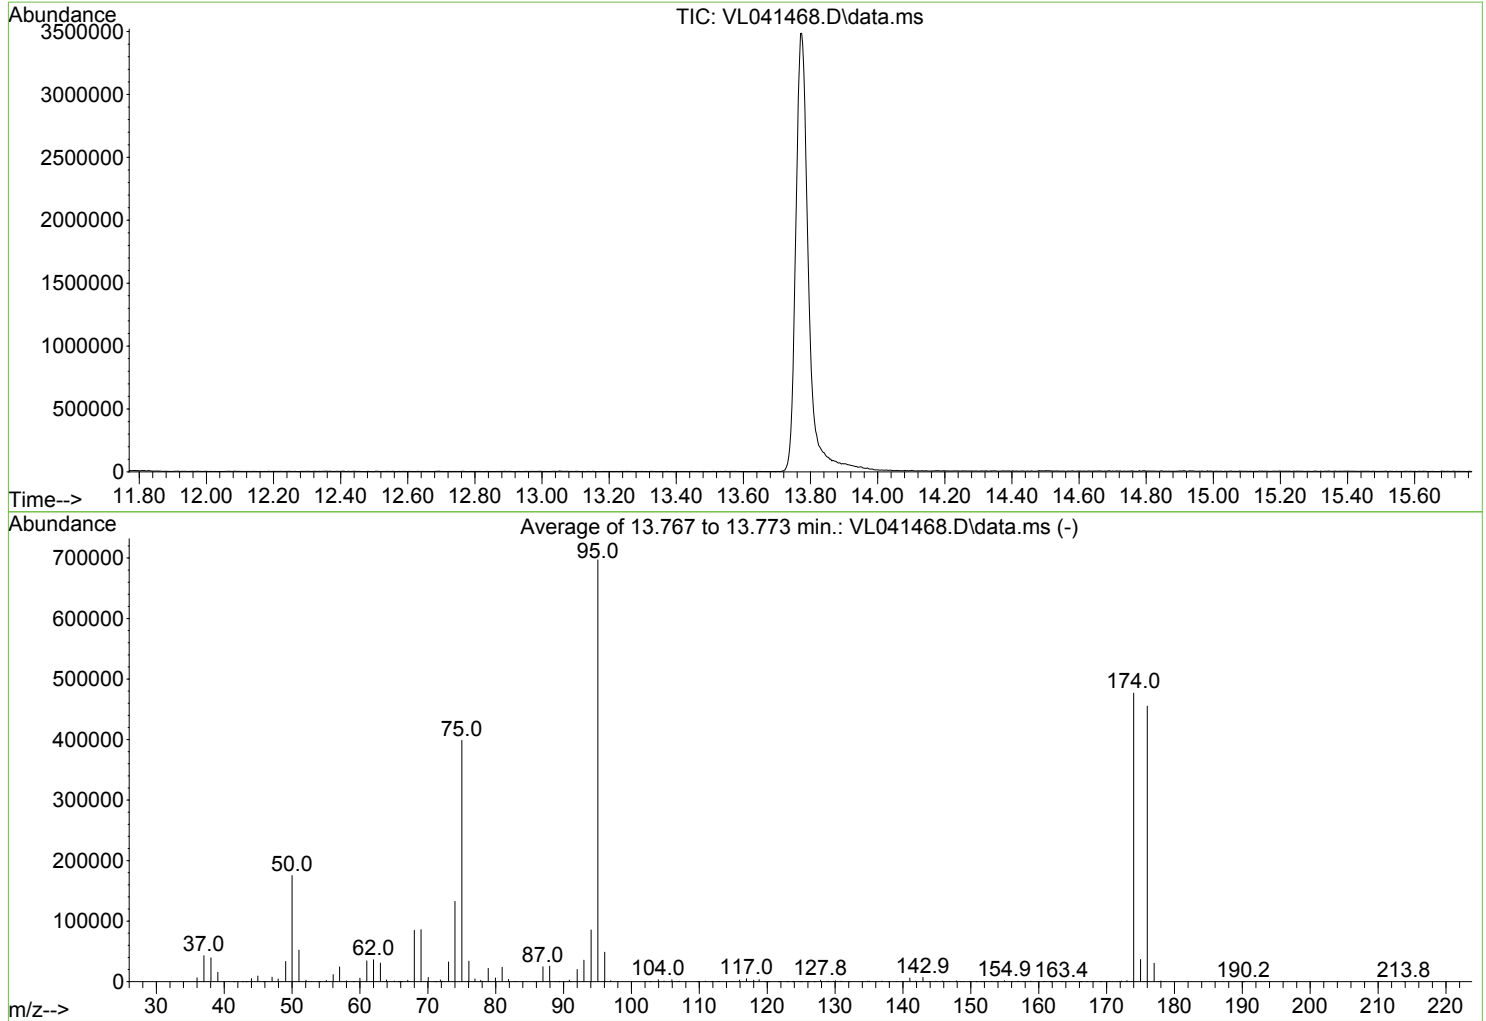

AutoFind: Scans 3472, 3473, 3474; Background Corrected with Scan 3444

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	25.2	175339	PASS
75	95	30	66	57.2	398677	PASS
95	95	100	100	100.0	696981	PASS
96	95	5	9	7.0	48744	PASS
173	174	0.00	2	0.4	1757	PASS
174	95	50	120	68.4	476779	PASS
175	174	4	9	7.6	36464	PASS
176	174	93	101	95.5	455189	PASS
177	176	5	9	6.7	30317	PASS

Average of 13.767 to 13.773 min.: VL041468.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	6444	46.05	491	56.05	11741	65.90	61
37.00	42941	47.05	7413	57.00	24355	66.10	11
38.05	39320	47.95	4573	58.00	1452	67.05	235
39.05	15681	49.05	33365	59.05	123	68.00	8495
40.00	219	50.00	175339	60.00	5790	69.00	85853
41.40	79	51.00	52155	61.00	34352	70.05	6917
42.70	80	52.05	2394	62.00	36203	70.95	311
43.20	138	52.85	351	63.00	30749	71.20	81
44.00	5182	53.90	182	63.90	2901	71.85	3028
44.95	9271	54.10	90	65.05	1031	72.10	954
45.80	118	55.05	2026	65.70	101	73.05	32525

Average of 13.767 to 13.773 min.: VL041468.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
74.00	132707	83.10	377	93.00	35413	109.70	384
75.00	398677	83.90	146	94.05	85429	109.90	84
76.05	33901	85.70	318	95.05	696981	110.90	850
76.95	4591	86.00	522	96.05	48744	111.80	288
77.80	2105	86.95	24621	96.95	1580	111.95	610
78.10	922	87.95	25296	102.75	159	112.80	166
78.90	21848	88.80	182	103.95	3308	112.95	350
79.95	6169	89.30	81	104.80	1001	114.75	363
80.95	23845	90.85	2611	105.95	3237	115.10	242
81.90	3678	91.10	651	106.80	197	115.90	2655
82.75	456	92.00	20109	107.05	767	116.95	4910

Average of 13.767 to 13.773 min.: VL041468.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.00	2470	125.10	103	132.10	72	141.85	929
118.80	3393	125.70	230	133.80	160	142.95	7089
119.70	88	126.10	99	134.00	63	143.90	287
120.00	134	126.90	58	134.80	925	144.10	190
120.20	98	127.85	2357	135.05	696	144.85	821
121.70	74	128.70	322	135.90	180	145.85	1089
122.80	160	129.00	958	136.90	1011	146.80	454
123.00	159	129.80	844	137.80	52	147.90	1312
123.70	93	130.05	1651	139.05	281	148.50	197
123.90	459	130.85	849	140.00	540	148.95	371
124.80	64	131.10	336	141.00	6166	149.80	516

Average of 13.767 to 13.773 min.: VL041468.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
150.00	165	159.90	98	170.90	163	190.00	73
150.80	56	160.70	176	171.50	370	190.20	89
151.50	116	160.90	628	171.90	498	213.80	69
151.90	260	161.70	71	172.20	1116		
153.10	447	161.90	76	173.00	1757		
153.85	479	163.40	128	174.00	476779		
154.95	1505	166.20	112	175.00	36464		
156.00	78	167.10	160	176.00	455189		
156.95	931	169.10	71	177.00	30317		
157.75	340	169.90	85	177.70	294		
158.85	795	170.45	206	178.00	997		