


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL080421\
 Data File : VL037312.D
 Acq On : 4 Aug 2021 16:46
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL080421AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Aug 04 22:53:01 2021
 Last Update : Wed Aug 04 22:53:01 2021

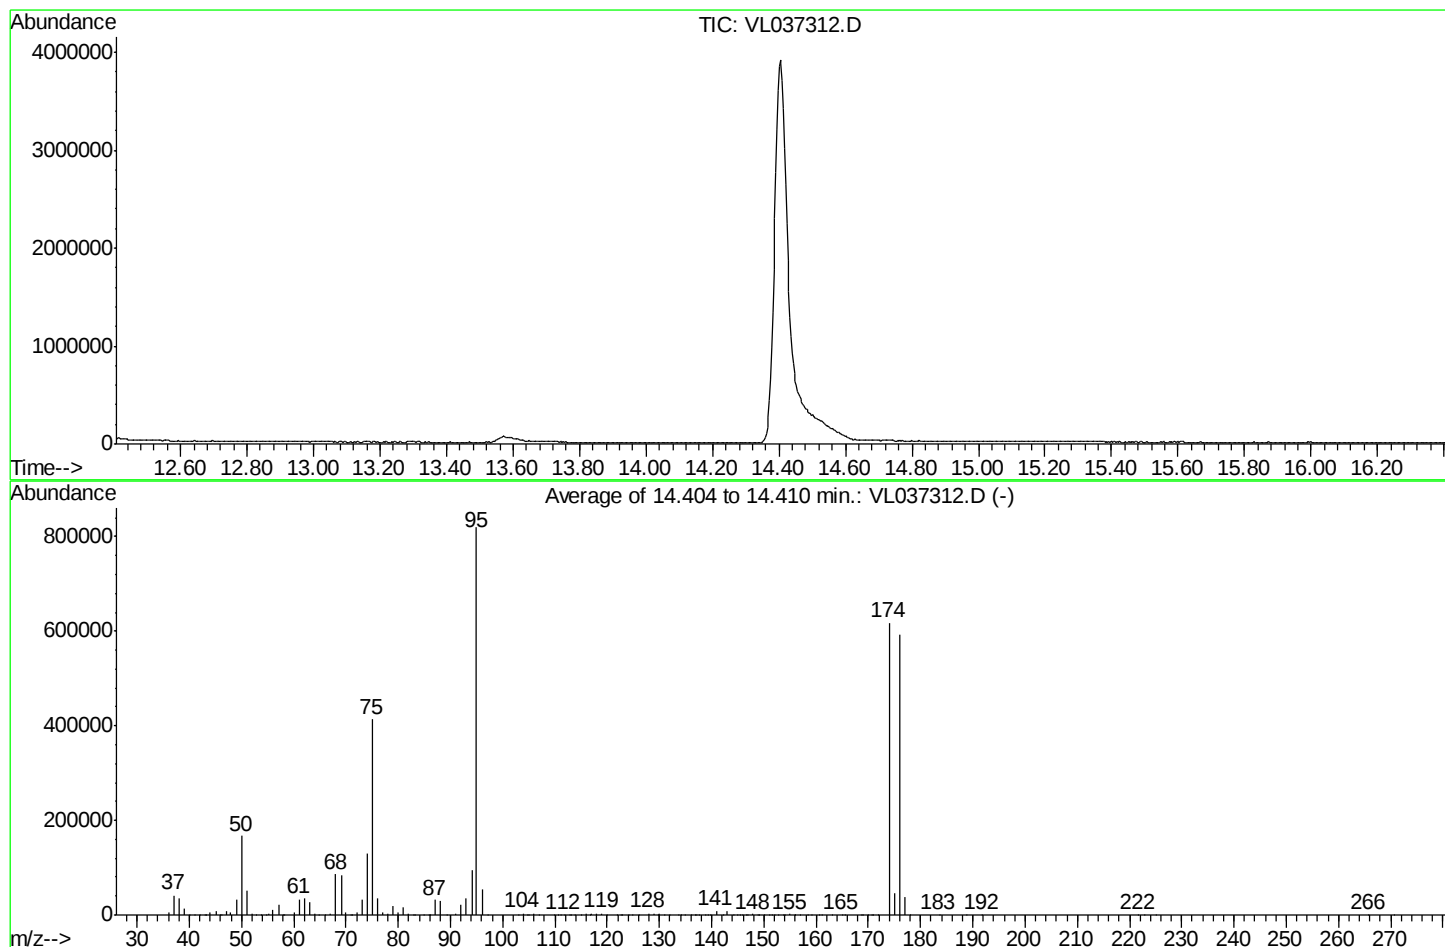

AutoFind: Scans 3613, 3614, 3615; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	20.5	167765	PASS
75	95	30	66	50.5	413932	PASS
95	95	100	100	100.0	819520	PASS
96	95	5	9	6.5	53440	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.4	618176	PASS
175	174	4	9	7.6	46901	PASS
176	174	93	101	96.0	593194	PASS
177	176	5	9	6.5	38768	PASS