


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL080519\
 Data File : VL034085.D
 Acq On : 5 Aug 2019 12:04
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL080519AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 02 09:11:40 2019
 Last Update : Fri Aug 02 09:11:40 2019

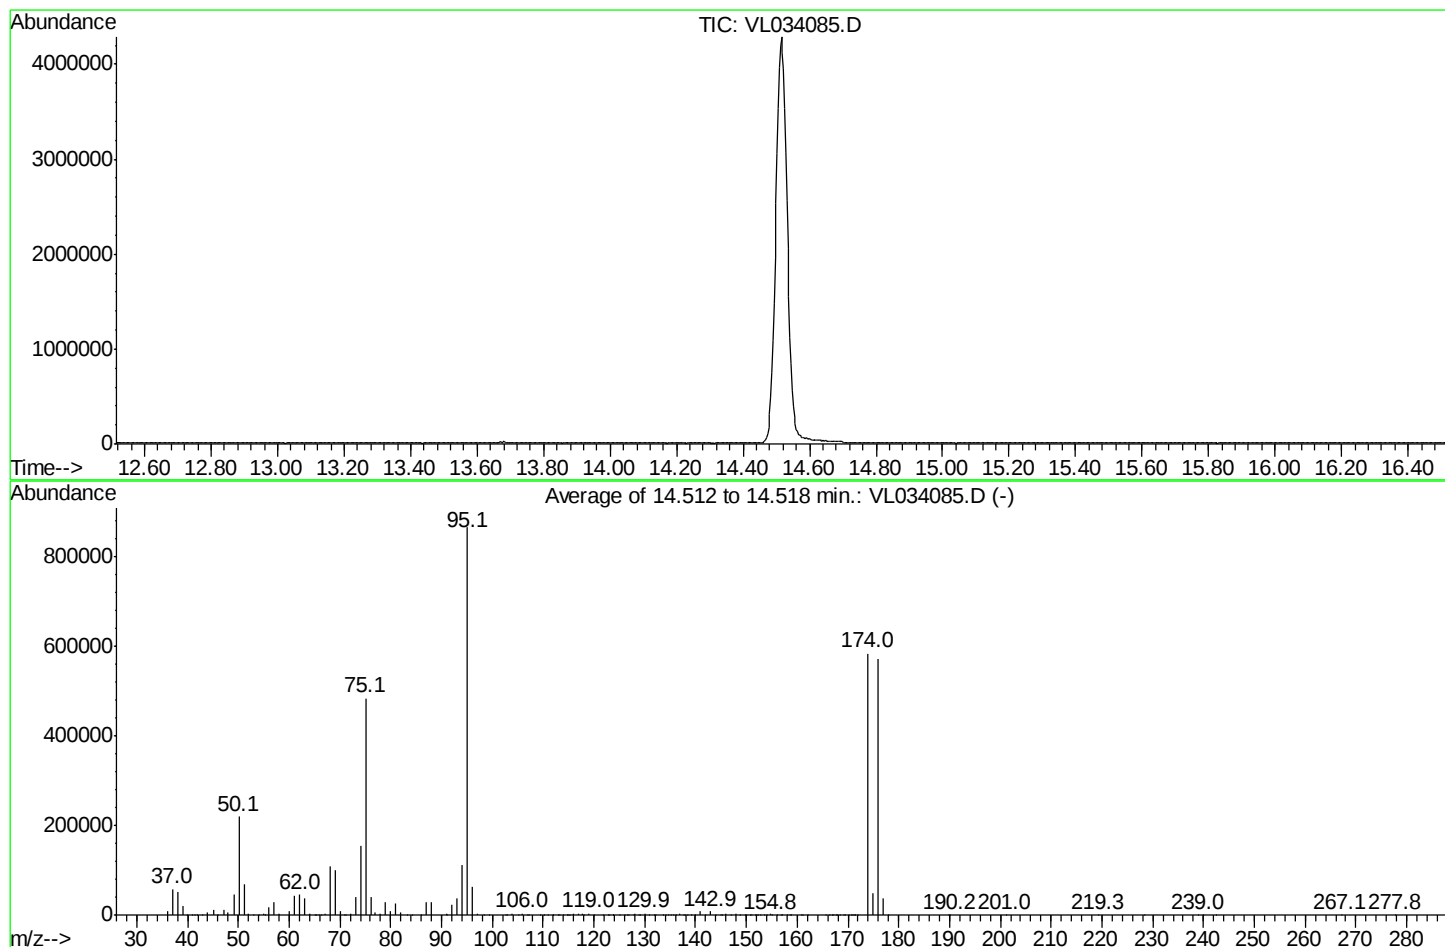

AutoFind: Scans 3600, 3601, 3602; Background Corrected with Scan 3576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.4	219840	PASS
75	95	30	66	55.9	483840	PASS
95	95	100	100	100.0	865066	PASS
96	95	5	9	7.4	63637	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.5	584021	PASS
175	174	4	9	8.5	49677	PASS
176	174	93	101	98.0	572138	PASS
177	176	5	9	6.5	37272	PASS