


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL080520\
 Data File : VL035332.D
 Acq On : 5 Aug 2020 8:01
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL080520AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Tue Aug 04 12:30:41 2020
 Last Update : Tue Aug 04 12:30:41 2020

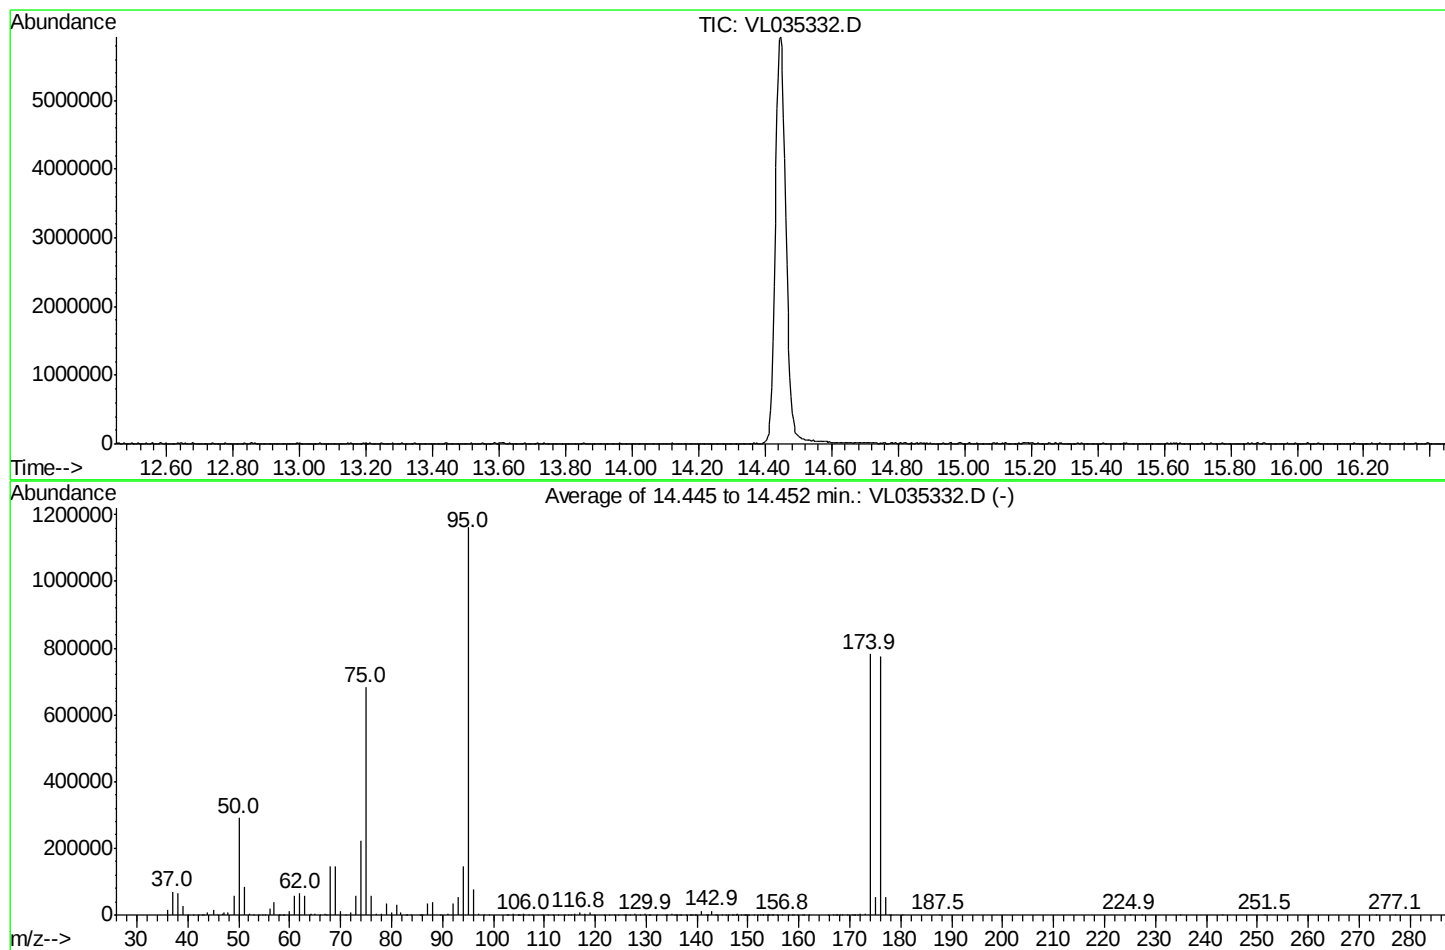

AutoFind: Scans 3626, 3627, 3628; Background Corrected with Scan 3603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.1	291456	PASS
75	95	30	66	58.6	681621	PASS
95	95	100	100	100.0	1162410	PASS
96	95	5	9	6.5	76117	PASS
173	174	0.00	2	0.7	5356	PASS
174	95	50	120	67.3	782485	PASS
175	174	4	9	7.0	55120	PASS
176	174	93	101	99.2	776106	PASS
177	176	5	9	6.7	52325	PASS