


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL080620\
 Data File : VL035341.D
 Acq On : 6 Aug 2020 7:12
 Operator : SY/AP
 Sample : BFB
 Misc : 400ml/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL080520AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Aug 05 13:04:46 2020
 Last Update : Wed Aug 05 13:04:46 2020

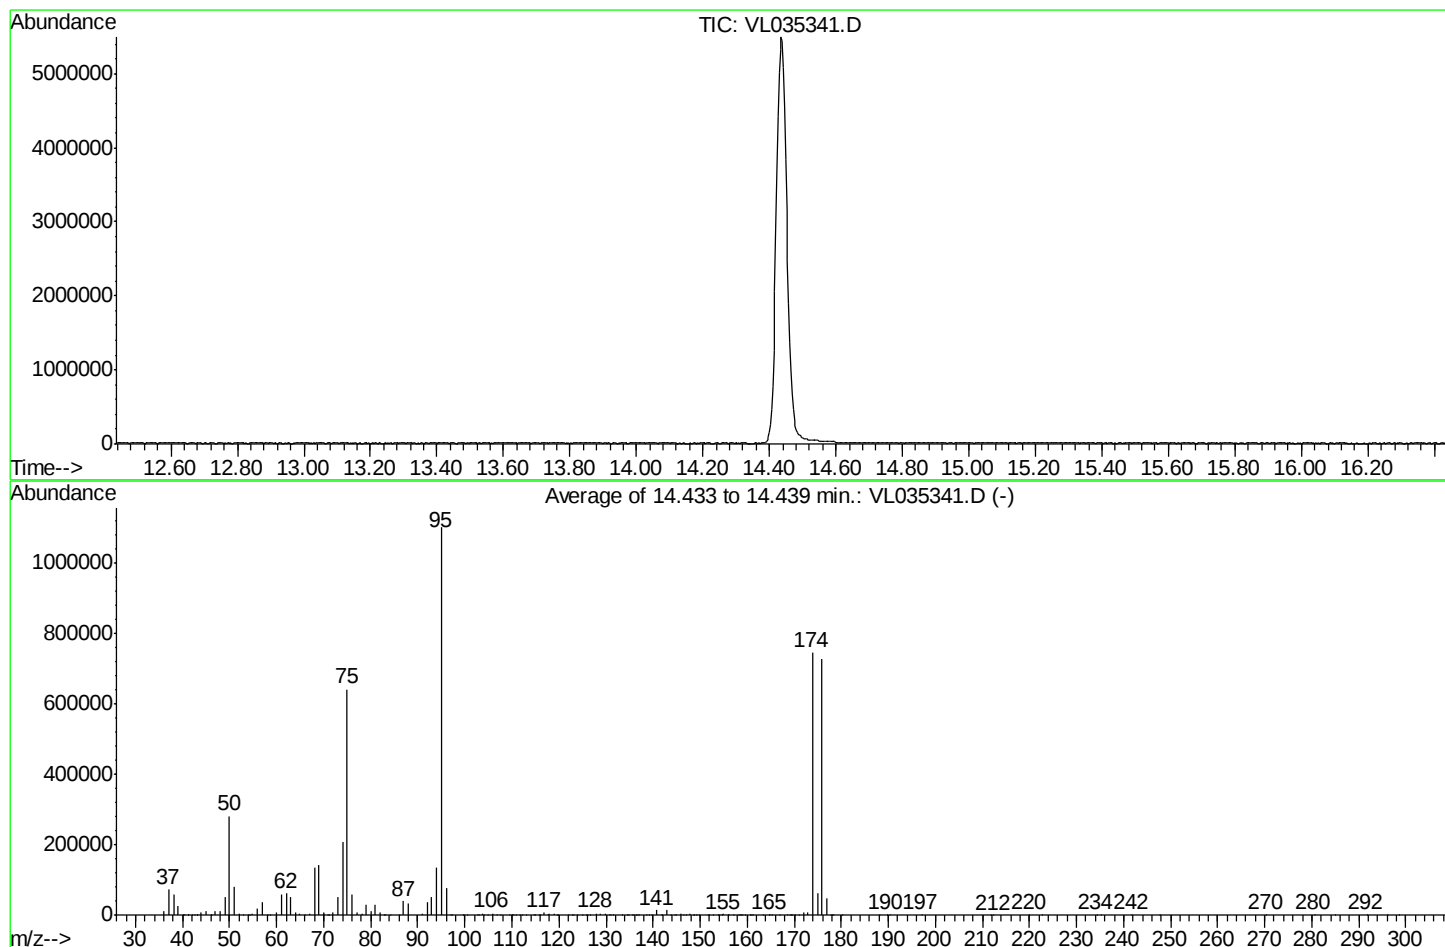

AutoFind: Scans 3622, 3623, 3624; Background Corrected with Scan 3594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.4	280192	PASS
75	95	30	66	58.3	641984	PASS
95	95	100	100	100.0	1101824	PASS
96	95	5	9	7.0	77509	PASS
173	174	0.00	2	0.8	5710	PASS
174	95	50	120	67.6	744661	PASS
175	174	4	9	8.2	61005	PASS
176	174	93	101	97.5	726165	PASS
177	176	5	9	6.8	49085	PASS