


Data Path : Z:\voasrv\HPCHEM1\MSVOA L\Data\VL080621\
 Data File : VL037340.D
 Acq On : 6 Aug 2021 11:19
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL080621AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 06 17:52:04 2021
 Last Update : Fri Aug 06 17:52:04 2021

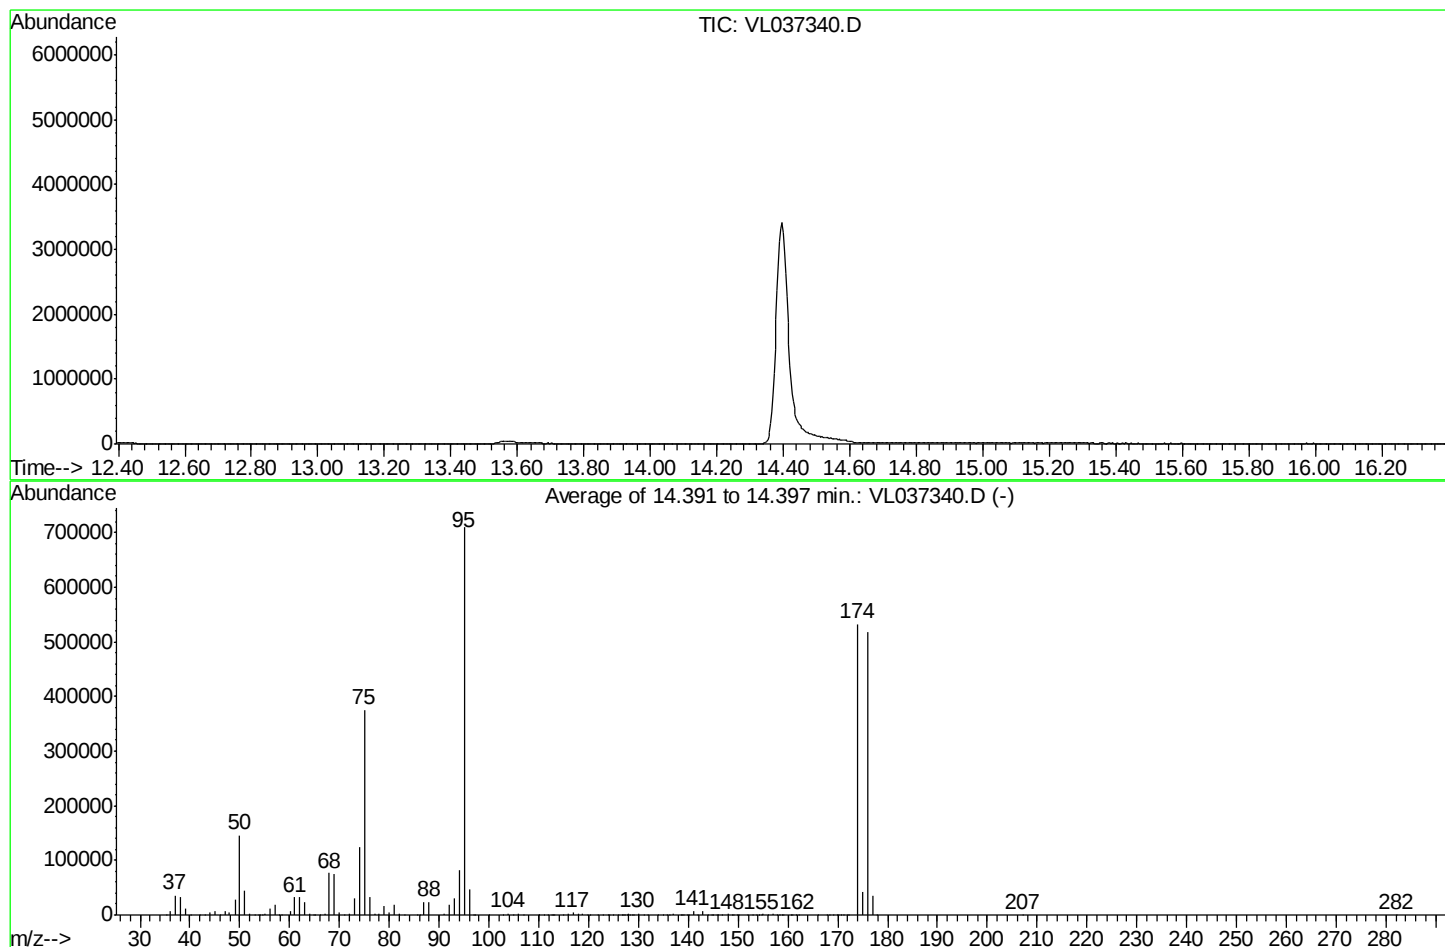

AutoFind: Scans 3609, 3610, 3611; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	20.6	145877	PASS
75	95	30	66	52.9	375552	PASS
95	95	100	100	100.0	709717	PASS
96	95	5	9	6.6	47053	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.0	532480	PASS
175	174	4	9	7.7	41181	PASS
176	174	93	101	97.1	517248	PASS
177	176	5	9	6.8	35042	PASS