
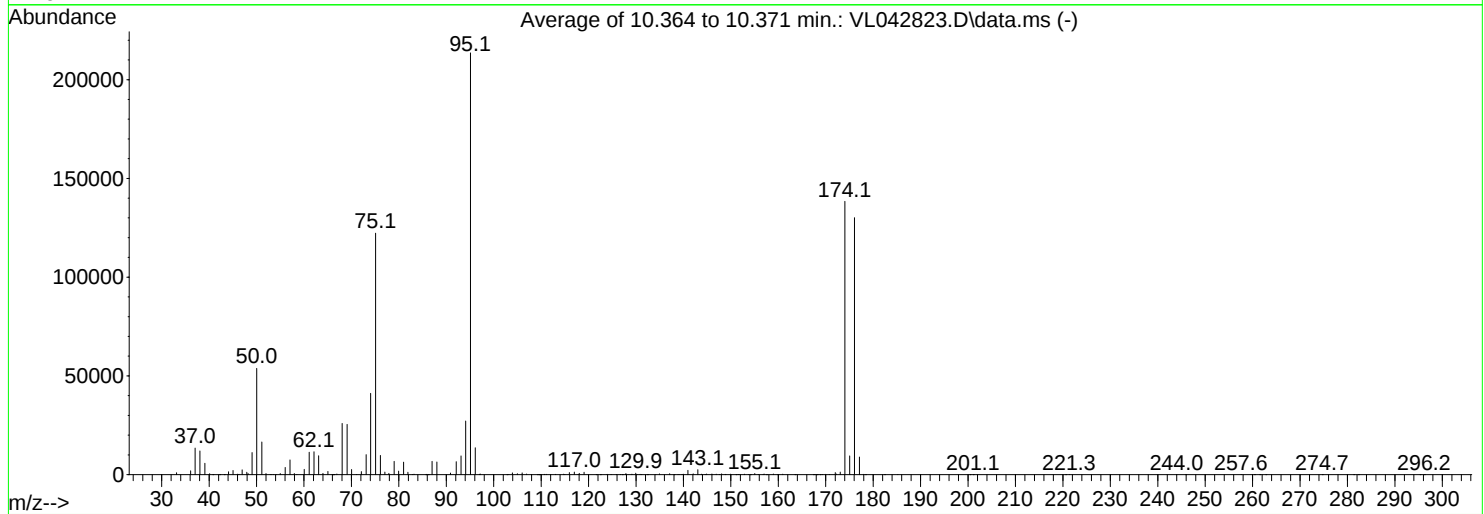


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL080725\
Data File : VL042823.D
Acq On : 07 Aug 2025 07:42
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072325AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Jul 24 05:24:41 2025

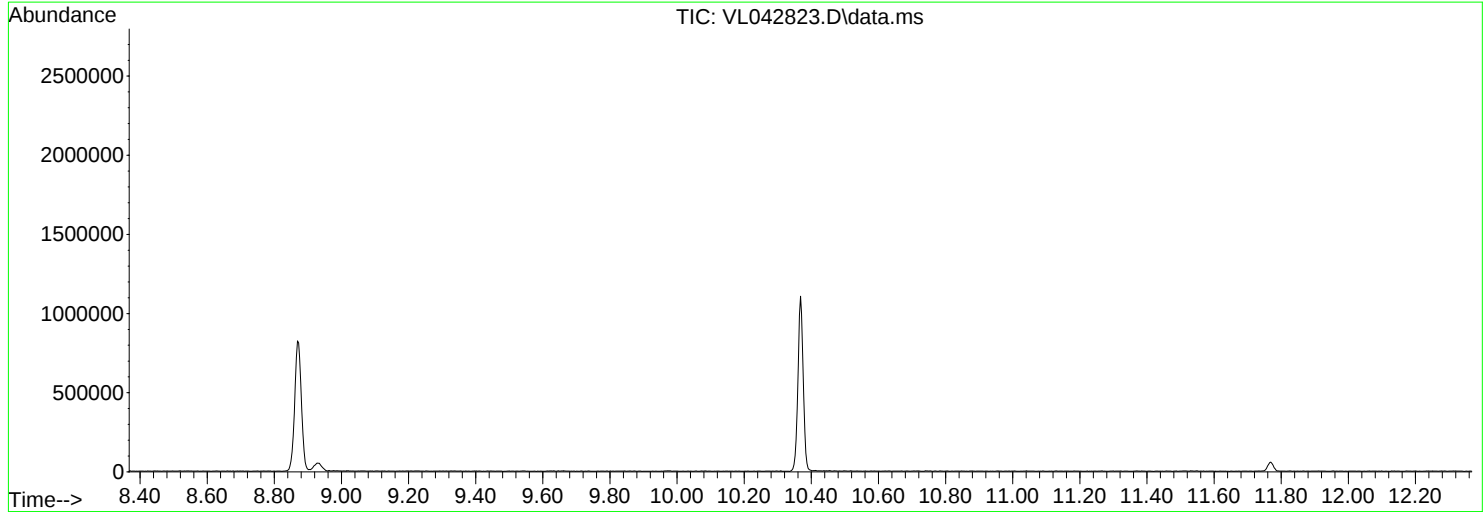

AutoFind: Scans 3175, 3176, 3177; Background Corrected with Scan 3162

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	25.2	53840	PASS
75	95	30	66	57.2	122251	PASS
95	95	100	100	100.0	213589	PASS
96	95	5	9	6.4	13653	PASS
173	174	0.00	2	1.0	1322	PASS
174	95	50	120	64.8	138379	PASS
175	174	4	9	6.9	9520	PASS
176	174	93	101	94.0	130096	PASS
177	176	5	9	6.8	8909	PASS

Average of 10.364 to 10.371 min.: VL042823.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.15	1010	46.00	282	53.60	93	64.00	681
36.10	1971	46.30	186	54.10	59	65.05	166
37.05	13479	46.95	2475	55.00	547	65.95	121
38.05	12024	47.95	1241	56.05	3667	66.10	40
39.10	5775	48.20	546	57.05	7472	66.30	47
40.10	507	49.05	11198	57.95	583	66.95	362
40.80	23	50.05	53840	58.50	59	68.05	25928
42.20	17	51.10	16524	60.05	2684	69.10	25432
43.20	42	52.00	575	61.10	11377	70.05	2568
44.10	1496	52.90	126	62.10	11618	71.10	77
45.05	2118	53.20	60	63.10	9557	72.10	1557

Average of 10.364 to 10.371 min.: VL042823.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.10	10163	83.20	226	96.10	13653	109.50	33
74.05	41195	85.70	41	97.00	136	109.70	30
75.10	122251	85.90	140	97.15	301	110.70	135
76.10	9723	86.20	21	102.80	26	111.10	165
77.05	1267	87.00	6738	103.20	63	112.00	106
77.90	643	88.00	6381	103.95	923	113.05	187
79.00	6692	90.90	828	105.00	481	114.75	246
79.95	1812	92.10	6549	106.00	925	115.00	64
81.00	6351	93.10	9478	106.95	297	115.95	1084
81.90	1233	94.10	27136	107.95	74	117.00	1328
82.85	117	95.10	213589	109.20	29	117.80	149

Average of 10.364 to 10.371 min.: VL042823.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.05	663	129.15	270	139.10	59	147.60	54
119.05	1257	129.95	732	139.70	57	148.05	394
121.60	26	130.20	122	139.95	225	148.80	116
122.50	29	130.85	155	140.95	2184	148.95	167
123.90	165	131.20	75	142.05	391	149.95	229
124.75	77	132.40	26	143.05	2493	151.10	18
125.85	98	134.15	60	143.85	214	151.60	50
126.70	64	134.95	390	144.60	113	151.90	69
127.10	32	137.10	482	144.90	359	152.85	222
127.80	430	138.00	35	146.00	297	153.75	70
128.00	324	138.85	124	146.90	241	154.10	33

Average of 10.364 to 10.371 min.: VL042823.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.05	545	167.90	28	176.05	130096	245.90	29
155.80	65	168.20	24	177.10	8909	257.60	67
156.80	114	168.80	17	178.00	168	260.40	18
157.00	311	169.35	90	178.40	21	261.50	47
157.50	21	170.00	203	182.40	20	262.80	43
158.95	357	170.75	108	185.20	67	274.70	28
159.90	18	172.00	1054	200.40	17	281.30	20
160.95	241	172.20	332	201.10	29	282.30	19
163.50	45	173.05	1322	220.60	23	295.30	24
167.40	35	174.05	138379	221.35	78	296.20	36
167.70	91	175.05	9520	244.00	48		