
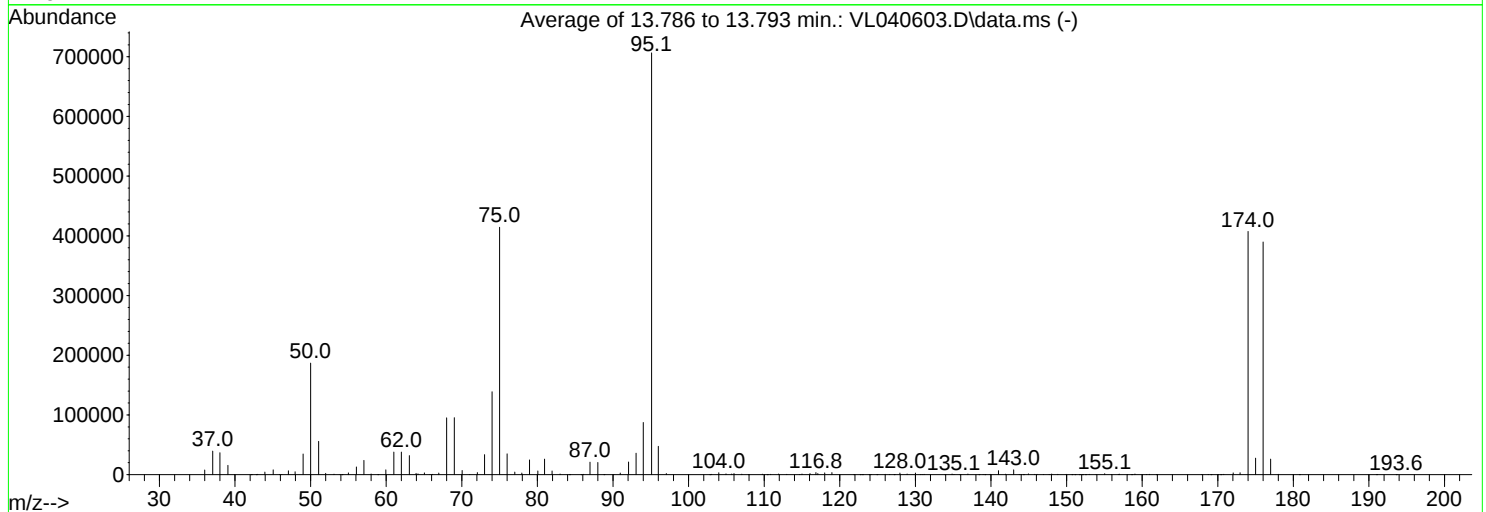


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL080923\
 Data File : VL040603.D
 Acq On : 9 Aug 2023 12:59
 Operator : SY/MD
 Sample : bfb
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL071023AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Mon Jul 10 16:32:00 2023

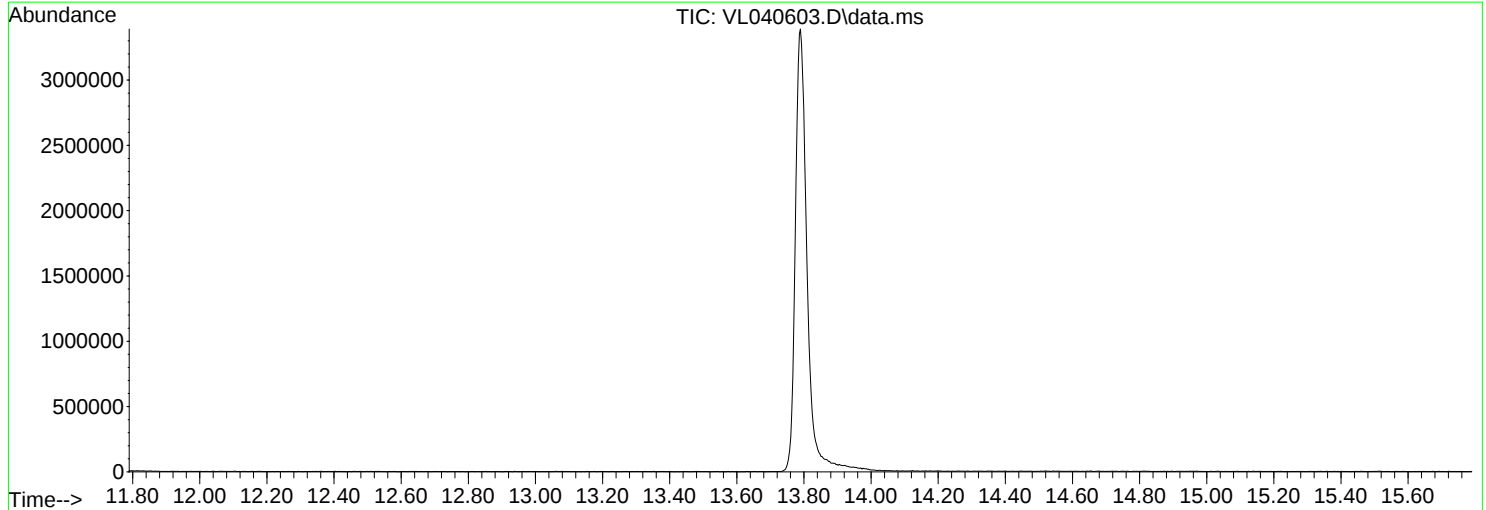

AutoFind: Scans 3478, 3479, 3480; Background Corrected with Scan 3456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.4	186816	PASS
75	95	30	66	58.6	414379	PASS
95	95	100	100	100.0	706539	PASS
96	95	5	9	6.7	47403	PASS
173	174	0.00	2	0.8	3201	PASS
174	95	50	120	57.6	407296	PASS
175	174	4	9	6.8	27517	PASS
176	174	93	101	95.7	389696	PASS
177	176	5	9	6.7	26123	PASS

Average of 13.786 to 13.793 min.: VL040603.D\data.ms

bfb

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	7859	46.20	278	56.05	12946	65.80	361
37.05	39453	47.05	6369	57.05	23909	66.10	477
38.00	36712	47.95	4826	58.00	1213	66.95	261
39.05	15595	49.00	34595	58.90	55	68.00	9520
39.95	361	50.00	186816	59.95	8180	69.00	95528
42.15	131	51.05	55851	61.00	37752	70.05	7085
42.80	75	52.00	2287	62.00	37907	71.05	361
43.00	428	53.10	806	63.05	31883	72.05	3510
43.95	4272	53.90	222	63.95	2092	73.00	33619
45.05	8078	54.15	154	64.20	1265	74.00	138795
45.90	228	55.00	3094	65.05	2892	75.00	414379

Average of 13.786 to 13.793 min.: VL040603.D\data.ms

bfb

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.00	34920	86.95	21019	102.80	67	111.90	1015
77.00	4430	88.00	20312	103.05	417	113.00	657
77.95	2732	88.80	131	104.00	3225	114.70	357
78.95	24560	90.10	193	104.95	1222	115.00	1079
80.05	6229	90.95	2780	105.70	966	116.05	1851
80.95	26011	92.05	21235	106.00	2027	116.85	3488
81.95	6073	93.05	35816	107.05	906	117.10	1803
83.00	1174	94.00	87400	107.90	89	118.00	2941
84.25	145	95.10	706539	109.75	712	118.95	3470
85.80	106	96.00	47403	110.40	106	121.85	137
86.10	662	97.05	1997	110.85	509	122.70	55

Average of 13.786 to 13.793 min.: VL040603.D\data.ms

bfb

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
123.00	88	130.90	352	141.00	6593	148.05	1179
123.90	157	131.15	509	141.95	727	148.85	548
124.15	406	133.90	124	143.00	8178	149.95	527
124.90	133	134.85	1111	143.75	254	150.70	79
126.00	514	135.10	375	144.00	162	151.10	56
126.60	210	135.90	71	144.30	55	151.70	103
127.20	53	136.95	1046	144.95	1255	152.10	71
127.95	2807	138.40	71	145.80	577	152.50	136
128.90	1045	138.95	369	146.10	602	153.00	578
130.00	2633	139.20	158	146.95	257	153.90	406
130.70	243	139.90	549	147.70	352	155.05	1679

Average of 13.786 to 13.793 min.: VL040603.D\data.ms

bfb

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
155.95	284	169.10	78	180.80	90		
156.85	505	170.05	240	191.00	55		
157.00	778	170.40	149	193.60	56		
158.05	195	170.80	418				
158.60	145	172.05	2901				
159.05	965	172.95	3201				
160.60	232	174.00	407296				
160.95	674	175.00	27517				
161.90	85	176.00	389696				
167.90	283	177.00	26123				
168.75	165	178.00	638				

Instrument :

MSVOA_L

ClientSampleId :

BFB