


Data Path : Z:\VOASRV\HPCHEM1\MSVOA L\DATA\VL081121\
 Data File : VL037374.D
 Acq On : 11 Aug 2021 1:45
 Operator : SY/AP
 Sample : BFB
 Misc : 400mL/MSVOA L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_L\METHODS\VL081121AIR.M
 Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Wed Aug 11 09:01:07 2021
 Last Update : Wed Aug 11 09:01:07 2021

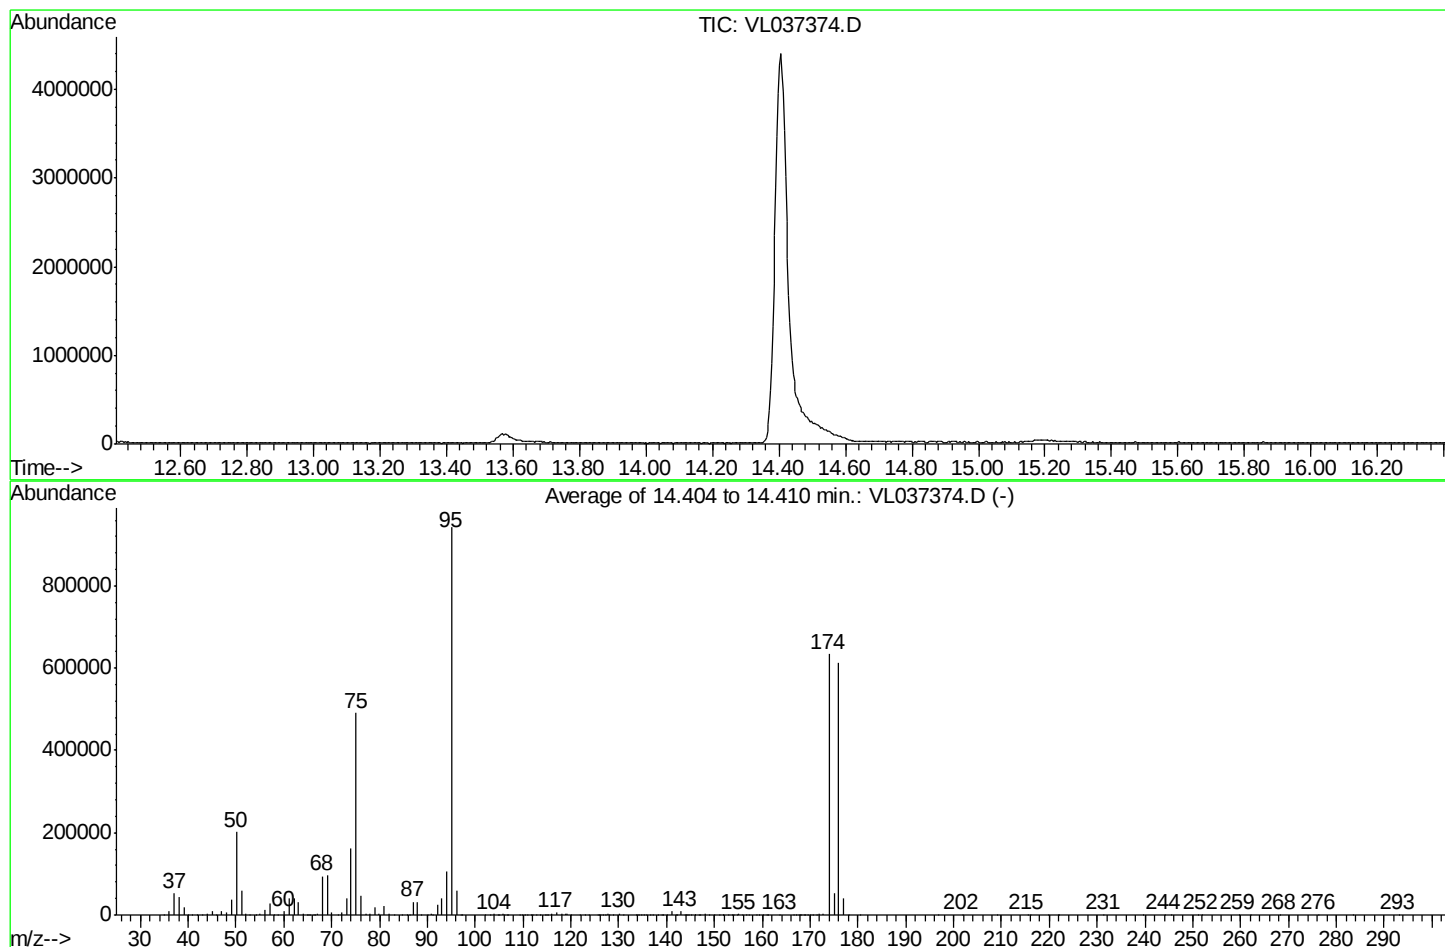

AutoFind: Scans 3613, 3614, 3615; Background Corrected with Scan 3588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	21.4	201514	PASS
75	95	30	66	52.0	490368	PASS
95	95	100	100	100.0	942420	PASS
96	95	5	9	6.3	59341	PASS
173	174	0.00	2	0.3	1872	PASS
174	95	50	120	67.2	633642	PASS
175	174	4	9	8.2	51810	PASS
176	174	93	101	96.6	611861	PASS
177	176	5	9	6.6	40256	PASS